
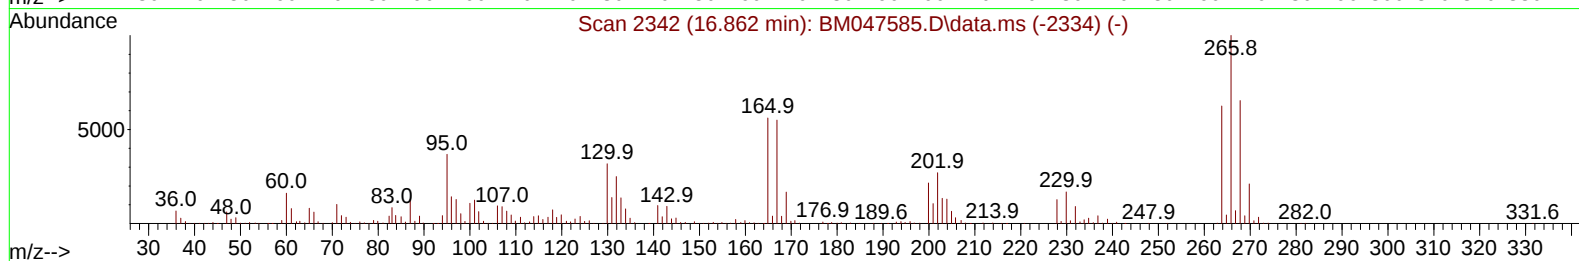
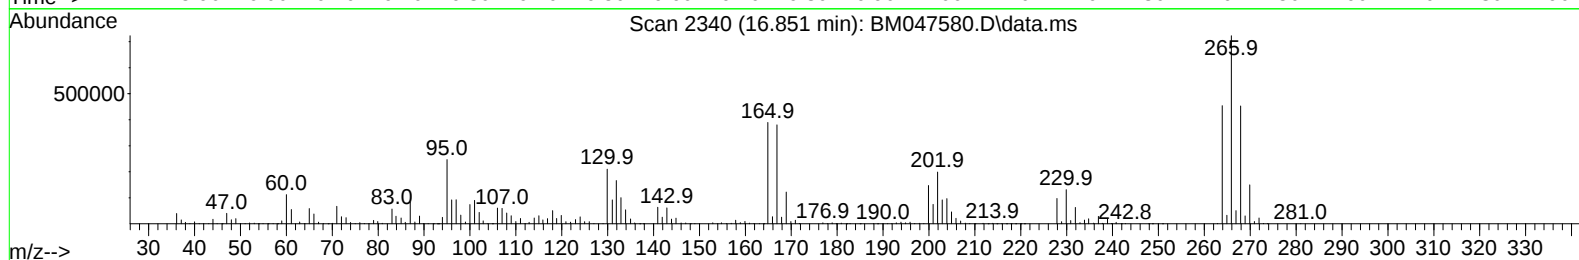


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047580.D
Acq On : 20 Sep 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 16:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:46:17 2024
Response via : Initial Calibration

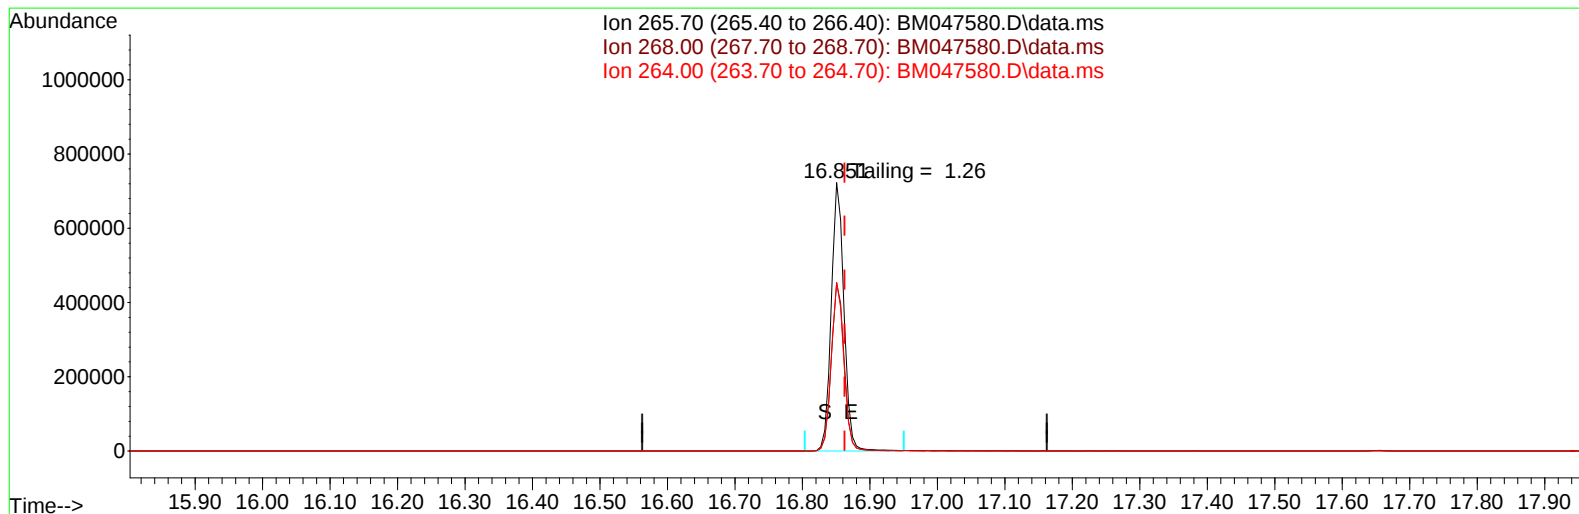

TIC: BM047580.D\data.ms

(70) Pentachlorophenol (C)




16.851min (-0.012) 2244989.51 ng

response 942708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.63
264.00	62.50	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047580.D
Acq On : 20 Sep 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 16:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:46:17 2024
Response via : Initial Calibration

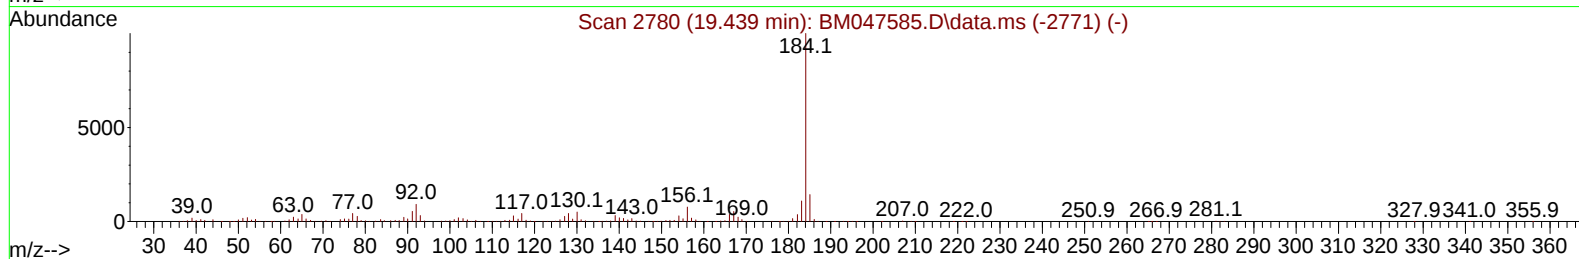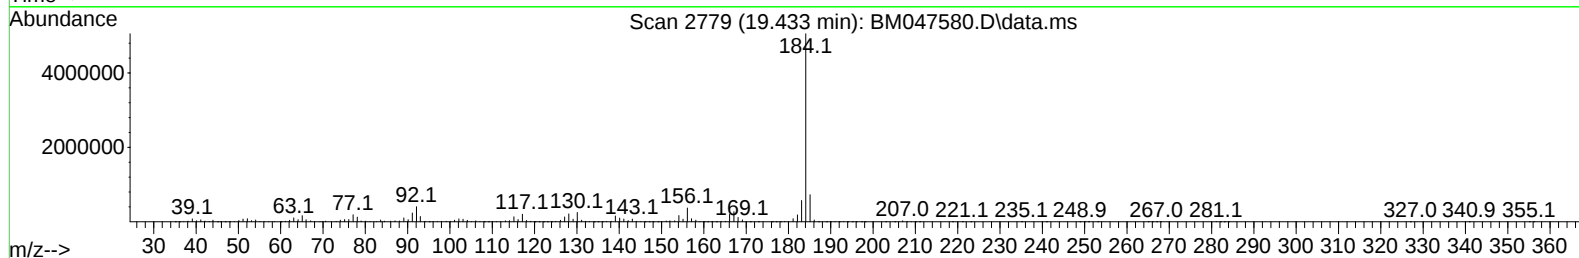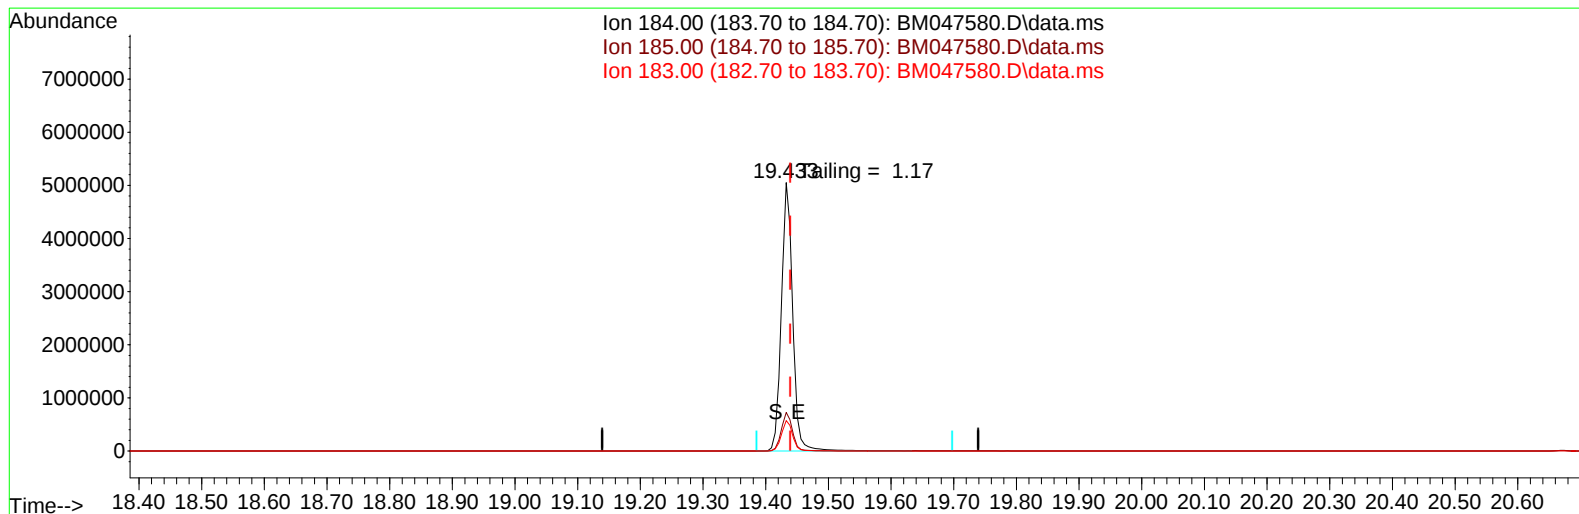

TIC: BM047580.D\data.ms

(77) Benzidine**19.433min (-0.006) 440805.88 ng****response 6381298**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.41
183.00	10.90	11.35
0.00	0.00	0.00