
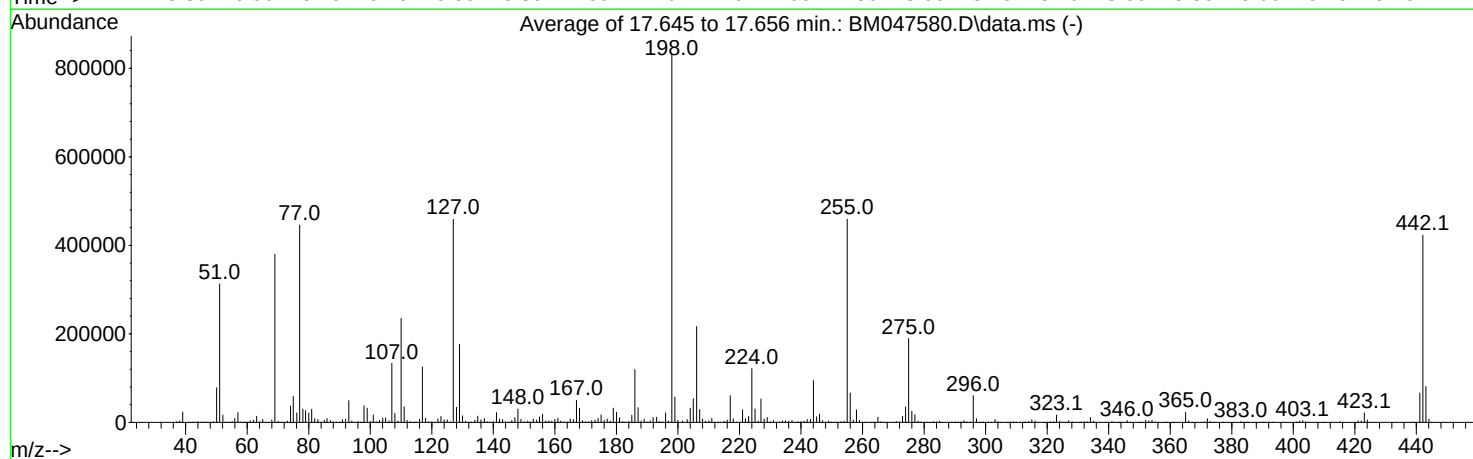


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047580.D
Acq On : 20 Sep 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 21 02:22:39 2024

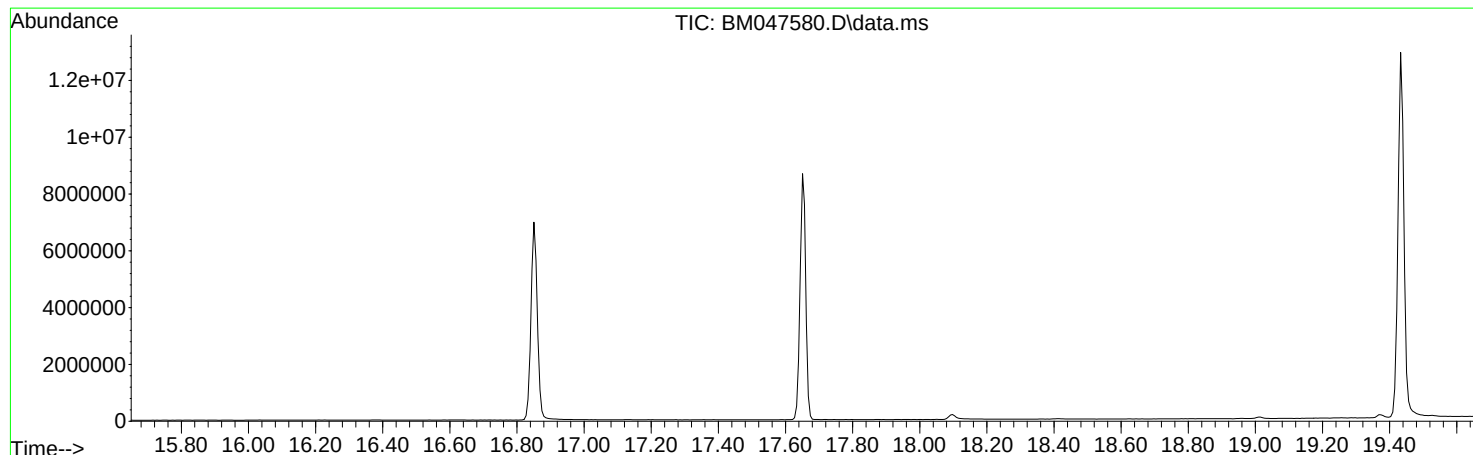

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	313211	PASS
68	69	0.00	2	1.5	5601	PASS
69	198	0.00	100	45.7	379786	PASS
70	69	0.00	2	0.6	2175	PASS
127	198	10	80	55.2	458880	PASS
197	198	0.00	2	0.4	3375	PASS
198	198	100	100	100.0	831296	PASS
199	198	5	9	6.9	57157	PASS
275	198	10	60	22.8	189387	PASS
365	198	1	100	2.7	22447	PASS
441	198	0.01	100	8.0	66259	PASS
442	442	50	100	100.0	423211	PASS
443	442	15	24	19.1	80891	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/20/2024	BNA_M	<u>BM047580.D</u>
Compound Name	Response	Retention Time
DDT	2641448	20.668
DDD	31829	20.286
DDE	907	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32736	2674184	1.22

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047580.D
Acq On : 20 Sep 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 20 16:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:46:17 2024
Response via : Initial Calibration

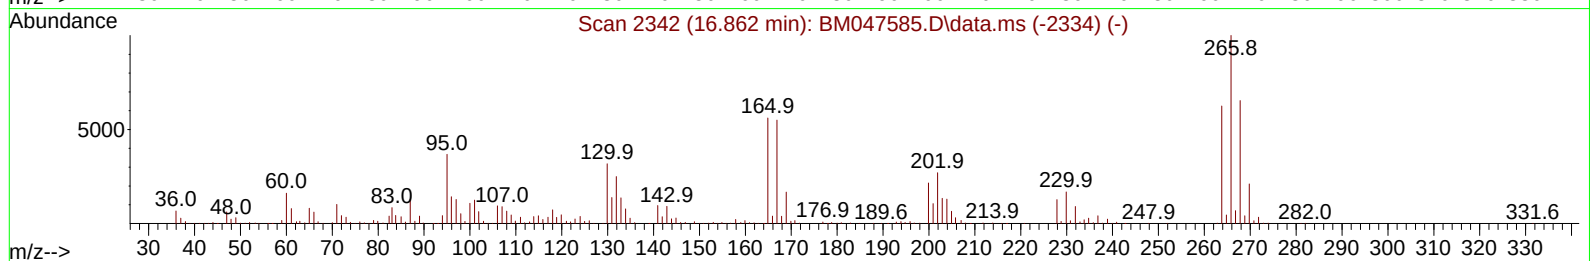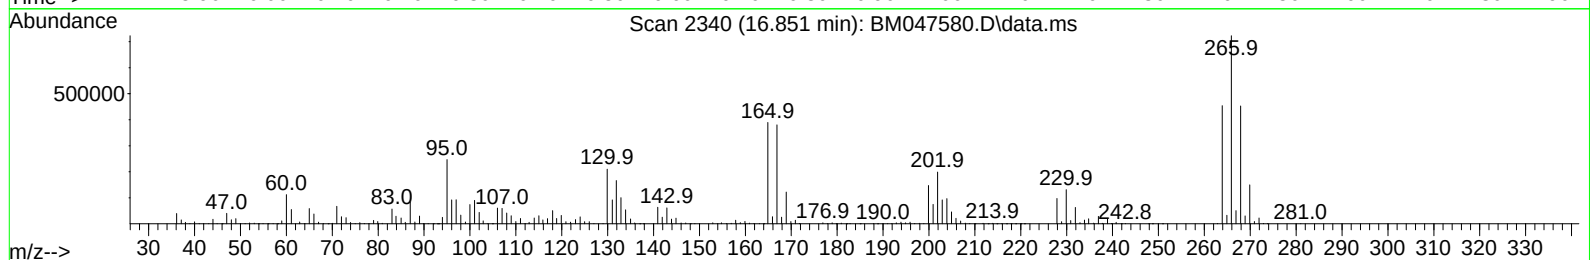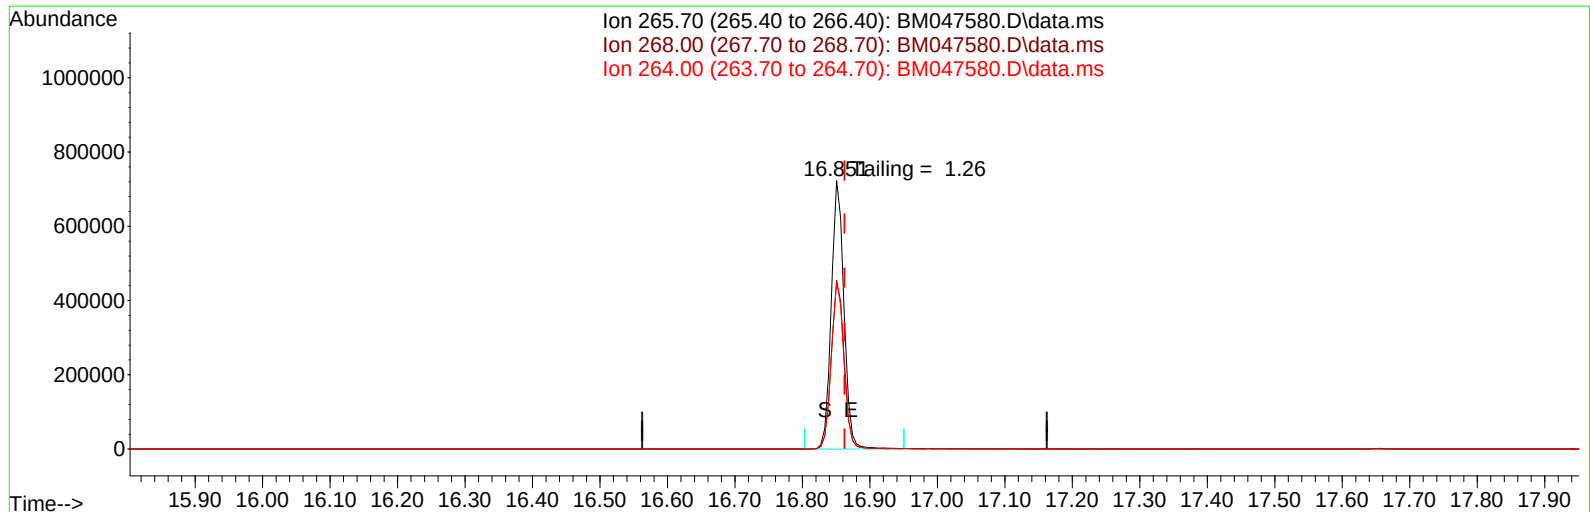

TIC: BM047580.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.012) 2244989.51 ng




response 942708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	62.63
264.00	62.50	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092024\
Data File : BM047580.D
Acq On : 20 Sep 2024 08:49
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Sep 20 16:46:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM092024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 16:46:17 2024
Response via : Initial Calibration

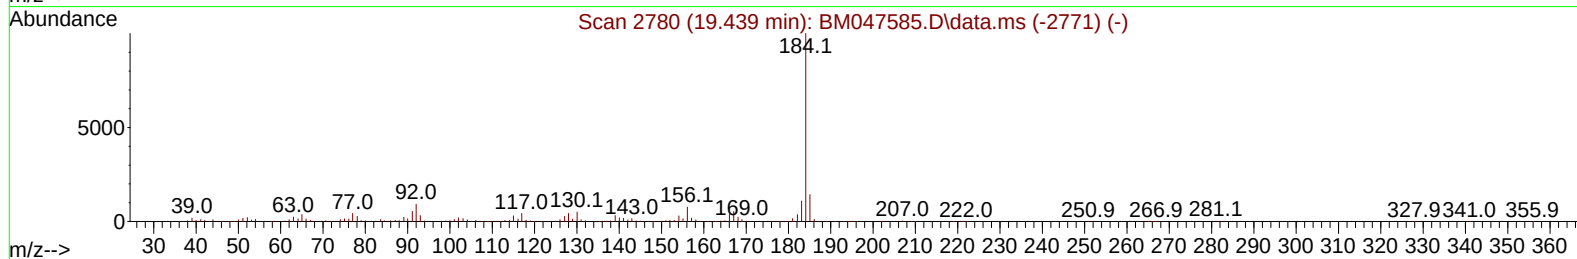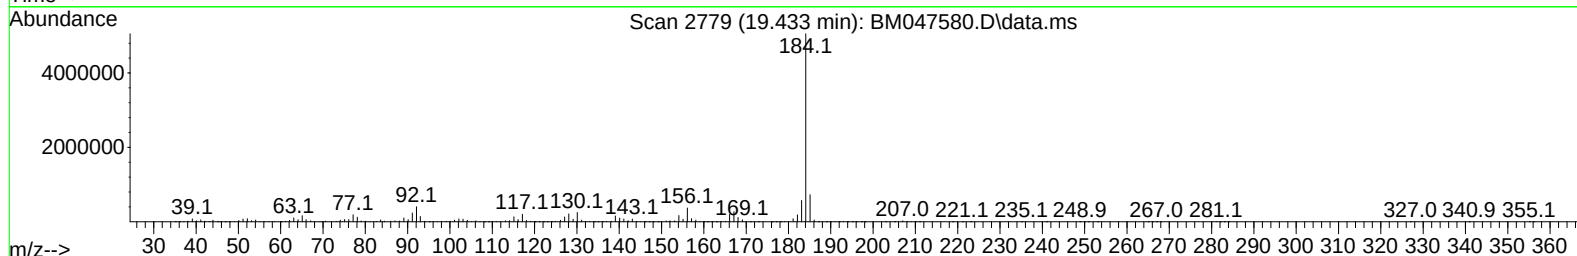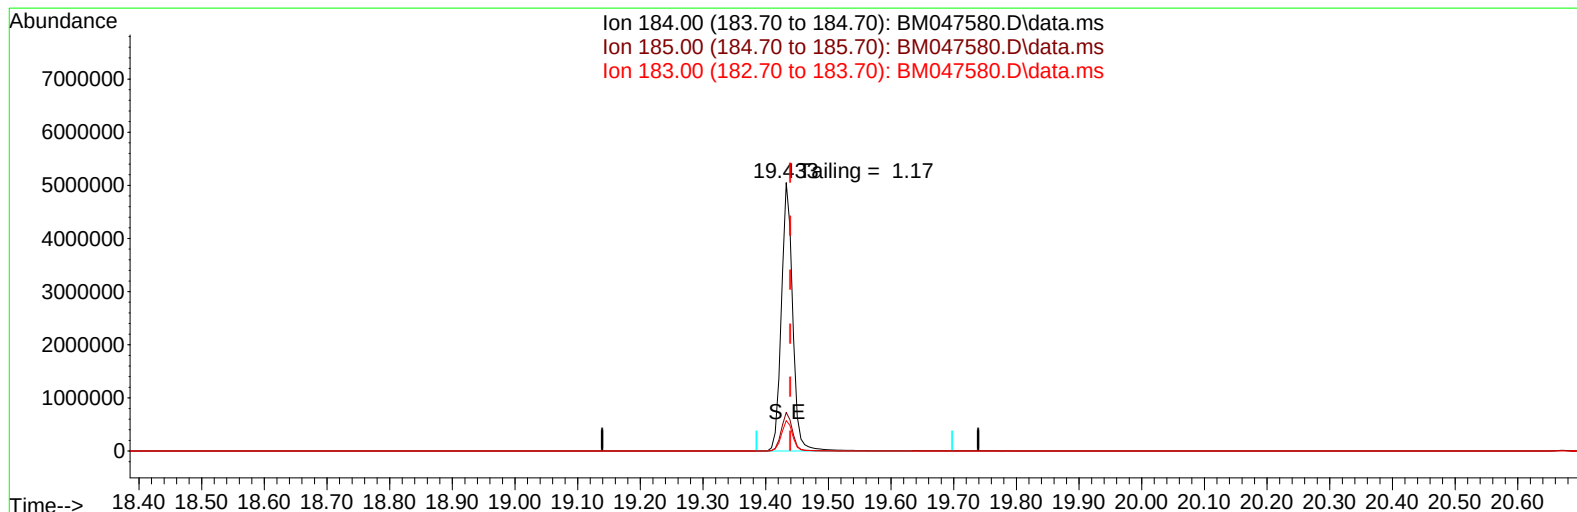

TIC: BM047580.D\data.ms

(77) Benzidine

19.433min (-0.006) 440805.88 ng

response 6381298

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.41
183.00	10.90	11.35
0.00	0.00	0.00