

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036655.D
 Acq On : 22 Sep 2022 10:24
 Operator : CG/JU
 Sample : N4649-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ38

Quant Time: Sep 23 00:58:46 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	390923	20.000	ng/u1	0.00
20) Naphthalene-d8	10.833	136	1800731	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1169076	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2323889	20.000	ng/u1	0.00
79) Chrysene-d12	21.544	240	1698545	20.000	ng/u1	0.00
88) Perylene-d12	23.991	264	1455197	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	36015	3.454	ng/uL	0.00
4) Pyridine-d5	3.822	84	244182	8.029	ng/u1	0.00
7) Phenol-d5	7.175	99	196045	5.612	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.345	67	585125	27.580	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	571587	22.726	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	385484	14.934	ng/u1	0.00
21) Nitrobenzene-d5	9.186	128	393232	32.263	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	372251	34.097	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	663885	26.240	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1009334	23.994	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2603769	33.023	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	2938459	31.418	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	68450	4.476	ng/u1	0.00
60) Fluorene-d10	15.633	176	2362345	33.433	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	249596	27.147	ng/u1	0.00
73) Anthracene-d10	17.480	188	3743631	35.233	ng/u1	0.00
81) Pyrene-d10	19.762	212	3886694	46.513	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	2655605	37.353	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	27617	2.458	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036655.D
Acq On : 22 Sep 2022 10:24
Operator : CG/JU
Sample : N4649-10
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ38

Quant Time: Sep 23 00:58:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

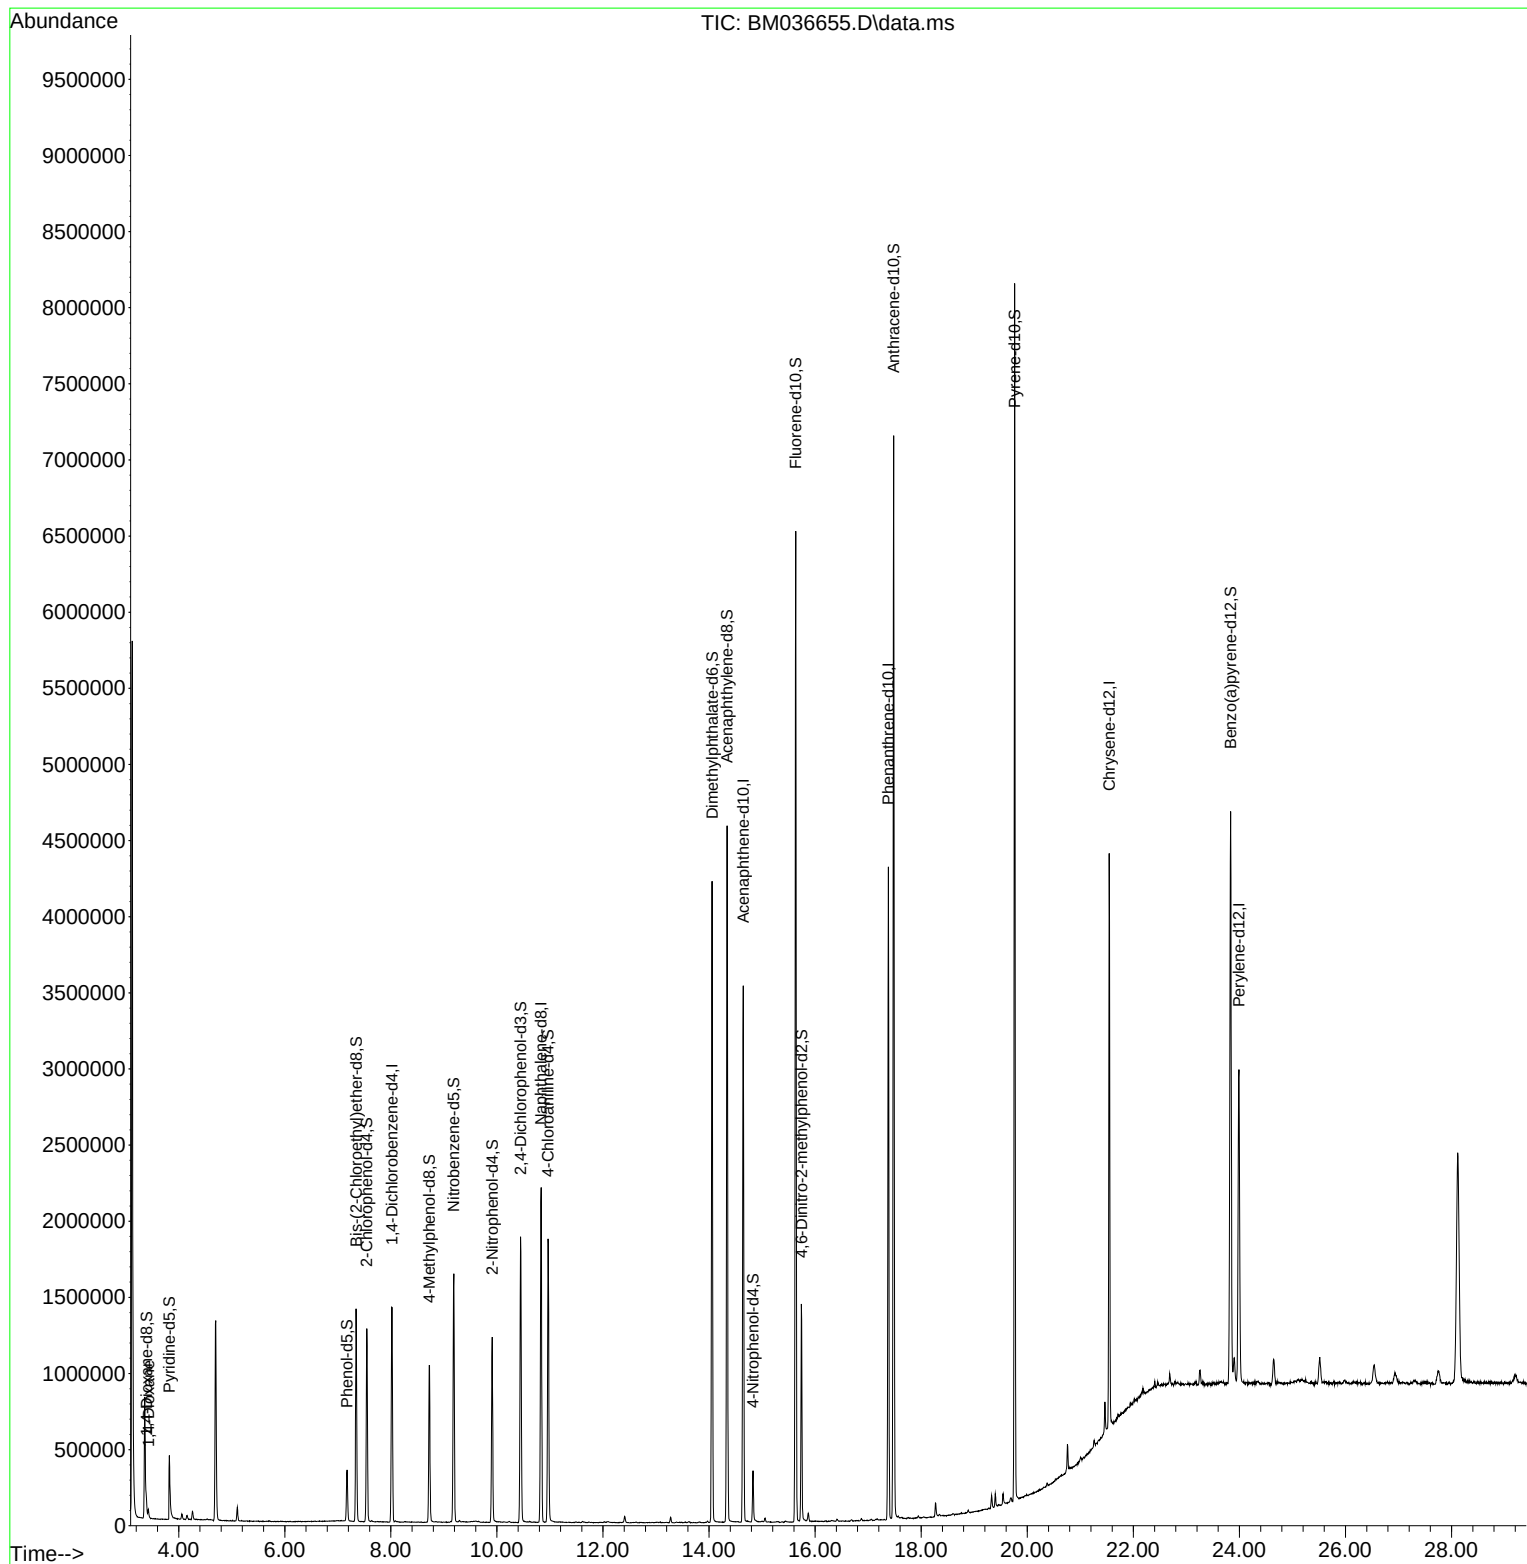

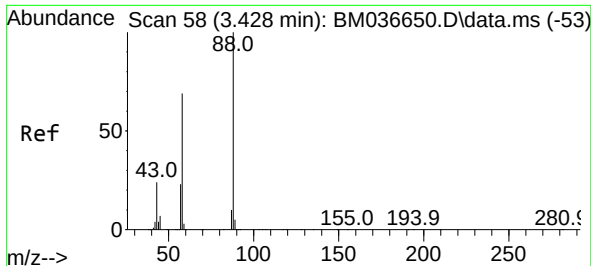

#2
 1,4-Dioxane
 Concen: 2.458 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM036655.D
 Acq: 22 Sep 2022 10:24

Instrument :
 BNA_M
 ClientSampleId :
 EXZ38

Tgt Ion	Ratio	Lower	Upper
88	100		
43	25.5	23.1	34.7
58	62.0	56.6	85.0

