

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036664.D
 Acq On : 22 Sep 2022 15:58
 Operator : CG/JU
 Sample : N4595-04DL 5X
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8G9DL

Quant Time: Sep 23 01:02:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	243986	20.000	ng/u1	0.00
20) Naphthalene-d8	10.833	136	1044698	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	606064	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	1135490	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	787267	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	709169	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	5168	0.794	ng/uL	0.00
4) Pyridine-d5	3.834	84	44271	2.332	ng/u1	0.02
7) Phenol-d5	7.175	99	53305	2.445	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.345	67	154880	11.697	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	151861	9.674	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	98329	6.103	ng/u1	0.00
21) Nitrobenzene-d5	9.187	128	92838	13.129	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	79938	12.621	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	160554	10.938	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	126780	5.195	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	545054	13.334	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	620174	12.791	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	14006	1.767	ng/u1	0.00
60) Fluorene-d10	15.633	176	476801	13.016	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	39906	8.883	ng/u1	0.00
73) Anthracene-d10	17.480	188	660632	12.725	ng/u1	0.00
81) Pyrene-d10	19.762	212	673663	17.394	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	463333	13.373	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.428	88	359042	51.211	ng/uL	96
86) Bis(2-ethylhexyl)phtha...	21.462	149	50746	1.825	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036664.D
Acq On : 22 Sep 2022 15:58
Operator : CG/JU
Sample : N4595-04DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G9DL

Quant Time: Sep 23 01:02:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration




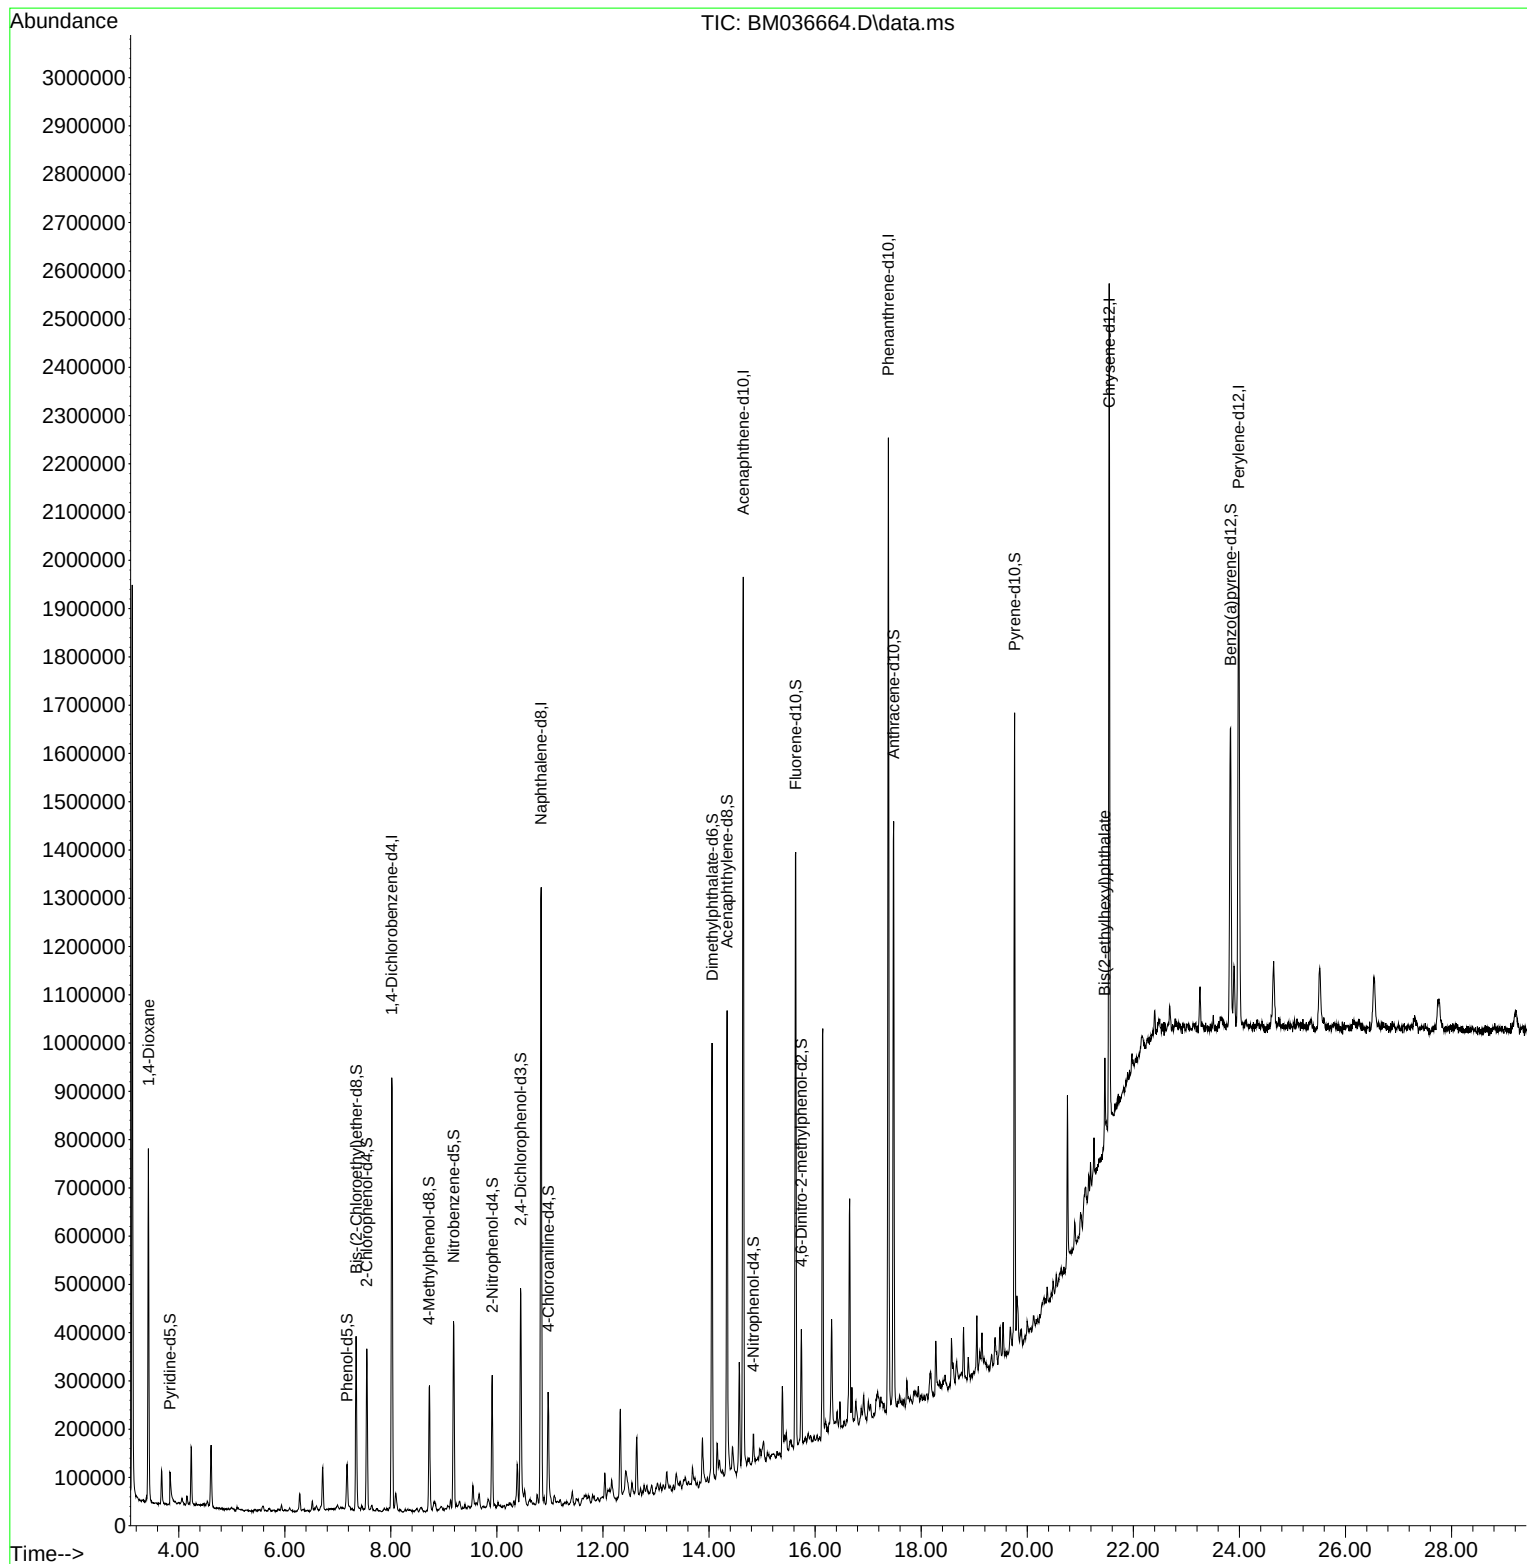


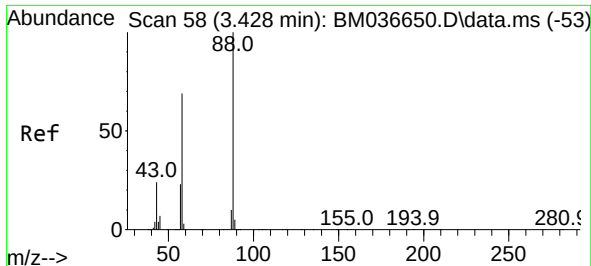

#2
 1,4-Dioxane
 Concen: 51.211 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM036664.D
 Acq: 22 Sep 2022 15:58

Instrument :
 BNA_M
 ClientSampleId :
 CB8G9DL

Tgt Ion: 88 Resp: 359042
 Ion Ratio Lower Upper
 88 100
 43 24.7 23.1 34.7
 58 68.4 56.6 85.0

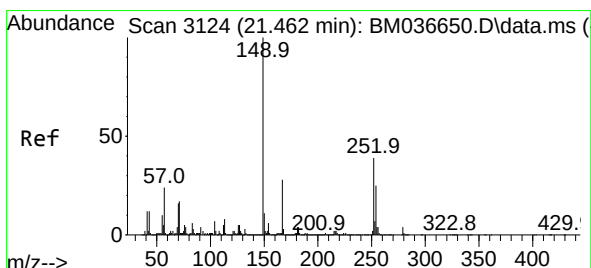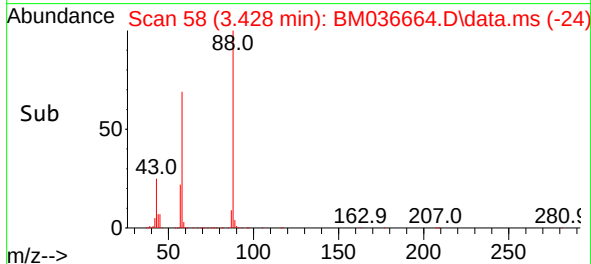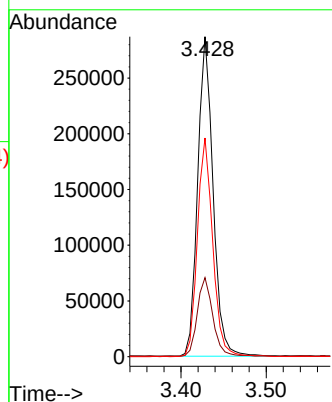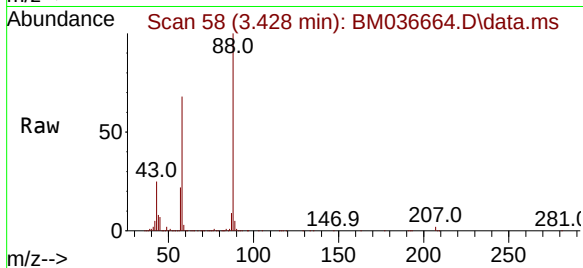

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.825 ng/uL
 RT: 21.462 min Scan# 3124
 Delta R.T. -0.006 min
 Lab File: BM036664.D
 Acq: 22 Sep 2022 15:58

Tgt Ion: 149 Resp: 50746
 Ion Ratio Lower Upper
 149 100
 167 26.9 22.0 33.0
 279 3.7 3.3 4.9

