




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036639.D
 Acq On : 22 Sep 2022 00:11
 Operator : CG/JU
 Sample : N4605-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5747

Manual IntegrationsAPPROVED

Quant Time: Sep 22 01:05:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/22/2022
 Supervised By :mohammad ahmed 09/23/2022

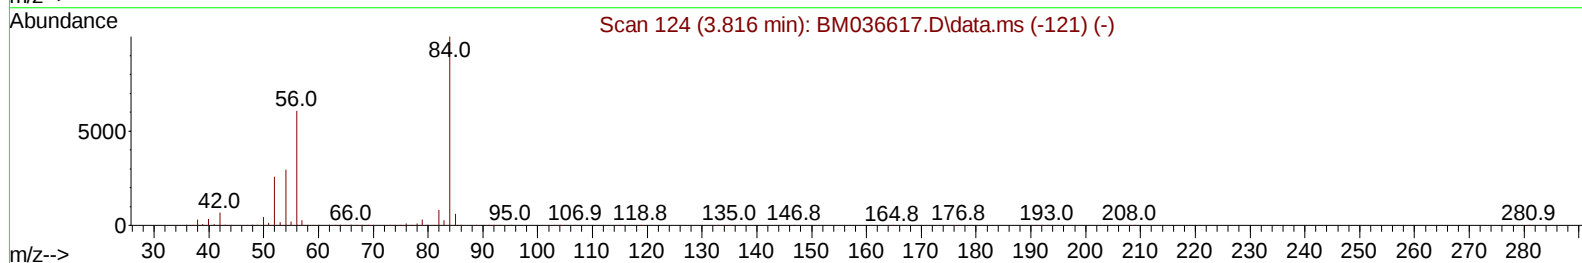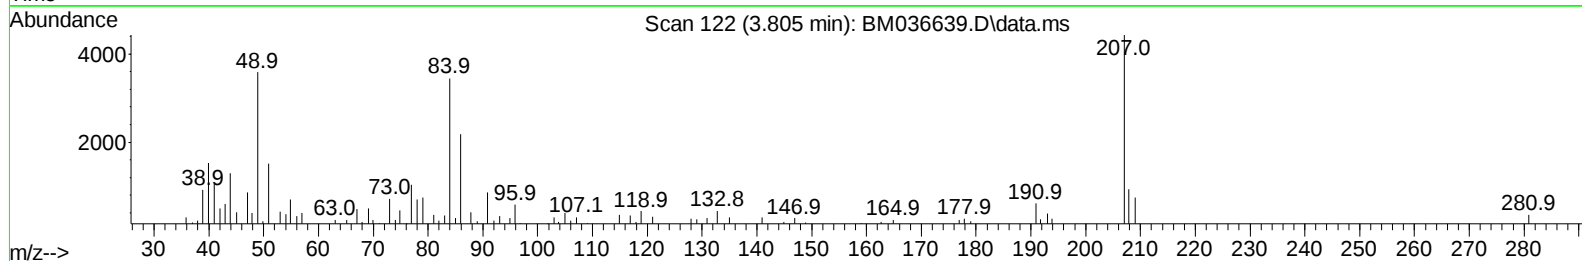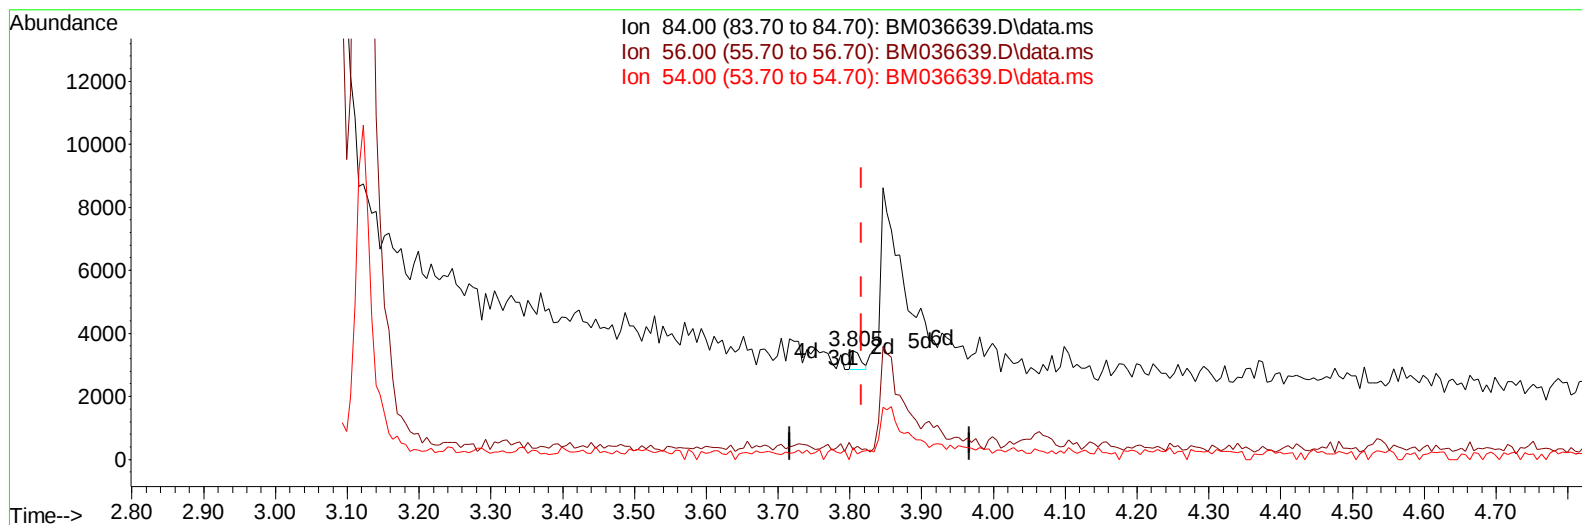

TIC: BM036639.D\data.ms

(4) Pyridine-d5 (S)

3.805min (-0.012) 0.02 ng/u1

response 525

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.90	9.39#
54.00	30.90	10.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036639.D
 Acq On : 22 Sep 2022 00:11
 Operator : CG/JU
 Sample : N4605-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5747

Manual IntegrationsAPPROVED

Quant Time: Sep 22 01:05:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/22/2022
 Supervised By :mohammad ahmed 09/23/2022

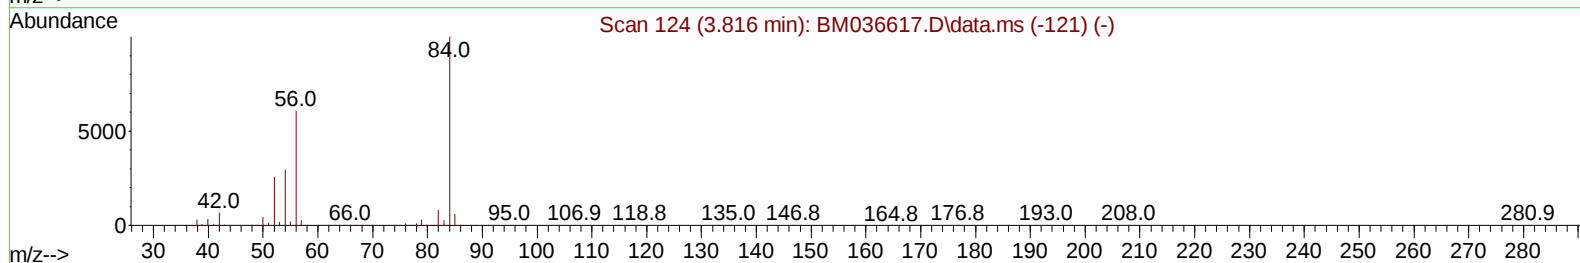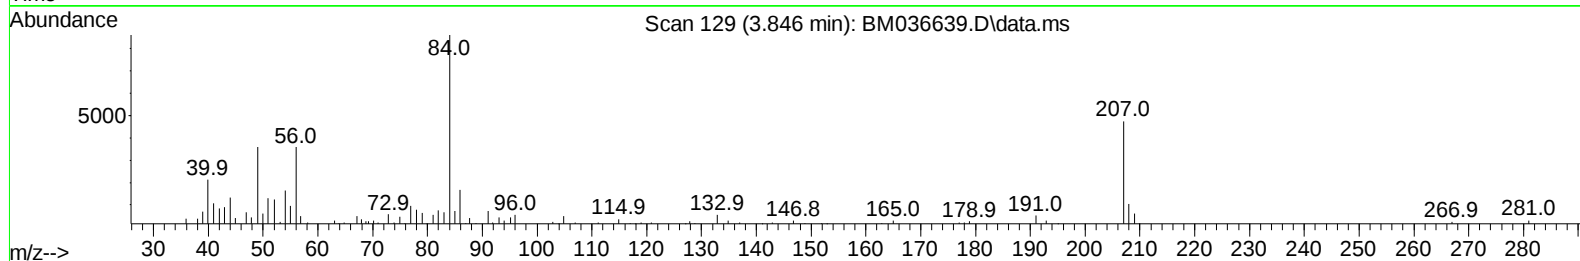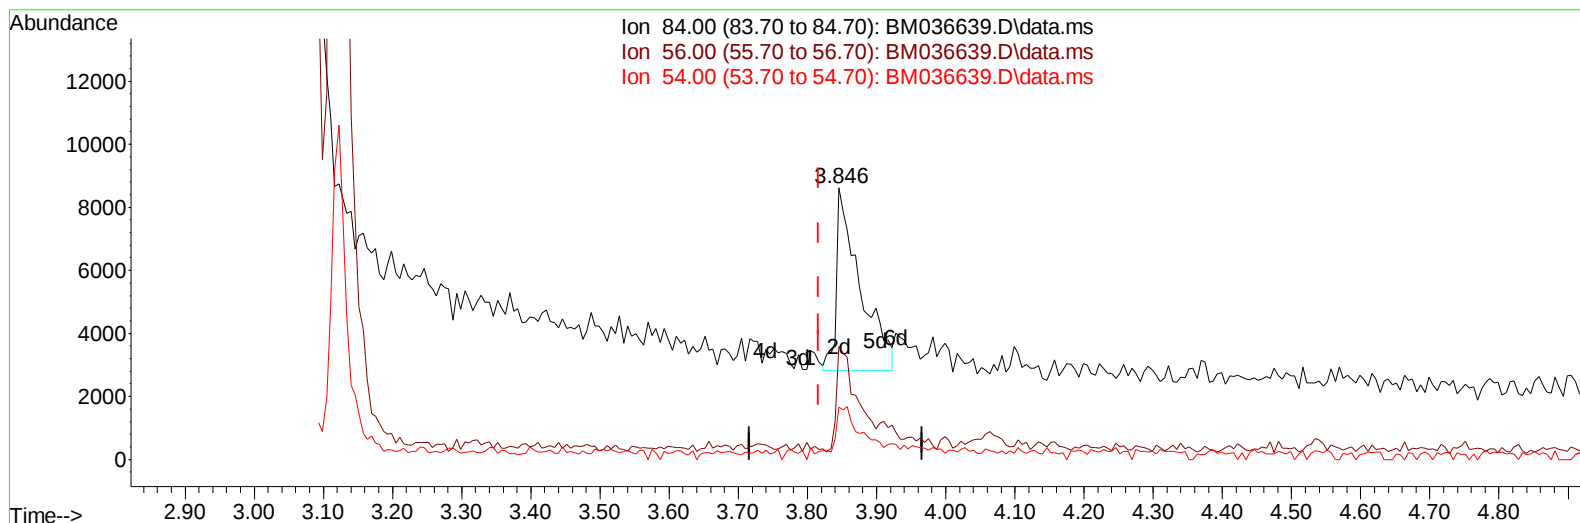

TIC: BM036639.D\data.ms

(4) Pyridine-d5 (S)

3.846min (+ 0.029) 0.57 ng/u1 m

response 13772

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	61.90	41.68#
54.00	30.90	19.19#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036639.D
 Acq On : 22 Sep 2022 00:11
 Operator : CG/JU
 Sample : N4605-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5747

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/22/2022
 Supervised By :mohammad ahmed 09/23/2022

Quant Time: Sep 22 01:05:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	308542	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	1397330	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	923877	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.380	188	1928819	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1849397	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	1868008	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	22151	2.691	ng/uL	0.00
4) Pyridine-d5	3.846	84	13772m	0.574	ng/ul	0.03
7) Phenol-d5	7.175	99	462253	16.765	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.346	67	279251	16.677	ng/ul	0.00
11) 2-Chlorophenol-d4	7.551	132	374240	18.852	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	389460	19.116	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	189721	20.060	ng/ul	0.00
24) 2-Nitrophenol-d4	9.910	143	191398	22.593	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	362157	18.446	ng/ul	0.00
31) 4-Chloroaniline-d4	10.969	131	339961	10.415	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	1281756	20.570	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	1457404	19.718	ng/ul	0.00
54) 4-Nitrophenol-d4	14.827	143	206851	17.115	ng/ul	0.00
60) Fluorene-d10	15.633	176	1142257	20.456	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	131119	17.182	ng/ul	0.00
73) Anthracene-d10	17.480	188	1807792	20.499	ng/ul	0.00
81) Pyrene-d10	19.762	212	2156745	23.705	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	2057051	22.540	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036639.D
Acq On : 22 Sep 2022 00:11
Operator : CG/JU
Sample : N4605-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A5747

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/22/2022
Supervised By :mohammad ahmed 09/23/2022

Quant Time: Sep 22 01:05:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

