

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036624.D
 Acq On : 21 Sep 2022 14:35
 Operator : CG/JU
 Sample : N4595-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8G7

Quant Time: Sep 21 22:49:21 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.022	152	475829	20.000	ng/u1	0.00
20) Naphthalene-d8	10.833	136	2170932	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1419412	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2924422	20.000	ng/u1	0.00
79) Chrysene-d12	21.550	240	2507241	20.000	ng/u1	0.00
88) Perylene-d12	23.991	264	2120373	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	44239	3.485	ng/uL	0.00
4) Pyridine-d5	3.822	84	171411	4.630	ng/u1	0.00
7) Phenol-d5	7.175	99	196946	4.632	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.351	67	560449	21.703	ng/u1	0.00
11) 2-Chlorophenol-d4	7.551	132	531658	17.366	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	381058	12.128	ng/u1	0.00
21) Nitrobenzene-d5	9.186	128	379268	25.811	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	329792	25.057	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.451	165	643894	21.110	ng/u1	0.00
31) 4-Chloroaniline-d4	10.969	131	530100	10.453	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2492850	26.040	ng/u1	0.00
49) Acenaphthylene-d8	14.345	160	2850531	25.103	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	78892	4.249	ng/u1	0.00
60) Fluorene-d10	15.633	176	2169564	25.289	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.745	200	267424	23.113	ng/u1	0.00
73) Anthracene-d10	17.480	188	3412664	25.522	ng/u1	0.00
81) Pyrene-d10	19.762	212	3796177	30.777	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.833	264	2792589	26.957	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.434	88	19644	1.437	ng/uL 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036624.D
Acq On : 21 Sep 2022 14:35
Operator : CG/JU
Sample : N4595-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G7

Quant Time: Sep 21 22:49:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

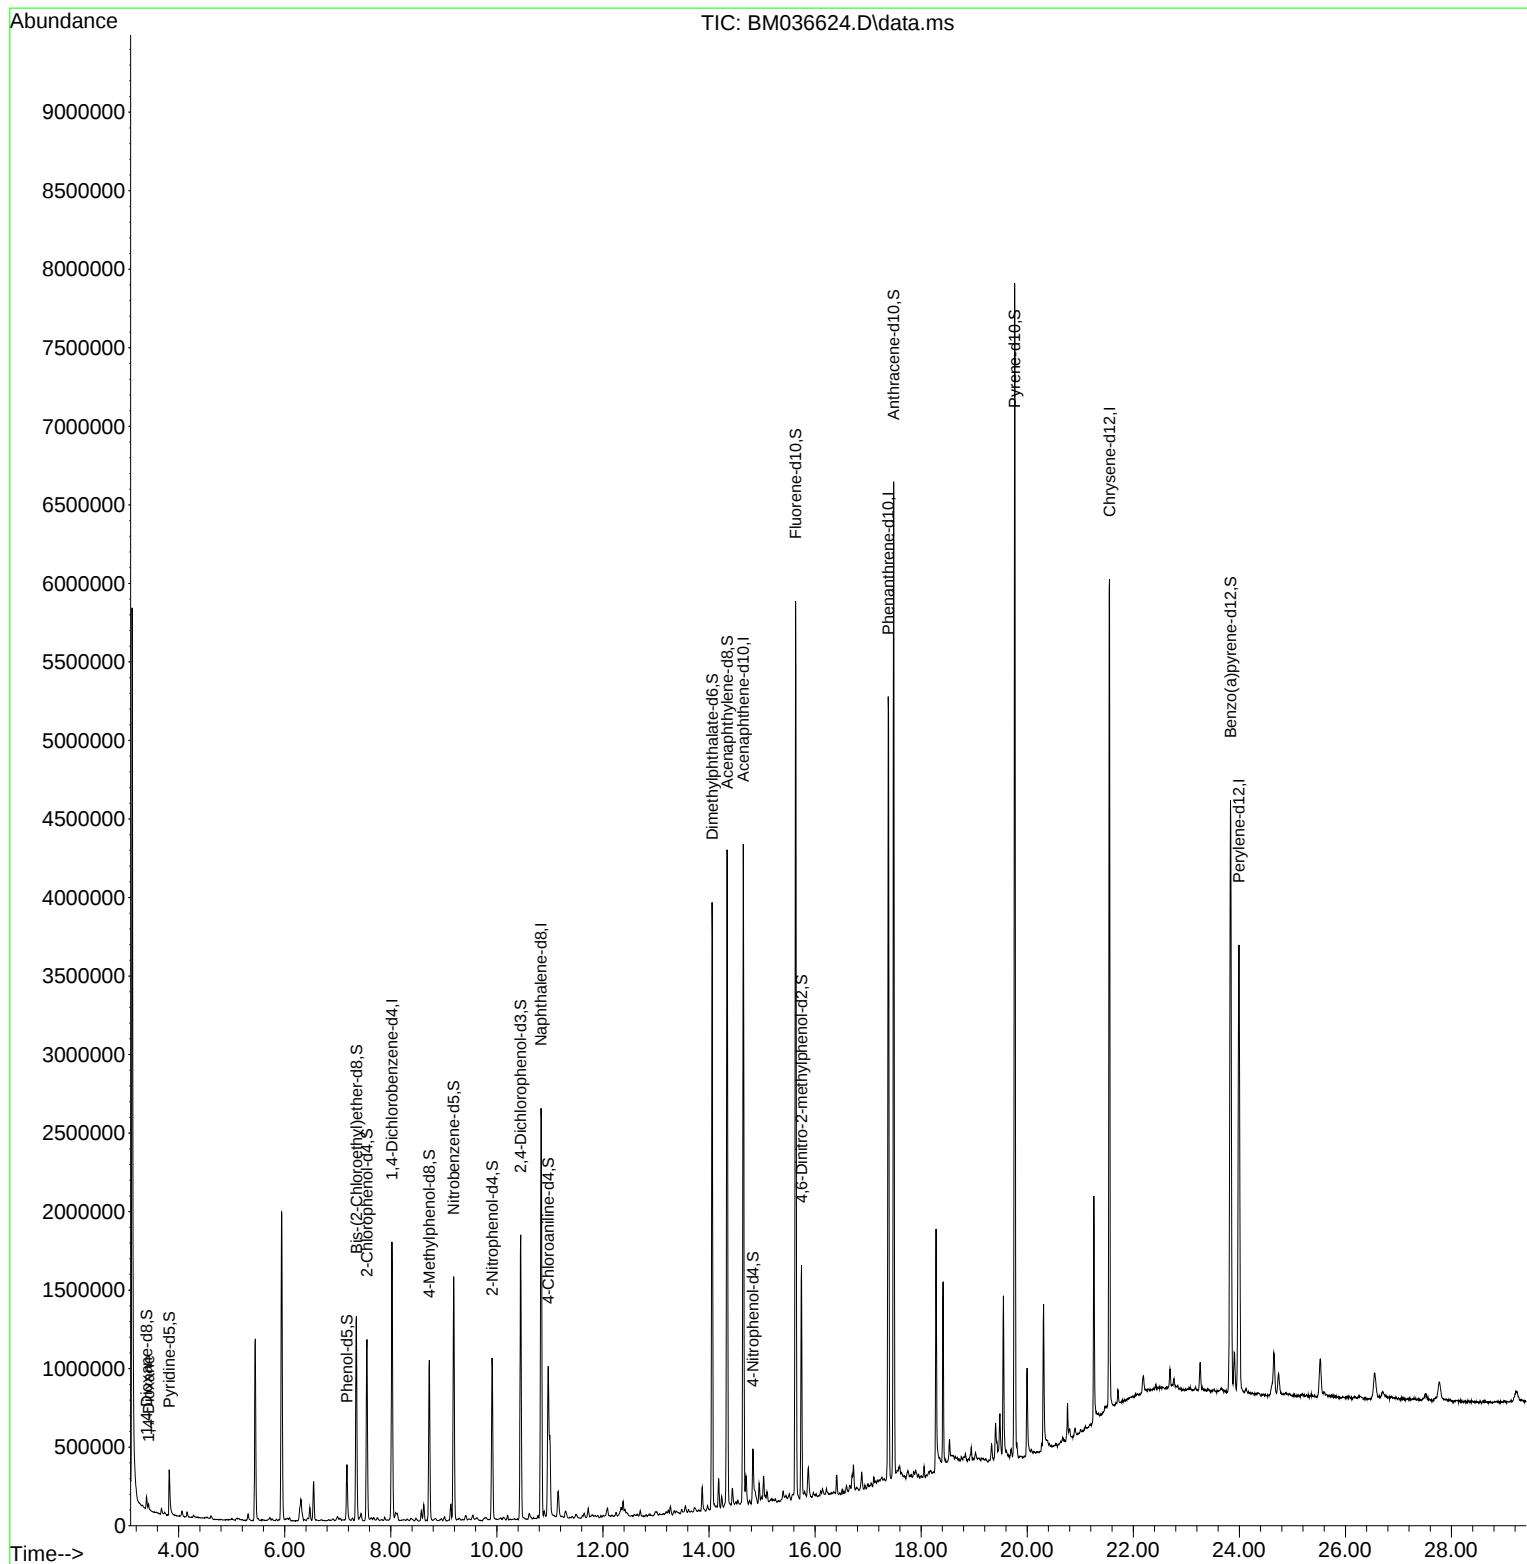

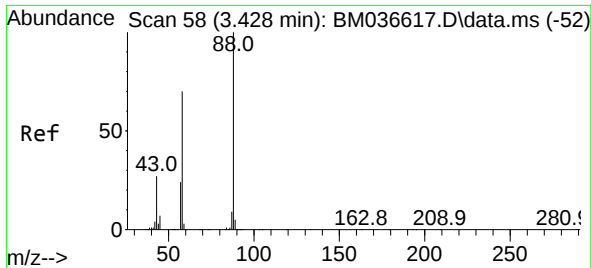

#2
 1,4-Dioxane
 Concen: 1.437 ng/uL
 RT: 3.434 min Scan# 59
 Delta R.T. 0.006 min
 Lab File: BM036624.D
 Acq: 21 Sep 2022 14:35

Instrument :
 BNA_M
 ClientSampleId :
 CB8G7

Tgt Ion: 88 Resp: 19644
 Ion Ratio Lower Upper
 88 100
 43 29.8 23.1 34.7
 58 60.4 56.6 85.0

