

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036649.D
 Acq On : 22 Sep 2022 06:09
 Operator : CG/JU
 Sample : N4649-09
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ37

Quant Time: Sep 22 06:44:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	404468	20.000	ng/u1	0.00
20) Naphthalene-d8	10.833	136	1819091	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.645	164	1153564	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2213470	20.000	ng/u1	0.00
79) Chrysene-d12	21.544	240	1533582	20.000	ng/u1	0.00
88) Perylene-d12	23.985	264	1370740	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	46566	4.316	ng/uL	0.00
4) Pyridine-d5	3.822	84	218672	6.949	ng/u1	0.00
7) Phenol-d5	7.175	99	220779	6.108	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.345	67	635232	28.939	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	638328	24.530	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	417364	15.627	ng/u1	0.00
21) Nitrobenzene-d5	9.186	128	423962	34.433	ng/u1	0.00
24) 2-Nitrophenol-d4	9.910	143	412005	37.358	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	718998	28.131	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	938021	22.074	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2502435	32.164	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	2933664	31.789	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	73471	4.869	ng/u1	0.00
60) Fluorene-d10	15.633	176	2248170	32.245	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	254253	29.033	ng/u1	0.00
73) Anthracene-d10	17.480	188	3588472	35.457	ng/u1	0.00
81) Pyrene-d10	19.762	212	3715155	49.242	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	2535184	37.856	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	11732	1.009	ng/uL	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036649.D
Acq On : 22 Sep 2022 06:09
Operator : CG/JU
Sample : N4649-09
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ37

Quant Time: Sep 22 06:44:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

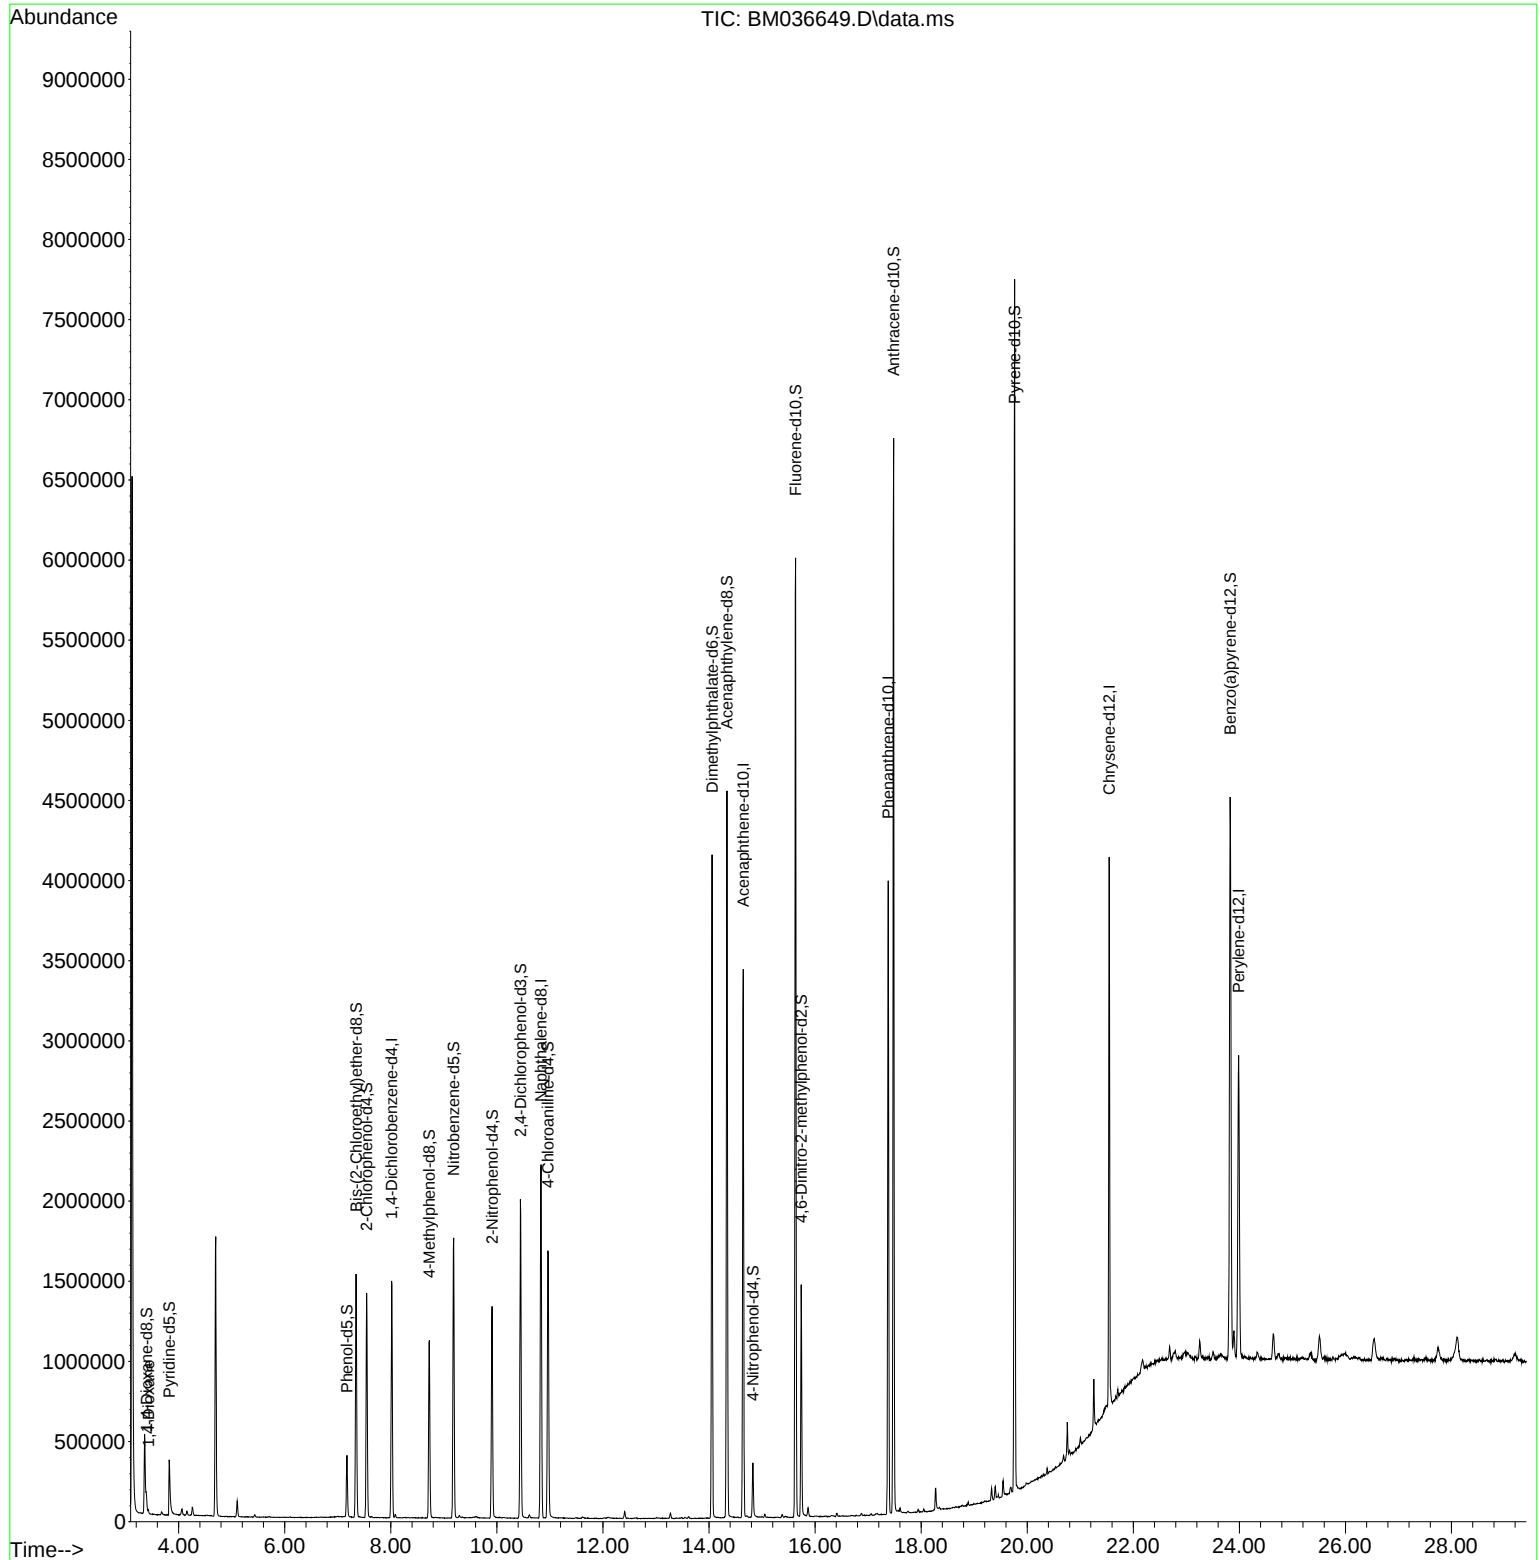

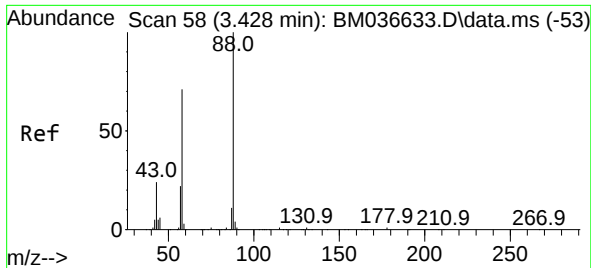

#2
 1,4-Dioxane
 Concen: 1.009 ng/uL
 RT: 3.428 min Scan# 58
 Delta R.T. -0.000 min
 Lab File: BM036649.D
 Acq: 22 Sep 2022 06:09

Instrument :
 BNA_M
 ClientSampleId :
 EXZ37

Tgt Ion: 88 Resp: 11732
 Ion Ratio Lower Upper
 88 100
 43 31.7 23.1 34.7
 58 59.6 56.6 85.0

