

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036618.D
 Acq On : 21 Sep 2022 11:00
 Operator : CG/JU
 Sample : PB147714BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK714

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	15	rVB	279348	385575	4.08%	0.405%
2	3.387	47	51	60	rVB	96726	133121	1.41%	0.140%
3	3.816	120	124	140	rBV	780632	1276397	13.50%	1.342%
4	4.157	177	182	186	rBV	24231	35281	0.37%	0.037%
5	7.169	686	694	704	rBV	1609830	2503530	26.48%	2.632%
6	7.345	716	724	733	rBV	1339907	2093386	22.14%	2.201%
7	7.545	750	758	766	rBV	1648698	2550527	26.98%	2.681%
8	8.016	830	838	848	rBV	1292070	2020105	21.37%	2.124%
9	8.722	950	958	972	rBV	2077278	3270695	34.59%	3.438%
10	9.181	1028	1036	1048	rBV	1546326	2527489	26.73%	2.657%
11	9.910	1150	1160	1170	rBV	1148535	1941876	20.54%	2.041%
12	10.445	1241	1251	1260	rBV	1987751	3264099	34.52%	3.431%
13	10.833	1307	1317	1329	rBV	1900399	3173423	33.56%	3.336%
14	10.963	1331	1339	1356	rBV	1237762	2051454	21.70%	2.157%
15	12.016	1511	1518	1520	rBV8	7190	14738	0.16%	0.015%
16	12.410	1576	1585	1590	rBV2	41382	67400	0.71%	0.071%
17	14.057	1858	1865	1876	rBV	3660476	5002427	52.91%	5.259%
18	14.339	1905	1913	1926	rBV	4157131	6116708	64.70%	6.430%
19	14.645	1958	1965	1974	rBV	3062812	4388883	46.42%	4.614%
20	14.821	1989	1995	2007	rBV	1787769	2579042	27.28%	2.711%
21	15.045	2032	2033	2041	rVB7	7340	9985	0.11%	0.010%
22	15.439	2095	2100	2105	rBV7	8343	14501	0.15%	0.015%
23	15.633	2125	2133	2145	rBV	5595379	7730382	81.76%	8.127%
24	15.739	2145	2151	2166	rVV	1350402	1893901	20.03%	1.991%
25	15.868	2168	2173	2179	rVB	50341	81545	0.86%	0.086%
26	16.192	2221	2228	2234	rBV9	5658	10383	0.11%	0.011%
27	16.410	2261	2265	2269	rBV3	12372	16652	0.18%	0.018%
28	16.510	2278	2282	2289	rVB7	6490	10209	0.11%	0.011%
29	16.880	2339	2345	2349	rBV2	26107	37570	0.40%	0.039%
30	17.380	2423	2430	2439	rBV	3671419	5167848	54.66%	5.433%
31	17.480	2440	2447	2458	rBV	6290397	8573311	90.68%	9.013%
32	17.751	2490	2493	2497	rBV6	7238	12471	0.13%	0.013%
33	17.951	2523	2527	2531	rBV2	27445	34843	0.37%	0.037%
34	18.280	2579	2583	2585	rBV5	9219	12617	0.13%	0.013%
35	18.892	2684	2687	2692	rVB3	28930	36027	0.38%	0.038%
36	19.327	2757	2761	2766	rBV3	68987	103069	1.09%	0.108%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036618.D
Acq On : 21 Sep 2022 11:00
Operator : CG/JU
Sample : PB147714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK714

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	19.398	2769	2773	2781	rVV	69344	105168	1.11%	0.111%
38	19.762	2829	2835	2848	rBV	7164673	9454681	100.00%	9.939%
39	20.762	3001	3005	3010	rBV	317244	366999	3.88%	0.386%
40	21.550	3134	3139	3144	rBV	3776597	4863757	51.44%	5.113%
41	23.839	3521	3528	3536	rVB2	3599764	7000707	74.04%	7.360%
42	23.997	3548	3555	3568	rVB2	2034836	4190266	44.32%	4.405%




Sum of corrected areas: 95123048

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036618.D
Acq On : 21 Sep 2022 11:00
Operator : CG/JU
Sample : PB147714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

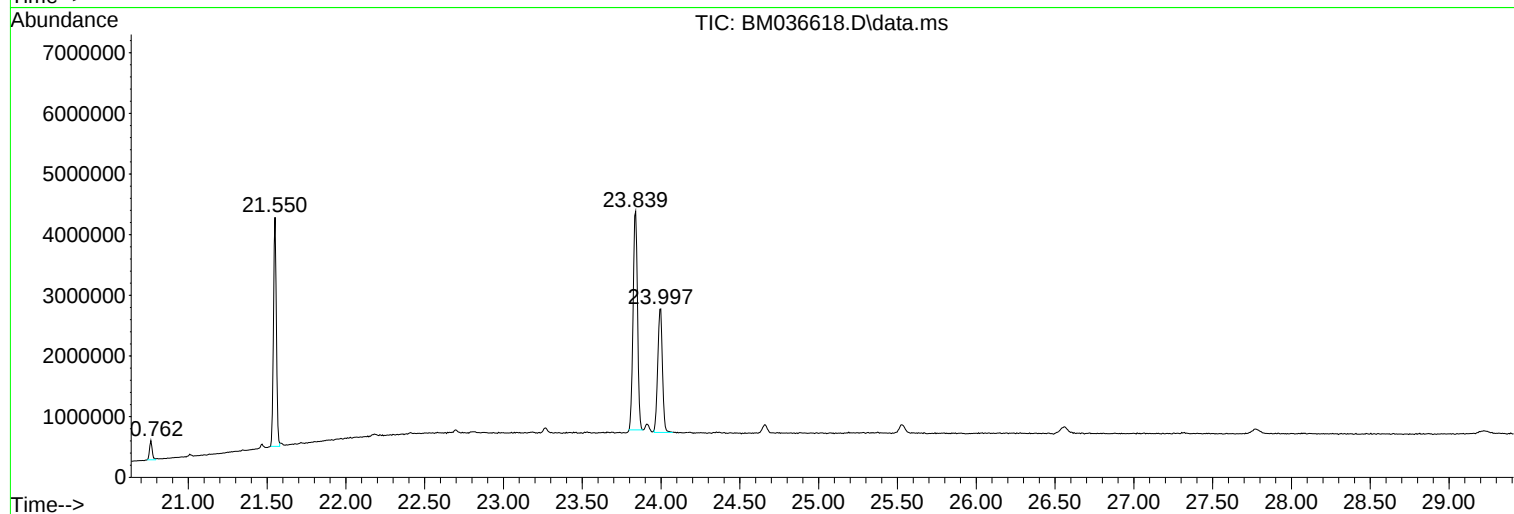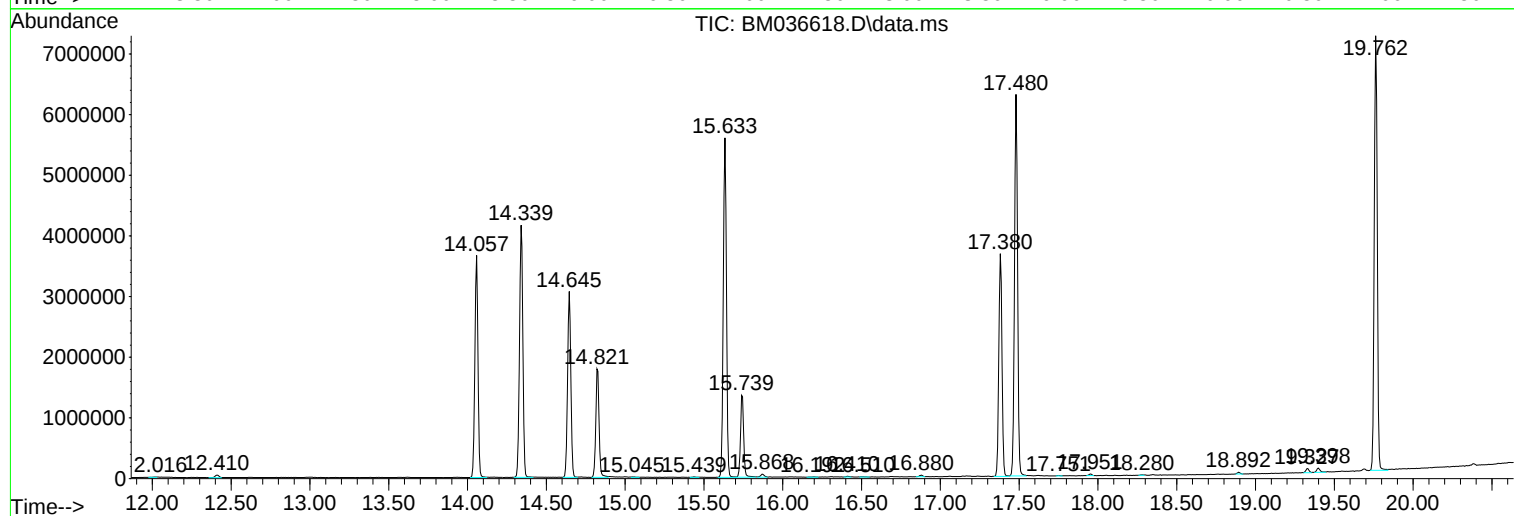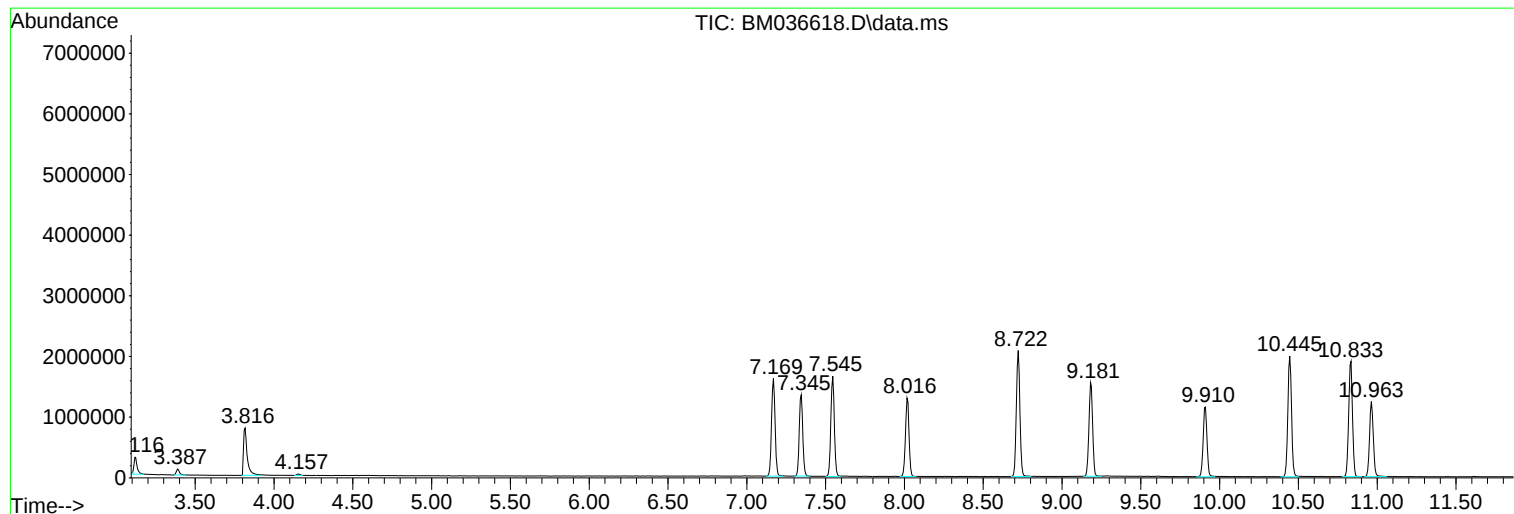

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036618.D
Acq On : 21 Sep 2022 11:00
Operator : CG/JU
Sample : PB147714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036618.D
Acq On : 21 Sep 2022 11:00
Operator : CG/JU
Sample : PB147714BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK714

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc