

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036619.D
 Acq On : 21 Sep 2022 11:35
 Operator : CG/JU
 Sample : PB147717BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK717

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	21	rVB	338897	458824	4.56%	0.434%
2	3.393	47	52	64	rVB	115751	165620	1.65%	0.157%
3	3.816	121	124	147	rBV	930211	1438163	14.30%	1.361%
4	4.157	178	182	192	rVB	28601	43948	0.44%	0.042%
5	7.175	687	695	705	rBV	1829759	2851999	28.35%	2.700%
6	7.345	717	724	733	rBV	1513156	2383399	23.69%	2.256%
7	7.545	751	758	772	rBV	1844259	2910907	28.93%	2.755%
8	8.022	832	839	848	rVB	1593999	2487671	24.73%	2.355%
9	8.728	949	959	970	rBV	2293048	3730042	37.08%	3.531%
10	9.186	1027	1037	1048	rBV	1825128	2883026	28.66%	2.729%
11	9.910	1151	1160	1172	rBV	1391125	2216874	22.04%	2.098%
12	10.445	1243	1251	1265	rBV	2241603	3724071	37.02%	3.525%
13	10.833	1309	1317	1325	rBV	2355874	3871090	38.48%	3.664%
14	10.969	1331	1340	1358	rBV	1371154	2305883	22.92%	2.183%
15	12.410	1579	1585	1593	rBV	45494	75407	0.75%	0.071%
16	14.057	1858	1865	1875	rBV	4018357	5469464	54.37%	5.177%
17	14.339	1906	1913	1923	rBV	4783115	6813831	67.73%	6.450%
18	14.645	1958	1965	1974	rBV	3685810	5235811	52.04%	4.956%
19	14.827	1988	1996	2008	rBV	2018031	2843046	28.26%	2.691%
20	15.004	2023	2026	2031	rVB7	6429	10382	0.10%	0.010%
21	15.633	2126	2133	2142	rBV	6343444	8482098	84.31%	8.029%
22	15.745	2145	2152	2160	rBV	1502092	2015149	20.03%	1.907%
23	15.868	2169	2173	2181	rVB	51510	79463	0.79%	0.075%
24	16.315	2242	2249	2253	rBV7	5897	13274	0.13%	0.013%
25	16.415	2258	2266	2270	rBV3	17263	27868	0.28%	0.026%
26	16.880	2341	2345	2352	rBV5	12136	15945	0.16%	0.015%
27	17.062	2372	2376	2379	rBV5	8353	11878	0.12%	0.011%
28	17.380	2424	2430	2440	rBV	4315245	6006058	59.70%	5.685%
29	17.480	2440	2447	2461	rVV	6726714	9325382	92.69%	8.827%
30	17.951	2524	2527	2531	rBV4	8900	11106	0.11%	0.011%
31	18.051	2539	2544	2548	rBV8	8560	16844	0.17%	0.016%
32	19.327	2757	2761	2766	rBV2	72712	105140	1.05%	0.100%
33	19.398	2769	2773	2779	rVV	71861	100267	1.00%	0.095%
34	19.762	2829	2835	2846	rBV	7903763	10060508	100.00%	9.523%
35	20.762	3002	3005	3011	rVB	142318	149746	1.49%	0.142%
36	21.550	3133	3139	3149	rBV	4142106	5430022	53.97%	5.140%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036619.D
Acq On : 21 Sep 2022 11:35
Operator : CG/JU
Sample : PB147717BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK717

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	23.833	3520	3527	3536	rBV2	3751443	7299241	72.55%	6.909%
38	23.991	3547	3554	3565	rVB2	2200905	4577620	45.50%	4.333%




Sum of corrected areas: 105647067

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036619.D
Acq On : 21 Sep 2022 11:35
Operator : CG/JU
Sample : PB147717BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

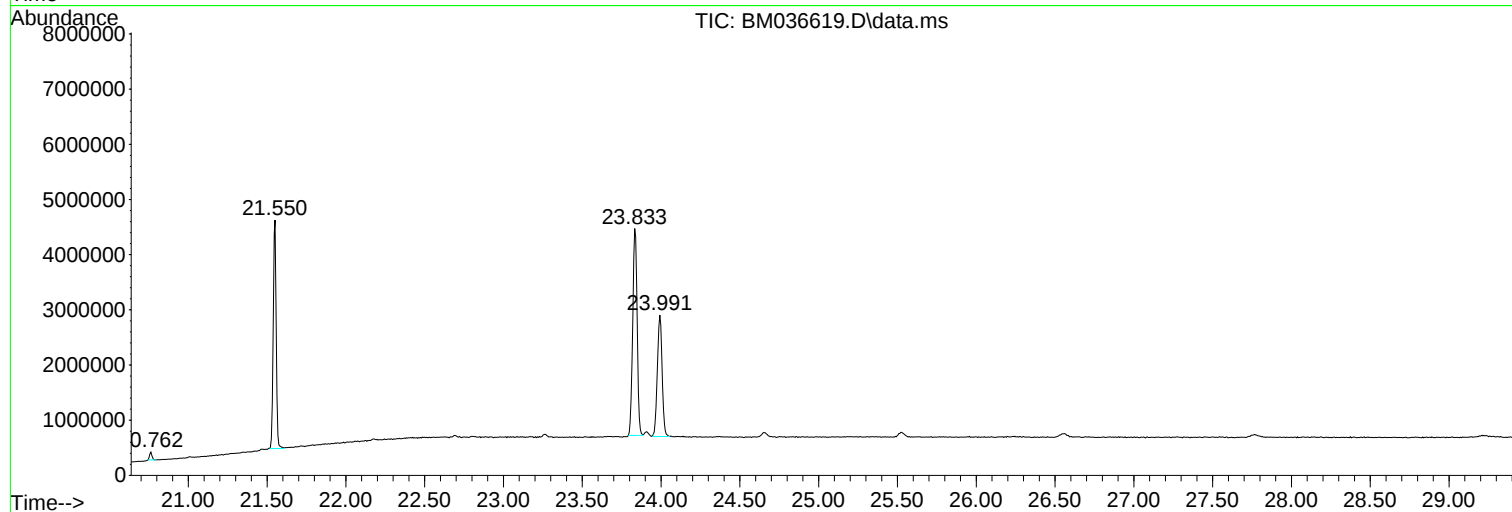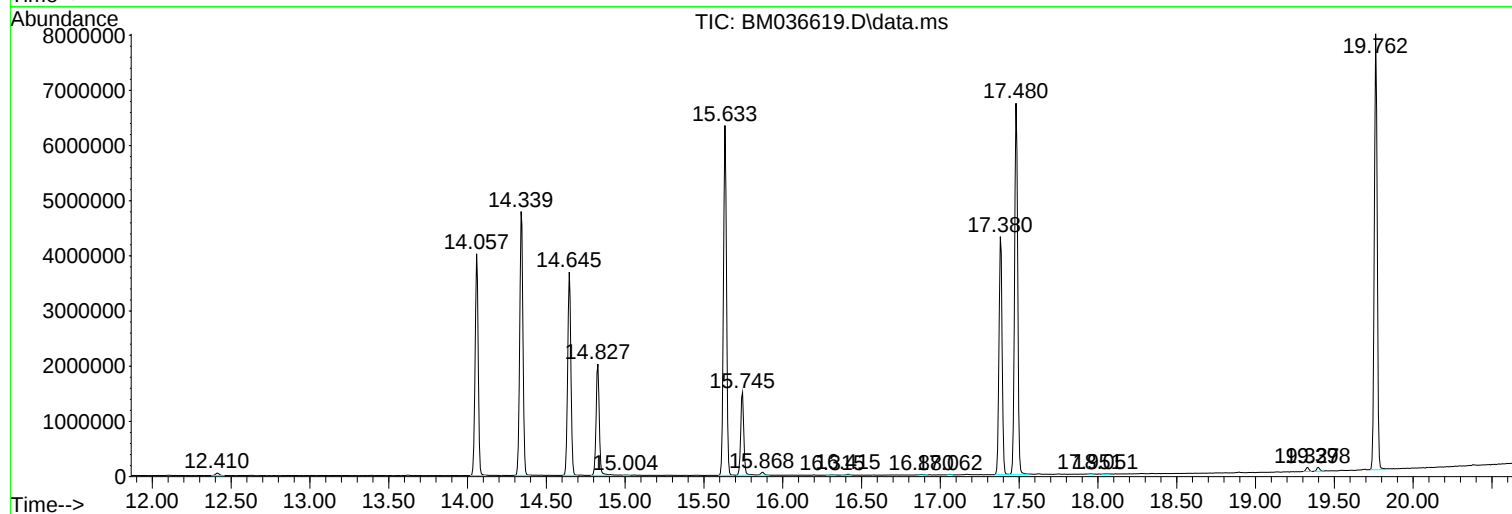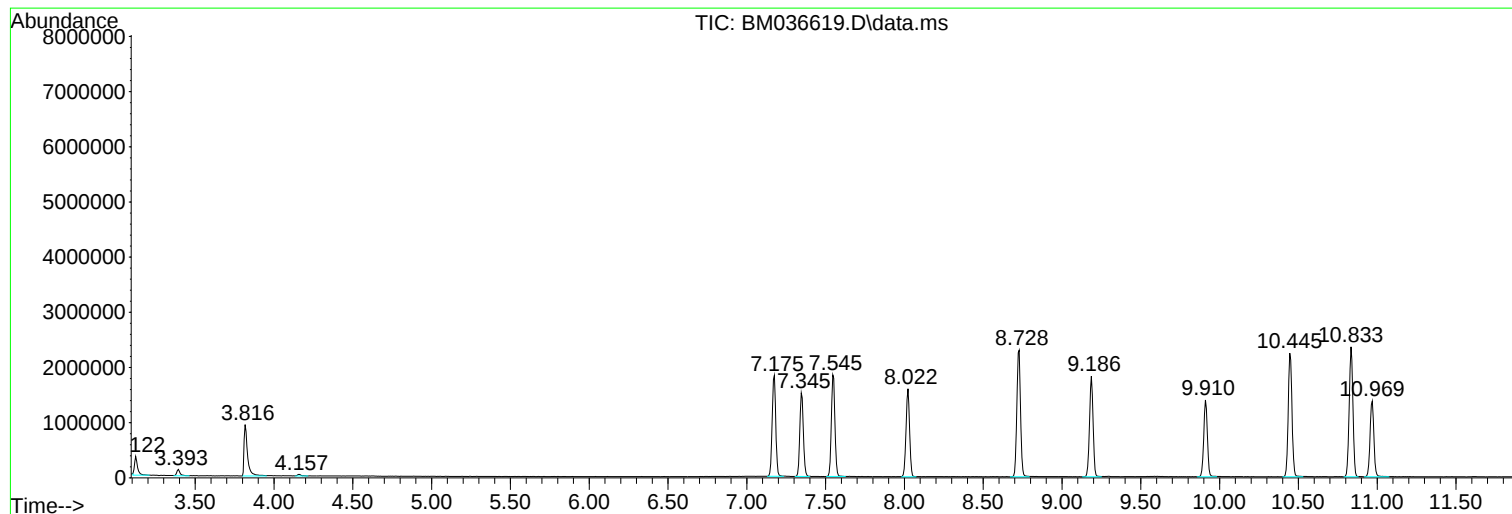

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036619.D
Acq On : 21 Sep 2022 11:35
Operator : CG/JU
Sample : PB147717BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036619.D
Acq On : 21 Sep 2022 11:35
Operator : CG/JU
Sample : PB147717BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK717

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc