

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036623.D
 Acq On : 21 Sep 2022 13:59
 Operator : CG/JU
 Sample : N4595-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036623.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	24	rVB	7475202	9979990	96.83%	9.620%
2	3.363	43	47	48	rBV3	23071	24124	0.23%	0.023%
3	3.393	48	52	61	rVB	82993	127190	1.23%	0.123%
4	3.822	122	125	140	rBV	306045	469083	4.55%	0.452%
5	4.063	160	166	177	rVB2	44907	76090	0.74%	0.073%
6	4.157	179	182	190	rVB	24351	33004	0.32%	0.032%
7	5.104	337	343	354	rVB	116141	176388	1.71%	0.170%
8	7.175	688	695	705	rVB	345899	558336	5.42%	0.538%
9	7.345	715	724	733	rBV	1323190	2101102	20.39%	2.025%
10	7.422	733	737	742	rVB2	7803	14438	0.14%	0.014%
11	7.551	748	759	770	rBV	1223177	1964556	19.06%	1.894%
12	8.022	832	839	846	rBV	1305018	2034741	19.74%	1.961%
13	8.087	847	850	855	rVB4	11600	17722	0.17%	0.017%
14	8.728	951	959	967	rBV	1055789	1684062	16.34%	1.623%
15	9.186	1027	1037	1047	rBV	1585680	2566326	24.90%	2.474%
16	9.292	1050	1055	1062	rVB7	8932	18770	0.18%	0.018%
17	9.622	1107	1111	1118	rVB5	8790	17176	0.17%	0.017%
18	9.910	1151	1160	1173	rBV	1193742	1939185	18.82%	1.869%
19	10.451	1243	1252	1268	rBV	1874051	3089263	29.97%	2.978%
20	10.616	1276	1280	1283	rBV4	12615	18756	0.18%	0.018%
21	10.833	1309	1317	1327	rBV	1951651	3226391	31.31%	3.110%
22	10.969	1332	1340	1349	rBV	1398325	2352865	22.83%	2.268%
23	11.198	1373	1379	1383	rBV9	10464	18791	0.18%	0.018%
24	11.610	1443	1449	1453	rBV9	8181	16593	0.16%	0.016%
25	11.716	1461	1467	1471	rBV7	5926	11199	0.11%	0.011%
26	12.110	1528	1534	1540	rBV5	7403	15593	0.15%	0.015%
27	12.327	1565	1571	1576	rBV8	8329	13527	0.13%	0.013%
28	12.410	1579	1585	1592	rVV	40189	69944	0.68%	0.067%
29	12.639	1619	1624	1628	rVB5	10897	17897	0.17%	0.017%
30	13.257	1722	1729	1738	rVB5	11869	28453	0.28%	0.027%
31	13.486	1763	1768	1772	rVB7	6592	10551	0.10%	0.010%
32	13.621	1786	1791	1795	rVB5	9736	14528	0.14%	0.014%
33	14.057	1858	1865	1875	rBV	4047536	5511454	53.48%	5.313%
34	14.339	1906	1913	1923	rVV	4413327	6481223	62.89%	6.248%
35	14.645	1955	1965	1975	rVV	3129661	4611123	44.74%	4.445%
36	14.721	1975	1978	1983	rVB7	7521	11399	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036623.D
 Acq On : 21 Sep 2022 13:59
 Operator : CG/JU
 Sample : N4595-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8G5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	14.821	1989	1995	2003	rBV	366626	560513	5.44%	0.540%
38	14.998	2019	2025	2030	rVB10	8197	20622	0.20%	0.020%
39	15.057	2030	2035	2040	rBV8	22535	36328	0.35%	0.035%
40	15.439	2095	2100	2106	rBV5	13497	26743	0.26%	0.026%
41	15.633	2124	2133	2144	rBV	6084238	8477210	82.25%	8.172%
42	15.745	2146	2152	2167	rVV	1616922	2242975	21.76%	2.162%
43	15.874	2169	2174	2181	rVB	52710	90104	0.87%	0.087%
44	16.139	2213	2219	2223	rBV5	14661	24232	0.24%	0.023%
45	16.204	2223	2230	2235	rVB10	9488	17867	0.17%	0.017%
46	16.415	2262	2266	2270	rVB5	15618	21566	0.21%	0.021%
47	16.527	2280	2285	2289	rBV7	5494	11212	0.11%	0.011%
48	16.645	2301	2305	2309	rVB6	10030	11932	0.12%	0.012%
49	16.874	2342	2344	2349	rVB4	14123	19510	0.19%	0.019%
50	17.062	2373	2376	2381	rVB7	13995	19645	0.19%	0.019%
51	17.145	2385	2390	2391	rBV4	11361	15241	0.15%	0.015%
52	17.380	2424	2430	2439	rBV	3816914	5334485	51.76%	5.142%
53	17.480	2441	2447	2459	rVV	6741367	9413677	91.34%	9.074%
54	17.751	2491	2493	2500	rVB8	9329	15097	0.15%	0.015%
55	17.956	2524	2528	2530	rVB	15188	17603	0.17%	0.017%
56	18.051	2542	2544	2551	rVB5	18089	24444	0.24%	0.024%
57	18.274	2578	2582	2590	rBV2	134771	205053	1.99%	0.198%
58	19.327	2757	2761	2768	rBV	80418	123472	1.20%	0.119%
59	19.398	2769	2773	2777	rBV	96448	130197	1.26%	0.126%
60	19.545	2795	2798	2803	rBV2	100654	135192	1.31%	0.130%
61	19.698	2820	2824	2828	rVB3	38882	55901	0.54%	0.054%
62	19.762	2829	2835	2848	rBV	7947067	10306230	100.00%	9.935%
63	20.762	3002	3005	3008	rVB	168099	177374	1.72%	0.171%
64	21.256	3086	3089	3095	rBV3	172076	227935	2.21%	0.220%
65	21.550	3134	3139	3144	rBV	3810879	4917445	47.71%	4.740%
66	23.833	3520	3527	3535	rBV2	3888969	7619508	73.93%	7.345%
67	23.991	3548	3554	3563	rVB2	2023495	4117153	39.95%	3.969%




Sum of corrected areas: 103738299

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036623.D
Acq On : 21 Sep 2022 13:59
Operator : CG/JU
Sample : N4595-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

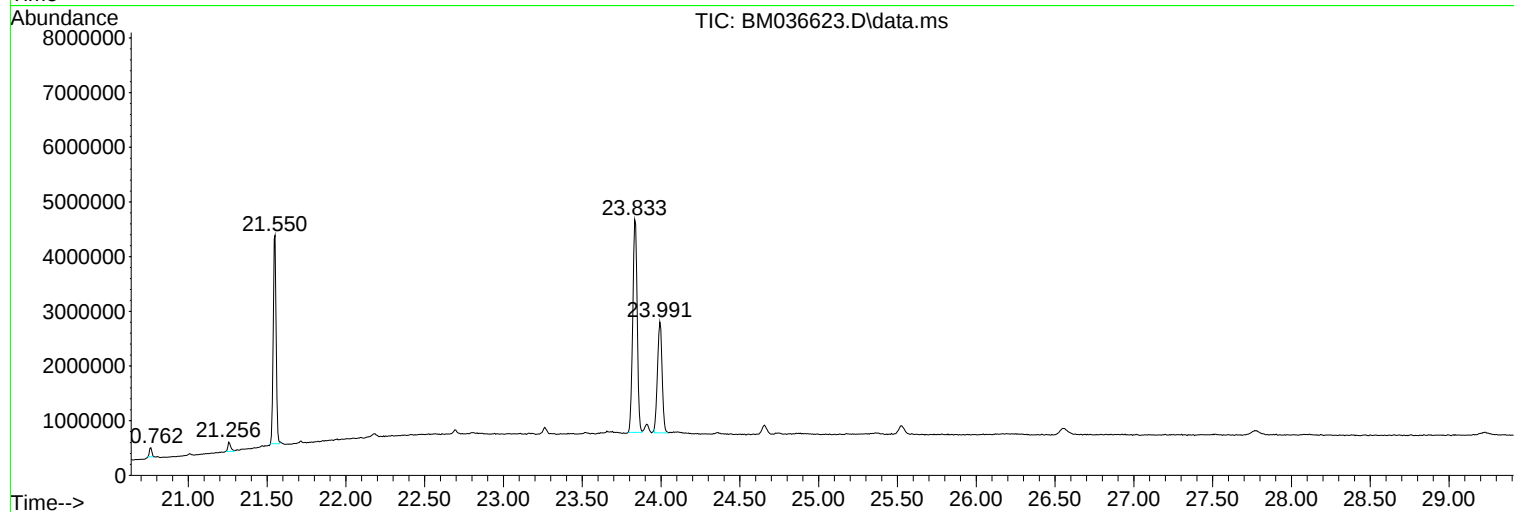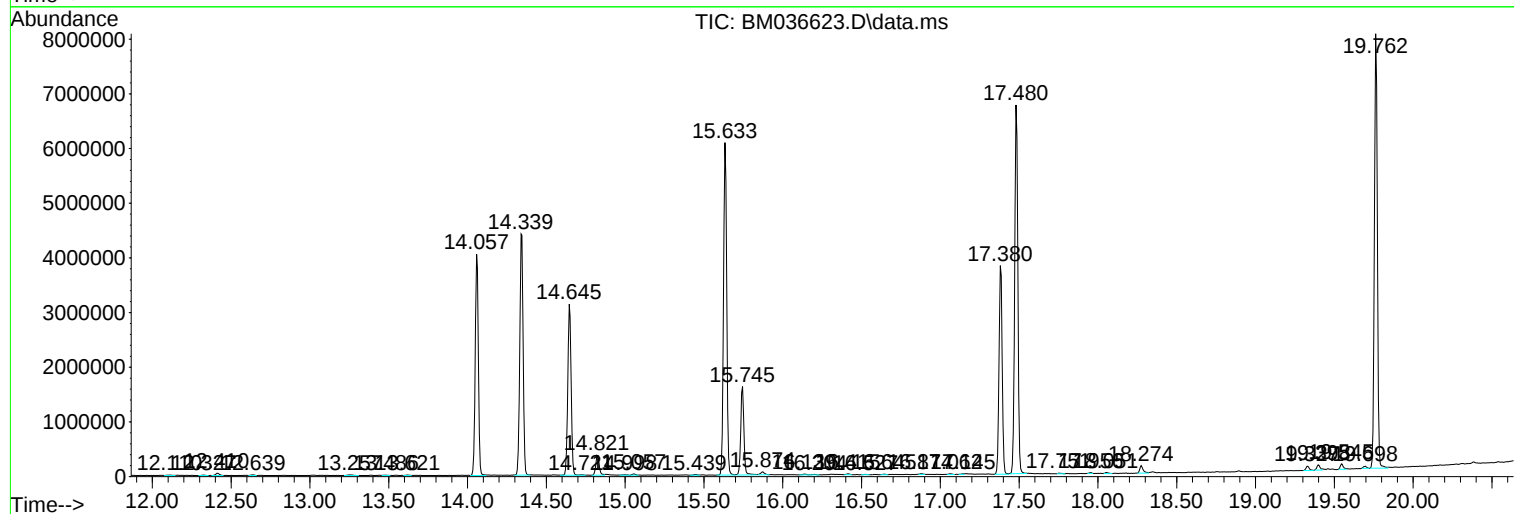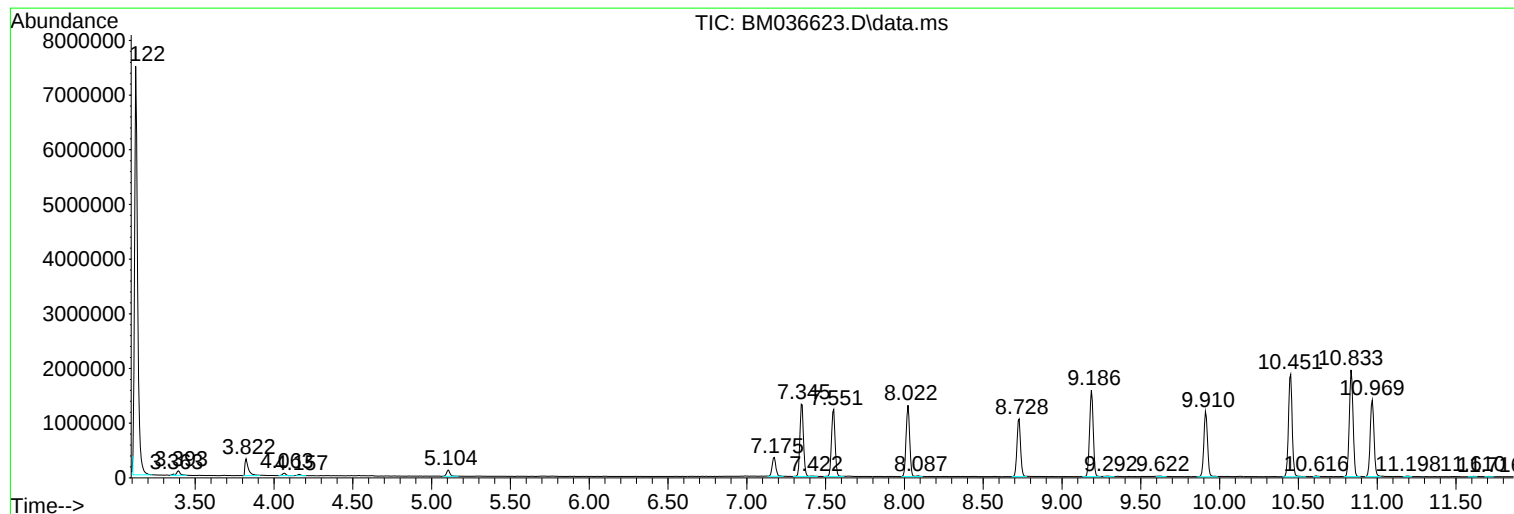

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036623.D
Acq On : 21 Sep 2022 13:59
Operator : CG/JU
Sample : N4595-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.122	98.10 ng/ul	9979990	1,4-Dichlorobenzene-d4	8.022

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

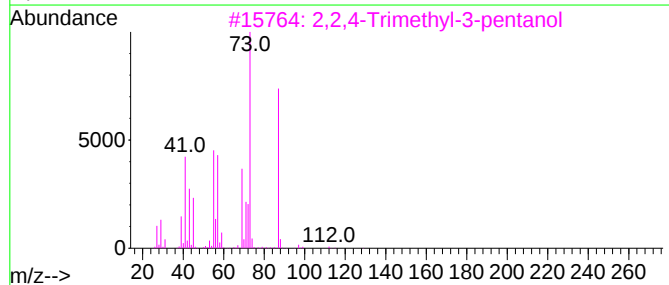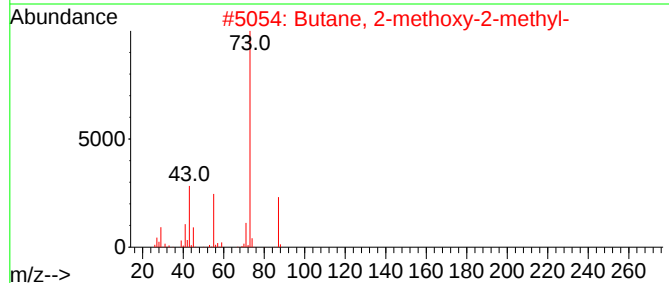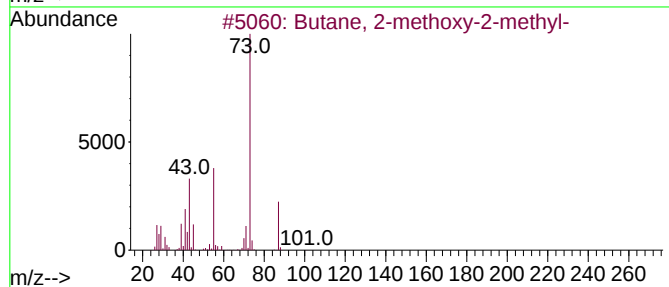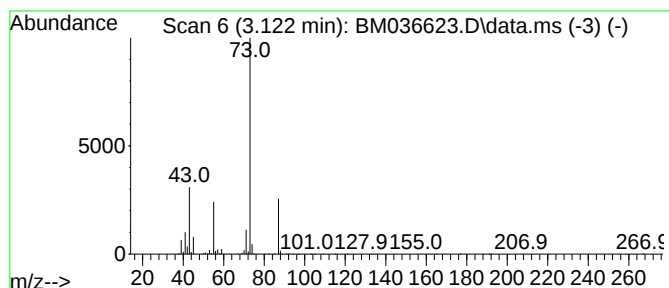

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036623.D
Acq On : 21 Sep 2022 13:59
Operator : CG/JU
Sample : N4595-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.122	98.1	ng/u1	9979990	1	8.022	2034740	20.0