

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036640.D
 Acq On : 22 Sep 2022 00:46
 Operator : CG/JU
 Sample : N4605-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5783

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	28	rVB	4843057	7653339	100.00%	15.866%
2	3.387	49	51	58	rVB	18876	29284	0.38%	0.061%
3	3.681	99	101	108	rVB	9100	12654	0.17%	0.026%
4	4.063	161	166	175	rVB	33695	61986	0.81%	0.129%
5	4.158	178	182	189	rVB	37491	62296	0.81%	0.129%
6	4.540	244	247	253	rVB8	5237	8098	0.11%	0.017%
7	5.093	337	341	349	rVB3	17444	32196	0.42%	0.067%
8	5.704	441	445	451	rVB6	6477	13767	0.18%	0.029%
9	7.004	660	666	669	rBV7	10913	22082	0.29%	0.046%
10	7.098	680	682	687	rVB4	6665	8992	0.12%	0.019%
11	7.175	687	695	704	rBV	342666	574537	7.51%	1.191%
12	7.346	718	724	733	rBV	334915	512070	6.69%	1.062%
13	7.546	751	758	768	rBV	360235	591794	7.73%	1.227%
14	7.640	771	774	777	rBV4	9748	14048	0.18%	0.029%
15	8.022	831	839	846	rBV	788318	1269851	16.59%	2.633%
16	8.728	952	959	968	rBV	382591	622029	8.13%	1.290%
17	8.845	973	979	986	rVB	30426	48936	0.64%	0.101%
18	9.187	1028	1037	1044	rBV	367382	613006	8.01%	1.271%
19	9.298	1051	1056	1060	rBV	12948	20826	0.27%	0.043%
20	9.610	1107	1109	1114	rVB5	7671	10724	0.14%	0.022%
21	9.910	1151	1160	1169	rBV	274688	471646	6.16%	0.978%
22	10.051	1179	1184	1189	rBV3	13312	23271	0.30%	0.048%
23	10.139	1196	1199	1204	rVB7	5417	8560	0.11%	0.018%
24	10.263	1217	1220	1227	rVB6	8063	15443	0.20%	0.032%
25	10.451	1244	1252	1261	rBV	444821	760153	9.93%	1.576%
26	10.610	1274	1279	1285	rBV3	16057	27795	0.36%	0.058%
27	10.834	1308	1317	1324	rBV	1199351	1998706	26.12%	4.143%
28	10.969	1328	1340	1352	rVV	236167	418334	5.47%	0.867%
29	11.363	1403	1407	1415	rVB	6880	14934	0.20%	0.031%
30	11.616	1446	1450	1457	rVB8	11080	18366	0.24%	0.038%
31	12.098	1525	1532	1536	rBV9	6023	13377	0.17%	0.028%
32	12.404	1580	1584	1592	rVB3	14025	24768	0.32%	0.051%
33	13.028	1684	1690	1694	rVB9	7042	13249	0.17%	0.027%
34	13.263	1726	1730	1734	rVB7	7228	12467	0.16%	0.026%
35	13.616	1786	1790	1795	rVB7	6045	10580	0.14%	0.022%
36	13.845	1827	1829	1834	rVB6	8658	11959	0.16%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036640.D
 Acq On : 22 Sep 2022 00:46
 Operator : CG/JU
 Sample : N4605-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A5783

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	13.975	1846	1851	1854	rVB7	6460	10317	0.13%	0.021%
38	14.057	1857	1865	1875	rBV	938143	1315010	17.18%	2.726%
39	14.292	1901	1905	1907	rBV5	5959	8748	0.11%	0.018%
40	14.339	1907	1913	1923	rVB	1066721	1523272	19.90%	3.158%
41	14.645	1957	1965	1975	rBV	1966058	2862247	37.40%	5.934%
42	14.827	1990	1996	2009	rBV	386973	589867	7.71%	1.223%
43	14.992	2019	2024	2027	rBV6	9063	13222	0.17%	0.027%
44	15.051	2029	2034	2042	rVV4	33505	55225	0.72%	0.114%
45	15.439	2094	2100	2101	rBV5	9804	13566	0.18%	0.028%
46	15.633	2125	2133	2142	rBV	1466212	2123109	27.74%	4.401%
47	15.739	2145	2151	2160	rBV	274113	402885	5.26%	0.835%
48	15.869	2169	2173	2177	rBV5	14581	20816	0.27%	0.043%
49	16.351	2252	2255	2262	rBV8	6403	14465	0.19%	0.030%
50	16.874	2340	2344	2349	rBV2	13929	21103	0.28%	0.044%
51	16.921	2350	2352	2357	rVB5	8642	10584	0.14%	0.022%
52	17.380	2424	2430	2440	rBV	2581535	3598430	47.02%	7.460%
53	17.480	2440	2447	2456	rVV	1708605	2401636	31.38%	4.979%
54	17.563	2458	2461	2466	rVB7	24765	38893	0.51%	0.081%
55	18.051	2540	2544	2549	rBV	76848	100192	1.31%	0.208%
56	18.274	2577	2582	2589	rBV	258189	395687	5.17%	0.820%
57	18.886	2684	2686	2690	rVB2	22024	22187	0.29%	0.046%
58	19.545	2794	2798	2804	rBV2	116637	171250	2.24%	0.355%
59	19.762	2829	2835	2840	rBV	2321534	3140170	41.03%	6.510%
60	20.756	3001	3004	3008	rBV	187586	212775	2.78%	0.441%
61	21.256	3085	3089	3095	rBV	707383	916028	11.97%	1.899%
62	21.545	3134	3138	3150	rVB	3429995	4532460	59.22%	9.396%
63	23.827	3521	3526	3534	rVB2	1665680	3213779	41.99%	6.662%
64	23.986	3547	3553	3562	rVB2	2204624	4483121	58.58%	9.294%




Sum of corrected areas: 48237167

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036640.D
Acq On : 22 Sep 2022 00:46
Operator : CG/JU
Sample : N4605-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A5783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

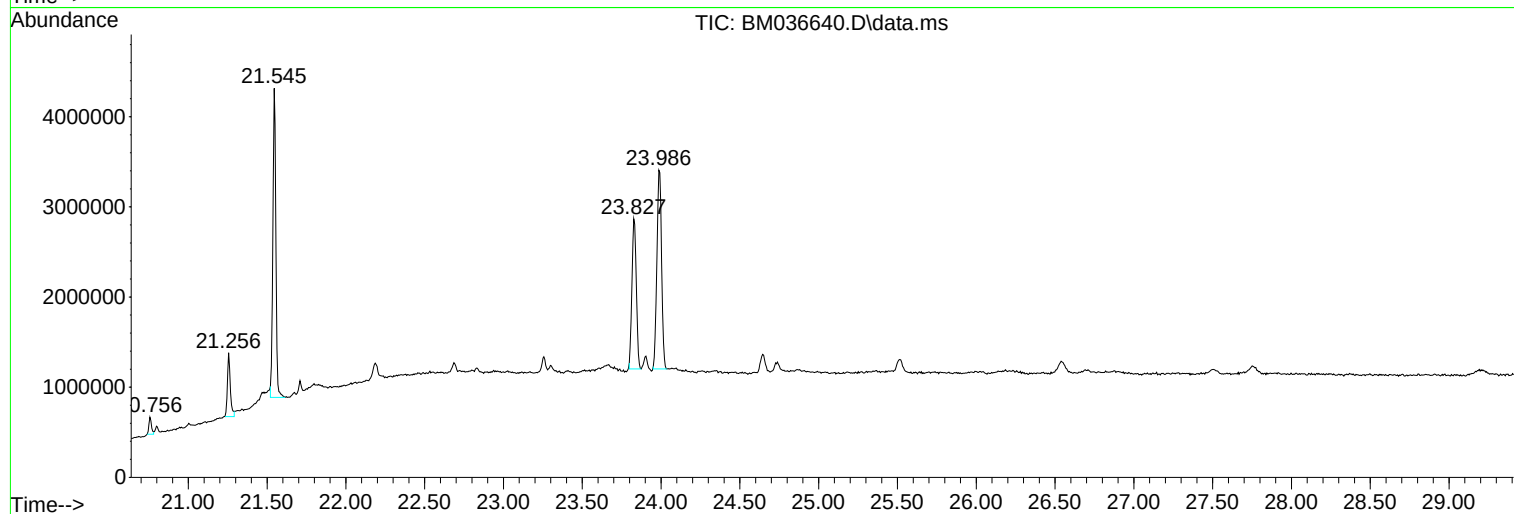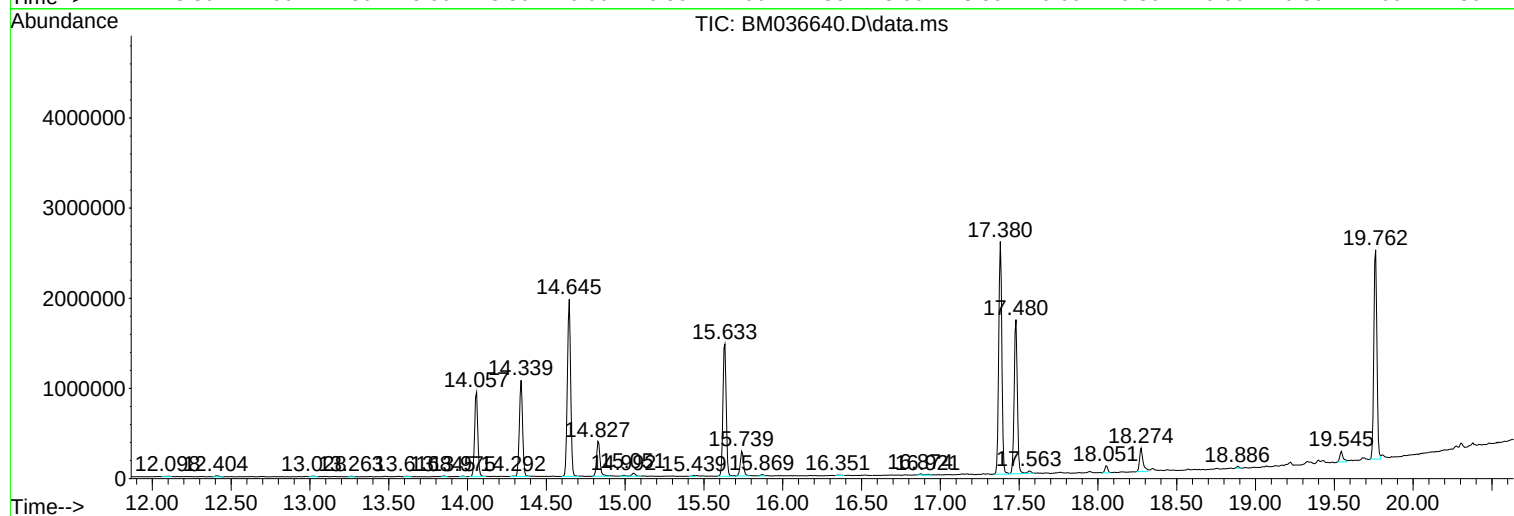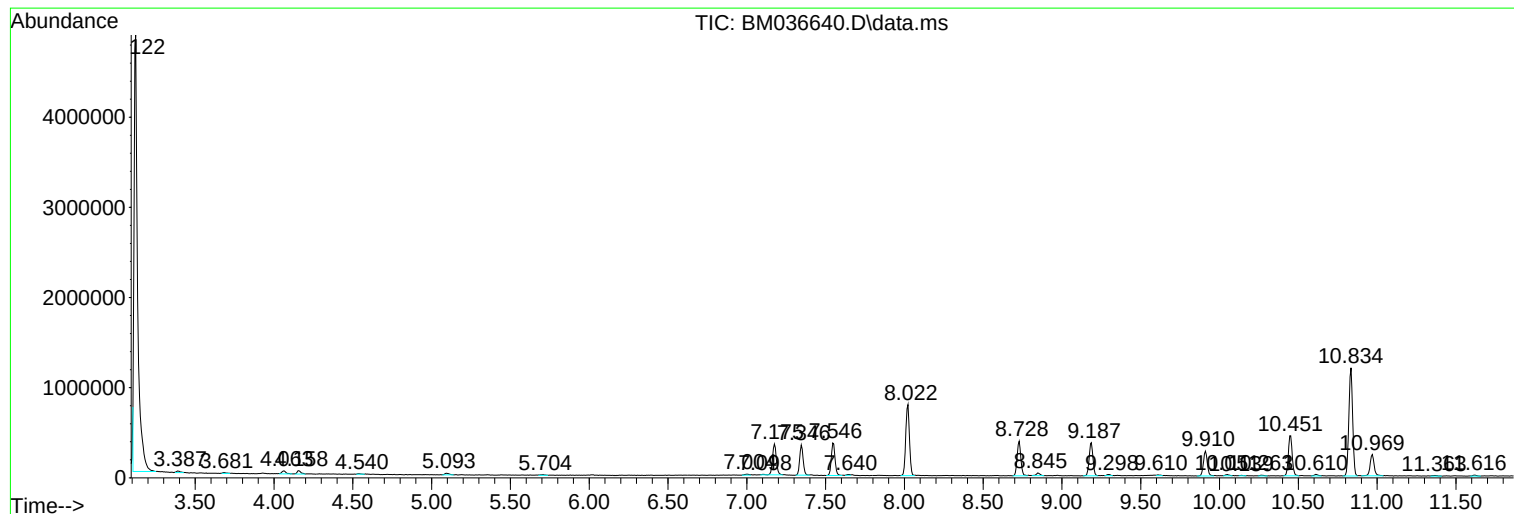

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036640.D
Acq On : 22 Sep 2022 00:46
Operator : CG/JU
Sample : N4605-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A5783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036640.D
Acq On : 22 Sep 2022 00:46
Operator : CG/JU
Sample : N4605-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A5783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc