

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036646.D
 Acq On : 22 Sep 2022 04:21
 Operator : CG/JU
 Sample : N4649-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.123	3	6	29	rVB	8203769	10877467	99.16%	8.976%
2	3.393	48	52	63	rVB	104058	156812	1.43%	0.129%
3	3.681	98	101	108	rVB	16346	25139	0.23%	0.021%
4	3.822	123	125	143	rBV	492573	809622	7.38%	0.668%
5	4.064	161	166	171	rVB	51514	75133	0.68%	0.062%
6	4.158	177	182	187	rBV	32706	48154	0.44%	0.040%
7	4.699	270	274	280	rVB	22764	32729	0.30%	0.027%
8	5.105	337	343	354	rVB	172622	240847	2.20%	0.199%
9	5.711	441	446	450	rBV5	6542	11871	0.11%	0.010%
10	7.175	688	695	706	rVB	488963	780765	7.12%	0.644%
11	7.346	717	724	734	rBV	1861709	2842033	25.91%	2.345%
12	7.546	751	758	770	rBV	1726845	2743505	25.01%	2.264%
13	7.640	770	774	778	rVB4	12887	17426	0.16%	0.014%
14	8.016	831	838	845	rBV	1702222	2721980	24.81%	2.246%
15	8.081	845	849	858	rVB3	17022	32707	0.30%	0.027%
16	8.728	950	959	968	rBV	1427889	2275453	20.74%	1.878%
17	9.187	1028	1037	1044	rBV	2120016	3453972	31.49%	2.850%
18	9.299	1050	1056	1060	rVB8	10042	17936	0.16%	0.015%
19	9.610	1106	1109	1114	rVB3	11149	16817	0.15%	0.014%
20	9.910	1151	1160	1173	rBV	1595492	2623804	23.92%	2.165%
21	10.446	1243	1251	1267	rBV	2439288	4048451	36.90%	3.341%
22	10.834	1307	1317	1325	rBV	2554533	4273054	38.95%	3.526%
23	10.963	1332	1339	1355	rBV	2270838	3849151	35.09%	3.176%
24	11.616	1445	1450	1453	rBV6	9638	17373	0.16%	0.014%
25	12.104	1530	1533	1540	rVB6	8563	14583	0.13%	0.012%
26	12.410	1578	1585	1592	rVB	51348	83723	0.76%	0.069%
27	13.275	1726	1732	1736	rVB2	15013	23253	0.21%	0.019%
28	13.475	1760	1766	1772	rVV	68063	94460	0.86%	0.078%
29	13.545	1775	1778	1785	rVV8	6066	12765	0.12%	0.011%
30	13.616	1785	1790	1795	rVB5	9454	18936	0.17%	0.016%
31	14.057	1858	1865	1875	rBV	4757053	6361567	57.99%	5.250%
32	14.287	1900	1904	1906	rBV5	7732	10976	0.10%	0.009%
33	14.339	1906	1913	1922	rVV	5568649	7817049	71.26%	6.451%
34	14.645	1956	1965	1974	rBV	3959086	5643041	51.44%	4.657%
35	14.828	1990	1996	2007	rBV	422979	620306	5.65%	0.512%
36	15.051	2030	2034	2040	rBV8	23556	33331	0.30%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036646.D
 Acq On : 22 Sep 2022 04:21
 Operator : CG/JU
 Sample : N4649-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	15.445	2096	2101	2104	rBV6	9099	17827	0.16%	0.015%
38	15.486	2104	2108	2117	rVB	91141	117636	1.07%	0.097%
39	15.633	2126	2133	2145	rBV	7281146	9954061	90.74%	8.214%
40	15.739	2145	2151	2165	rVV	1619833	2245722	20.47%	1.853%
41	15.869	2168	2173	2182	rVB	65165	105931	0.97%	0.087%
42	16.410	2261	2265	2270	rVB6	16393	23988	0.22%	0.020%
43	16.869	2338	2343	2348	rBV2	14477	22900	0.21%	0.019%
44	17.057	2372	2375	2380	rVB5	12004	17360	0.16%	0.014%
45	17.139	2385	2389	2403	rVV2	84477	135503	1.24%	0.112%
46	17.380	2423	2430	2438	rBV	4563921	6285362	57.30%	5.187%
47	17.480	2440	2447	2457	rVV	7596680	10636560	96.96%	8.778%
48	17.563	2458	2461	2465	rVB6	23029	35497	0.32%	0.029%
49	17.751	2490	2493	2498	rBV3	10159	16623	0.15%	0.014%
50	17.945	2524	2526	2531	rVB2	13760	17730	0.16%	0.015%
51	18.051	2540	2544	2548	rVB	41456	48535	0.44%	0.040%
52	18.274	2578	2582	2590	rBV2	132548	213136	1.94%	0.176%
53	18.574	2629	2633	2635	rBV2	23327	28940	0.26%	0.024%
54	19.327	2757	2761	2766	rBV3	91381	135063	1.23%	0.111%
55	19.392	2769	2772	2777	rBV	85254	122713	1.12%	0.101%
56	19.545	2794	2798	2803	rBV3	81157	127134	1.16%	0.105%
57	19.763	2829	2835	2841	rBV	8653127	10969944	100.00%	9.053%
58	20.757	3001	3004	3008	rVB	142192	141023	1.29%	0.116%
59	21.257	3086	3089	3095	rBV2	205309	239236	2.18%	0.197%
60	21.545	3133	3138	3146	rBV	4003712	5046110	46.00%	4.164%
61	23.827	3520	3526	3534	rVB2	3837588	7351447	67.01%	6.067%
62	23.986	3547	3553	3564	rVB2	2147856	4396247	40.08%	3.628%




Sum of corrected areas: 121178419

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036646.D
Acq On : 22 Sep 2022 04:21
Operator : CG/JU
Sample : N4649-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

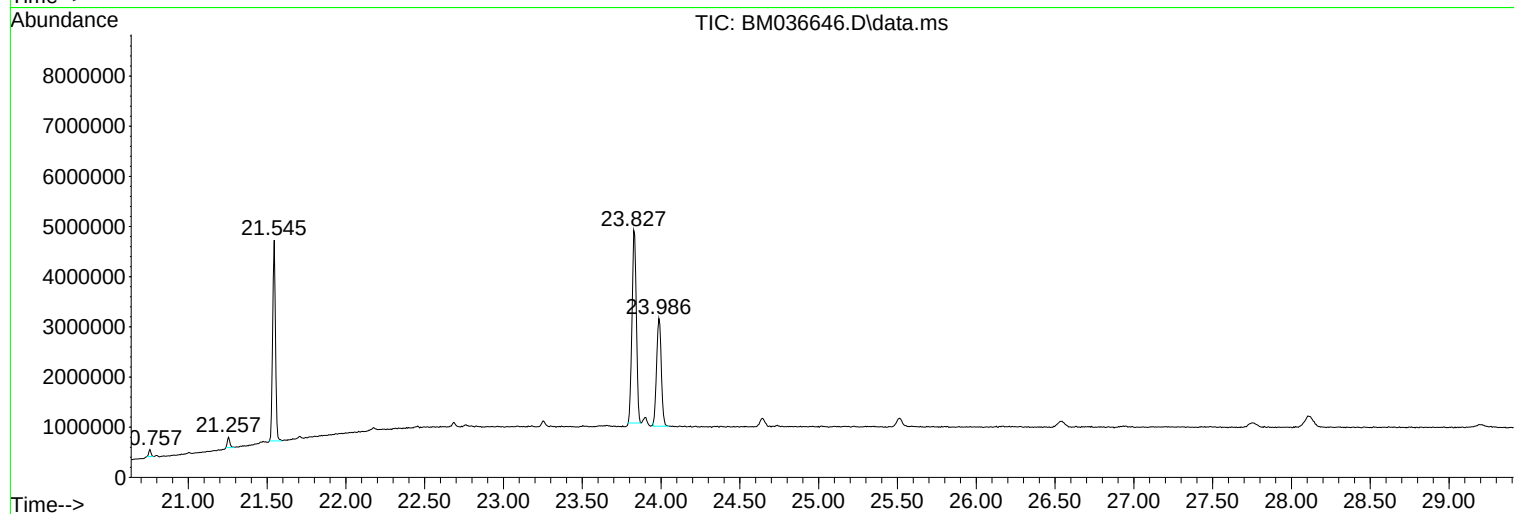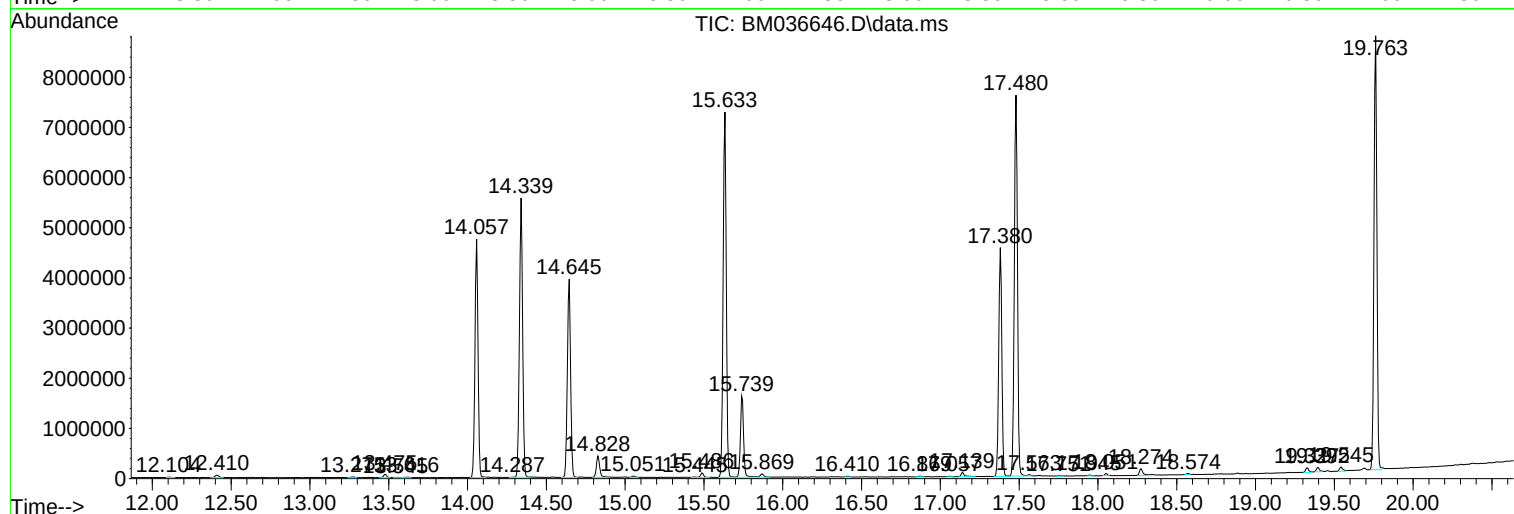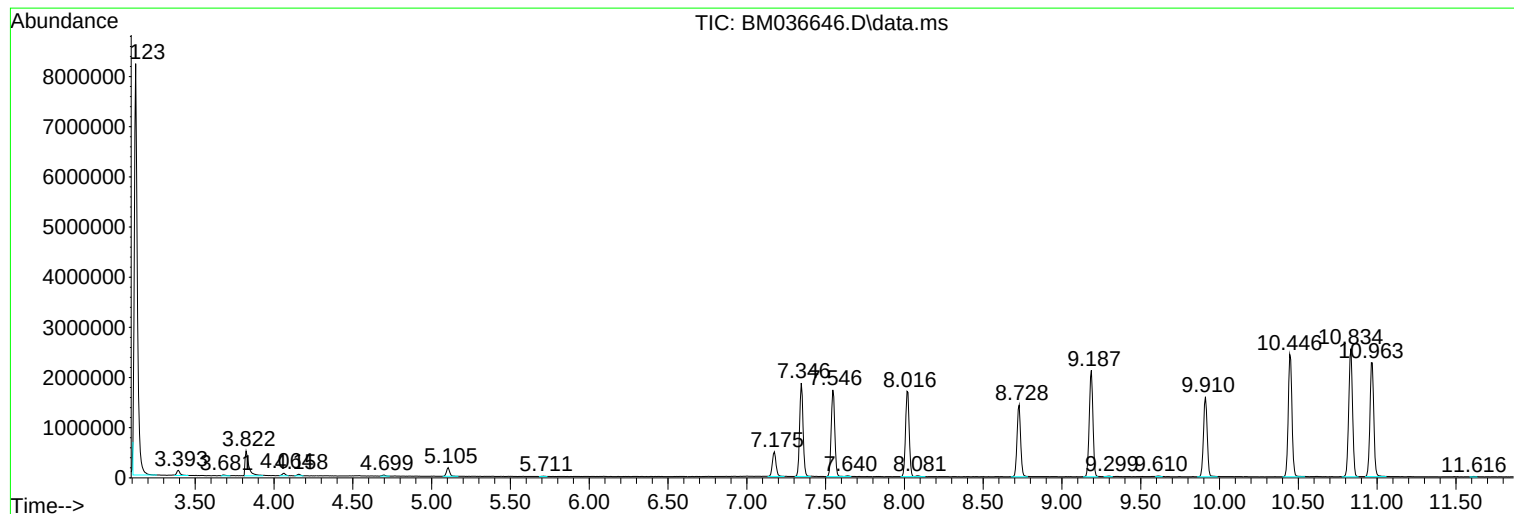

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036646.D
Acq On : 22 Sep 2022 04:21
Operator : CG/JU
Sample : N4649-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036646.D
Acq On : 22 Sep 2022 04:21
Operator : CG/JU
Sample : N4649-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ31

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc