

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036661.D
 Acq On : 22 Sep 2022 14:06
 Operator : CG/JU
 Sample : N4708-06
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	3	6	26	rVB	6874334	9174264	98.20%	9.373%
2	3.393	48	52	60	rVB	78792	115906	1.24%	0.118%
3	3.828	122	126	139	rBV	200574	340003	3.64%	0.347%
4	4.057	161	165	171	rVB	39506	60068	0.64%	0.061%
5	4.157	178	182	188	rVB	30159	41866	0.45%	0.043%
6	5.098	336	342	346	rBV7	10188	17487	0.19%	0.018%
7	6.016	493	498	503	rVV5	12519	19039	0.20%	0.019%
8	6.992	660	664	670	rVB4	13535	22127	0.24%	0.023%
9	7.104	679	683	687	rVB	20500	31628	0.34%	0.032%
10	7.175	688	695	711	rVB	389979	714671	7.65%	0.730%
11	7.345	717	724	731	rBV	1303967	2009776	21.51%	2.053%
12	7.545	751	758	767	rBV	1271315	1970166	21.09%	2.013%
13	7.639	770	774	776	rVV5	16461	23688	0.25%	0.024%
14	7.663	776	778	783	rVB	17354	23469	0.25%	0.024%
15	8.016	831	838	846	rBV	1399873	2260230	24.19%	2.309%
16	8.081	846	849	854	rVB3	10128	16427	0.18%	0.017%
17	8.581	927	934	942	rBV10	6176	13451	0.14%	0.014%
18	8.728	952	959	971	rBV	1085153	1719814	18.41%	1.757%
19	9.186	1030	1037	1046	rBV	1507256	2444769	26.17%	2.498%
20	9.292	1052	1055	1060	rVB5	12962	18662	0.20%	0.019%
21	9.351	1062	1065	1071	rVB7	9504	15713	0.17%	0.016%
22	9.610	1104	1109	1116	rVB2	28844	51821	0.55%	0.053%
23	9.910	1152	1160	1173	rBV	1132187	1820070	19.48%	1.860%
24	10.445	1241	1251	1266	rBV	1823051	3010136	32.22%	3.075%
25	10.610	1274	1279	1287	rBV2	59029	100070	1.07%	0.102%
26	10.833	1309	1317	1324	rBV	2210604	3590888	38.44%	3.669%
27	10.963	1331	1339	1354	rBV	900621	1612803	17.26%	1.648%
28	11.622	1446	1451	1457	rVB7	8676	15781	0.17%	0.016%
29	12.104	1528	1533	1541	rVB2	24104	42045	0.45%	0.043%
30	12.245	1548	1557	1561	rBV8	8270	16123	0.17%	0.016%
31	12.410	1578	1585	1593	rVB	37794	58721	0.63%	0.060%
32	13.016	1685	1688	1693	rBV6	6914	10448	0.11%	0.011%
33	13.263	1727	1730	1736	rVB6	9090	10087	0.11%	0.010%
34	13.474	1761	1766	1774	rVB2	30952	46954	0.50%	0.048%
35	13.545	1774	1778	1786	rBV7	9188	17490	0.19%	0.018%
36	13.621	1786	1791	1795	rVB5	8278	14283	0.15%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
 Data File : BM036661.D
 Acq On : 22 Sep 2022 14:06
 Operator : CG/JU
 Sample : N4708-06
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8K6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	14.057	1857	1865	1875	rBV	3756638	5035187	53.90%	5.145%
38	14.292	1901	1905	1907	rBV3	10576	15753	0.17%	0.016%
39	14.339	1907	1913	1926	rVB	4142645	5858373	62.71%	5.986%
40	14.539	1944	1947	1952	rVB6	13522	18768	0.20%	0.019%
41	14.645	1958	1965	1973	rBV	3430743	4926695	52.74%	5.034%
42	14.827	1988	1996	2007	rBV	362181	556602	5.96%	0.569%
43	14.998	2017	2025	2029	rBV9	10461	21293	0.23%	0.022%
44	15.051	2029	2034	2042	rVB10	16278	27467	0.29%	0.028%
45	15.445	2096	2101	2106	rBV3	12485	20858	0.22%	0.021%
46	15.486	2106	2108	2116	rVB4	14516	18908	0.20%	0.019%
47	15.633	2126	2133	2145	rBV	5543257	7780796	83.29%	7.950%
48	15.739	2145	2151	2167	rVV	1332013	1849758	19.80%	1.890%
49	15.868	2168	2173	2181	rVB	50848	81684	0.87%	0.083%
50	16.192	2227	2228	2235	rVB7	6125	9636	0.10%	0.010%
51	16.315	2245	2249	2251	rBV4	9287	10519	0.11%	0.011%
52	16.415	2261	2266	2272	rVB6	18421	30081	0.32%	0.031%
53	16.786	2325	2329	2333	rVB5	7177	10769	0.12%	0.011%
54	16.874	2339	2344	2349	rVB2	19996	25158	0.27%	0.026%
55	17.057	2373	2375	2381	rVB7	7162	10193	0.11%	0.010%
56	17.139	2385	2389	2392	rBV2	31184	44286	0.47%	0.045%
57	17.298	2413	2416	2421	rVB7	12089	14669	0.16%	0.015%
58	17.380	2423	2430	2440	rBV	4039818	5632820	60.29%	5.755%
59	17.480	2440	2447	2461	rVV	6249358	8625570	92.33%	8.813%
60	17.751	2490	2493	2498	rBV6	11463	19497	0.21%	0.020%
61	17.945	2524	2526	2530	rVB3	18021	19772	0.21%	0.020%
62	18.051	2541	2544	2548	rVB3	16849	19977	0.21%	0.020%
63	18.274	2577	2582	2588	rBV	152463	237691	2.54%	0.243%
64	18.345	2592	2594	2599	rVB	30270	37629	0.40%	0.038%
65	19.327	2757	2761	2767	rBV3	72009	104152	1.11%	0.106%
66	19.398	2769	2773	2777	rBV	78961	107278	1.15%	0.110%
67	19.539	2794	2797	2802	rBV3	69158	101290	1.08%	0.103%
68	19.762	2829	2835	2846	rBV	7172852	9342342	100.00%	9.545%
69	20.756	3001	3004	3010	rVB2	230178	248123	2.66%	0.254%
70	21.256	3086	3089	3094	rBV2	293046	375774	4.02%	0.384%
71	21.544	3133	3138	3148	rBV	3661639	4780248	51.17%	4.884%
72	23.833	3520	3527	3534	rBV2	3269121	6346954	67.94%	6.485%
73	23.991	3547	3554	3565	rVB2	1944416	4037630	43.22%	4.125%




Sum of corrected areas: 97875144

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036661.D
Acq On : 22 Sep 2022 14:06
Operator : CG/JU
Sample : N4708-06
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

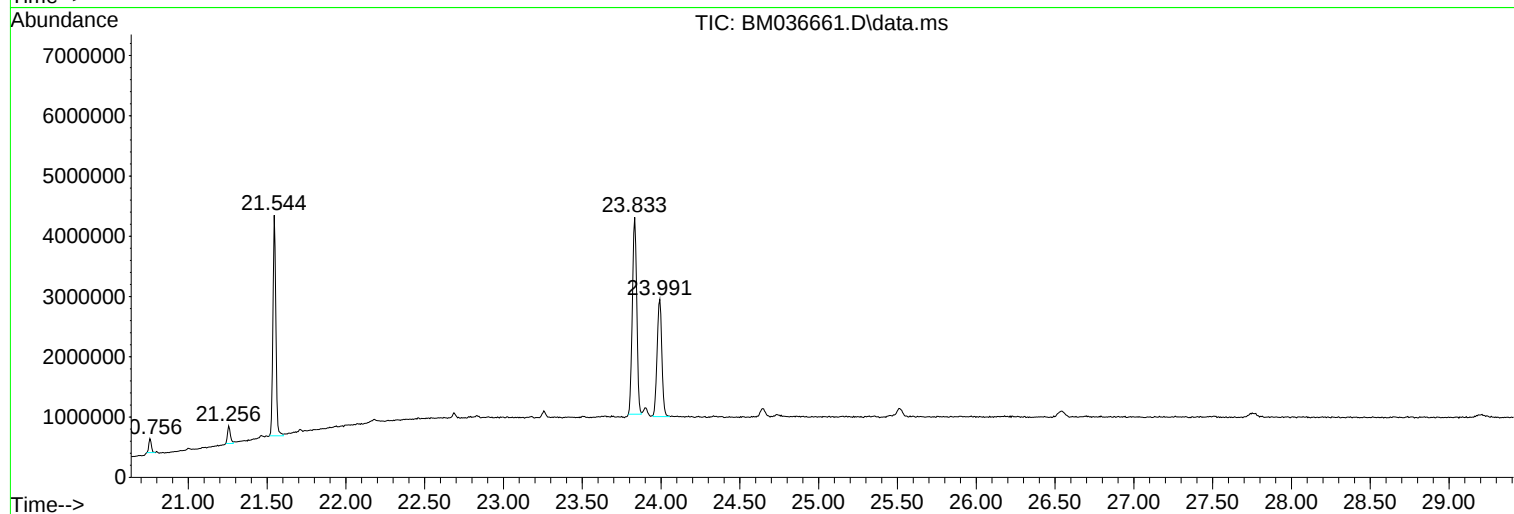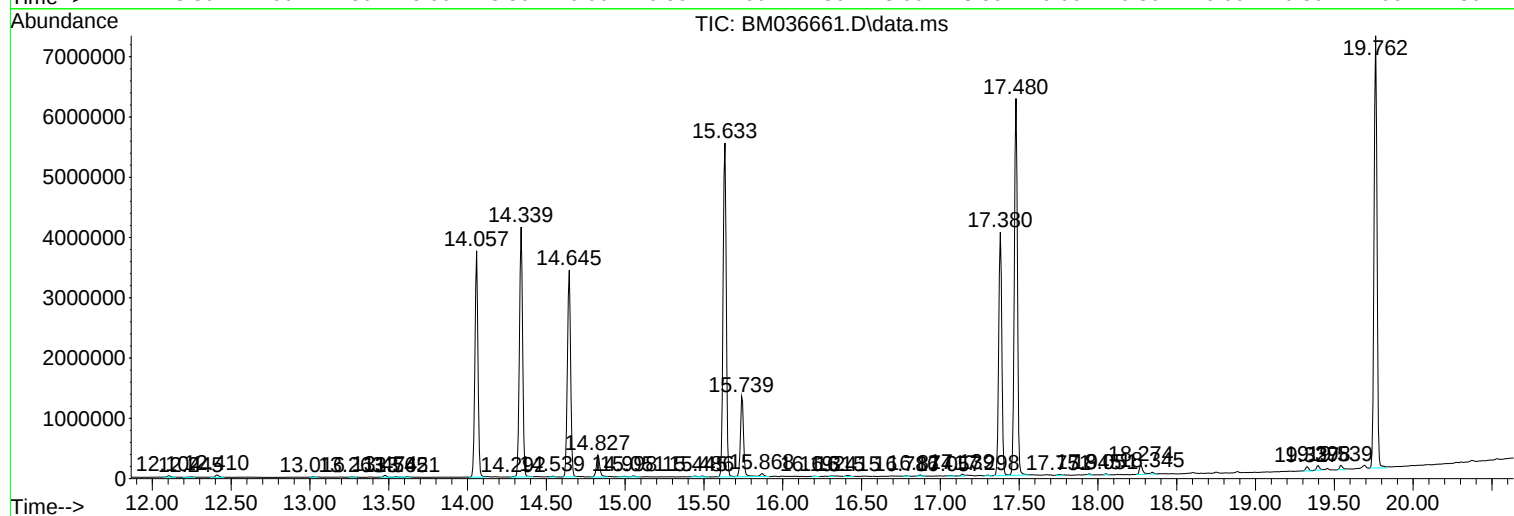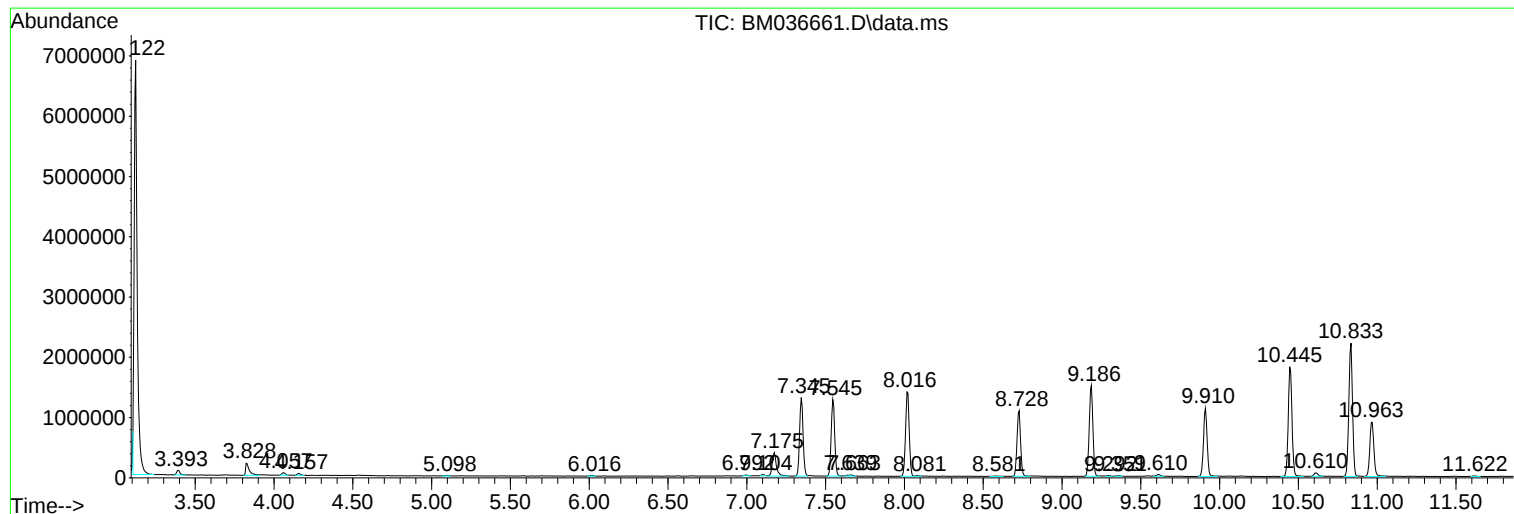

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036661.D
Acq On : 22 Sep 2022 14:06
Operator : CG/JU
Sample : N4708-06
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K6










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.122	81.18 ng/ul	9174260	1,4-Dichlorobenzene-d4	8.022

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

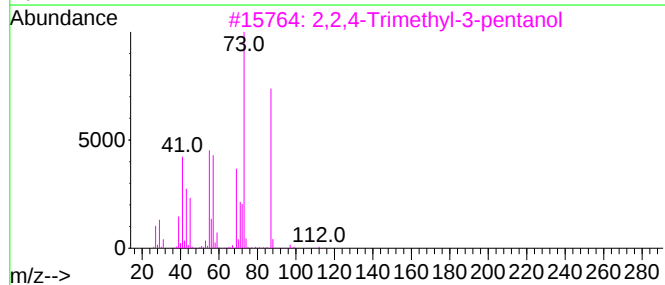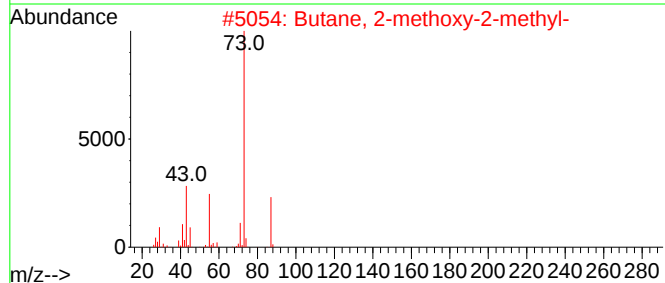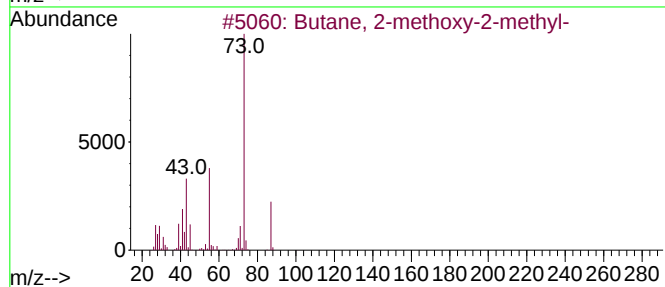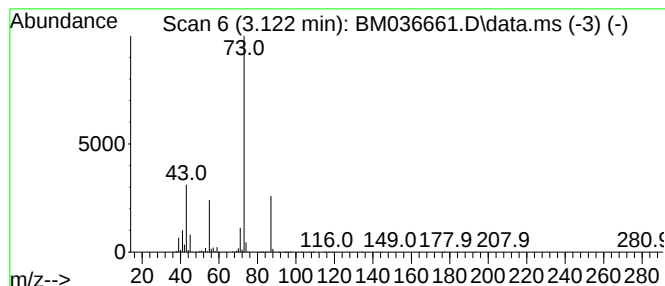

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092122\
Data File : BM036661.D
Acq On : 22 Sep 2022 14:06
Operator : CG/JU
Sample : N4708-06
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.122	81.2	ng/u1	9174260	1	8.022	2260230	20.0