


Data Path : Z:\HPCHEM1\BNA_M\Data\bm092215\
Data File : BM002703.D
Acq On : 22 Sep 2015 20:36
Operator : UM/IZ
Sample : G3741-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
Client Sampled :
JHAF6

Quant Time: Sep 23 09:08:56 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 03:40:59 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
9/23/2015 4:37:32 PM

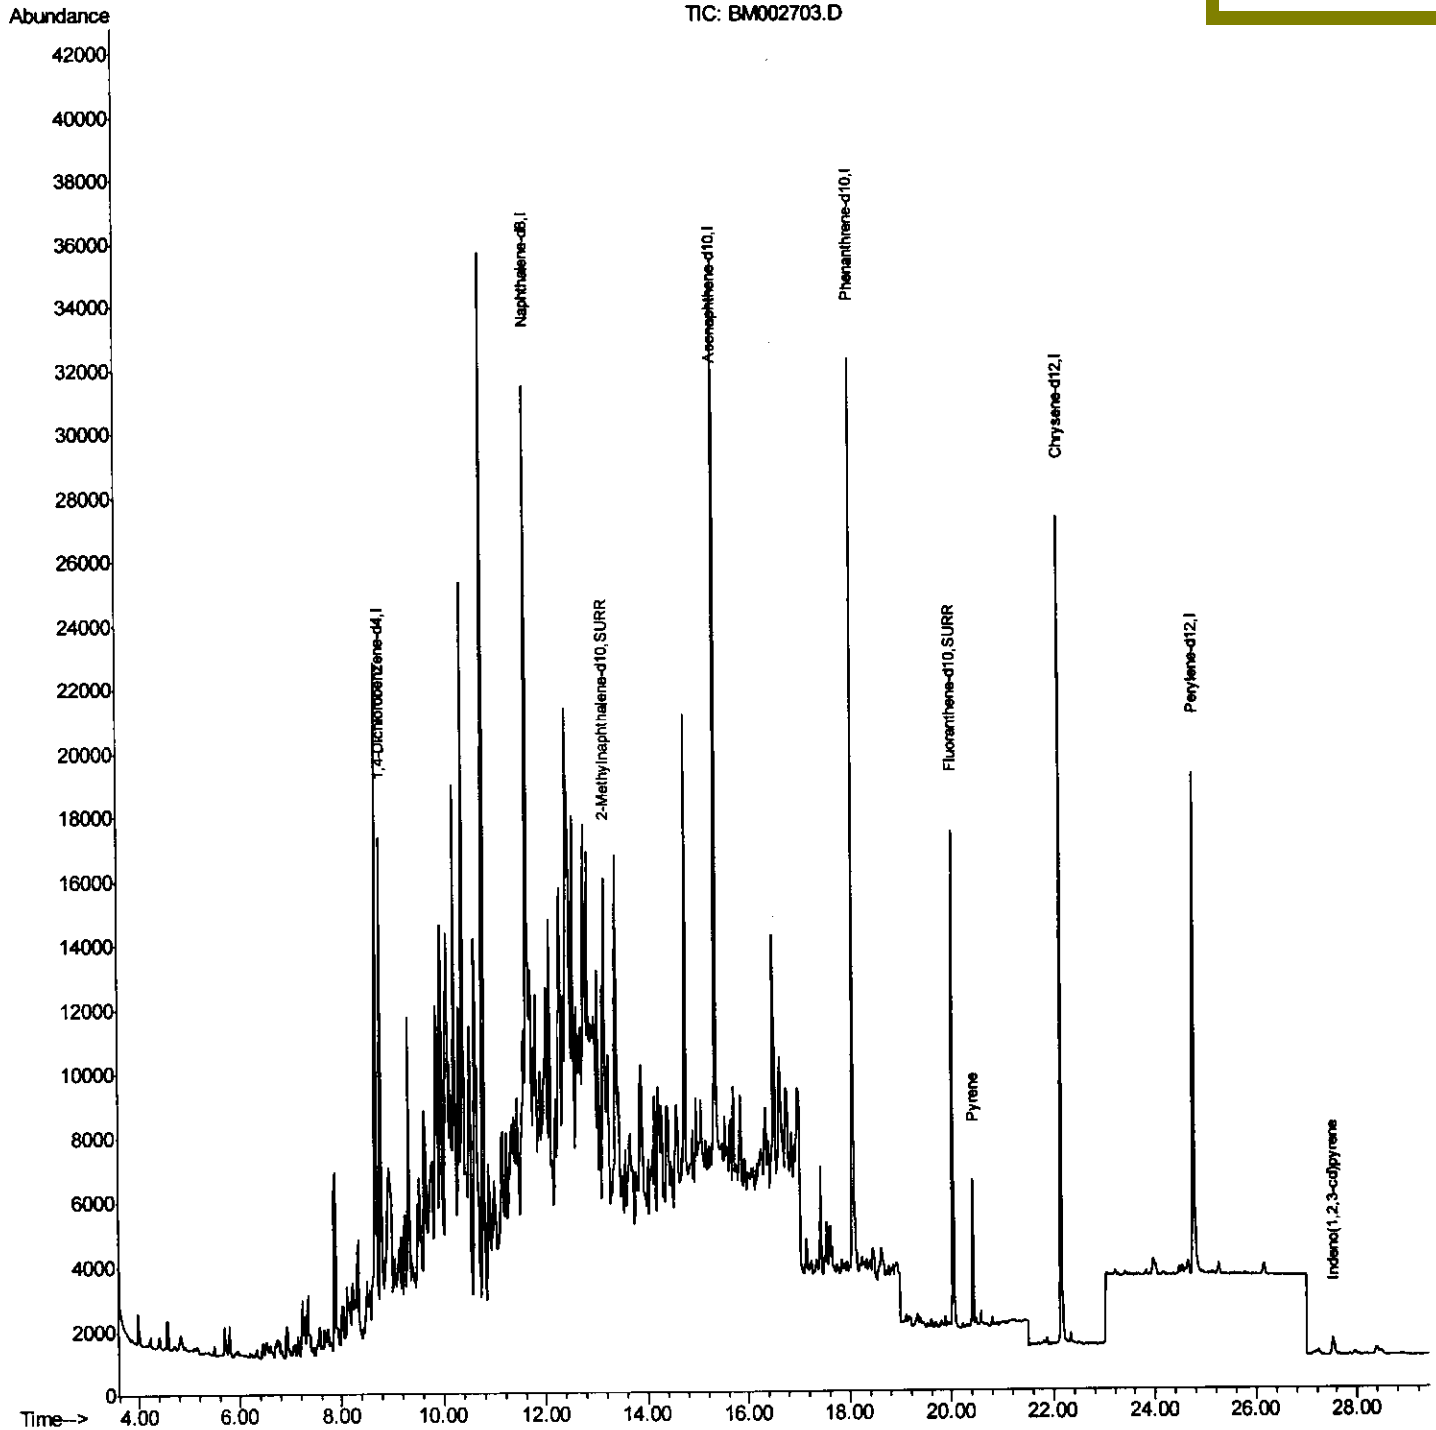

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\DATA\BM092215\
 Data File : BM002703.D
 Acq On : 22 Sep 2015 20:36
 Operator : UM/IZ
 Sample : G3741-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHAF6

Quant Time: Sep 23 03:42:12 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 03:40:59 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/23/2015 4:37:32 PM

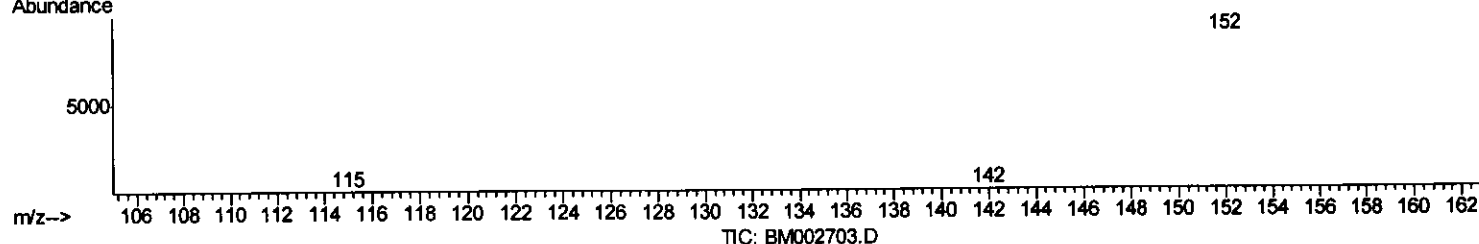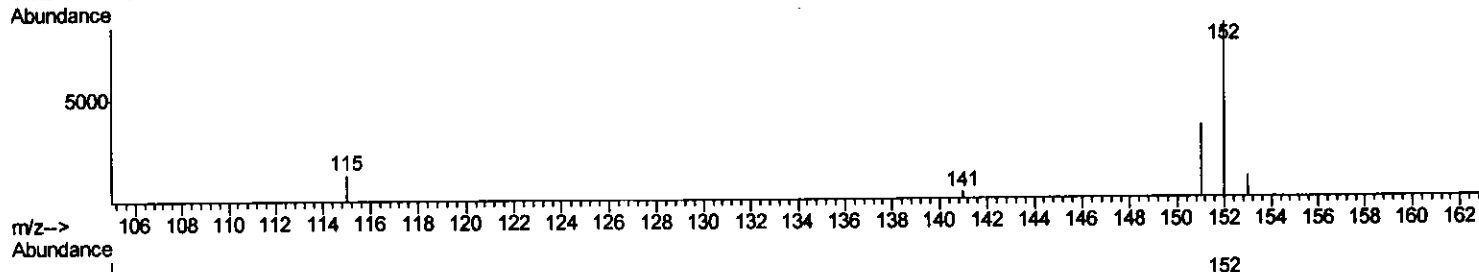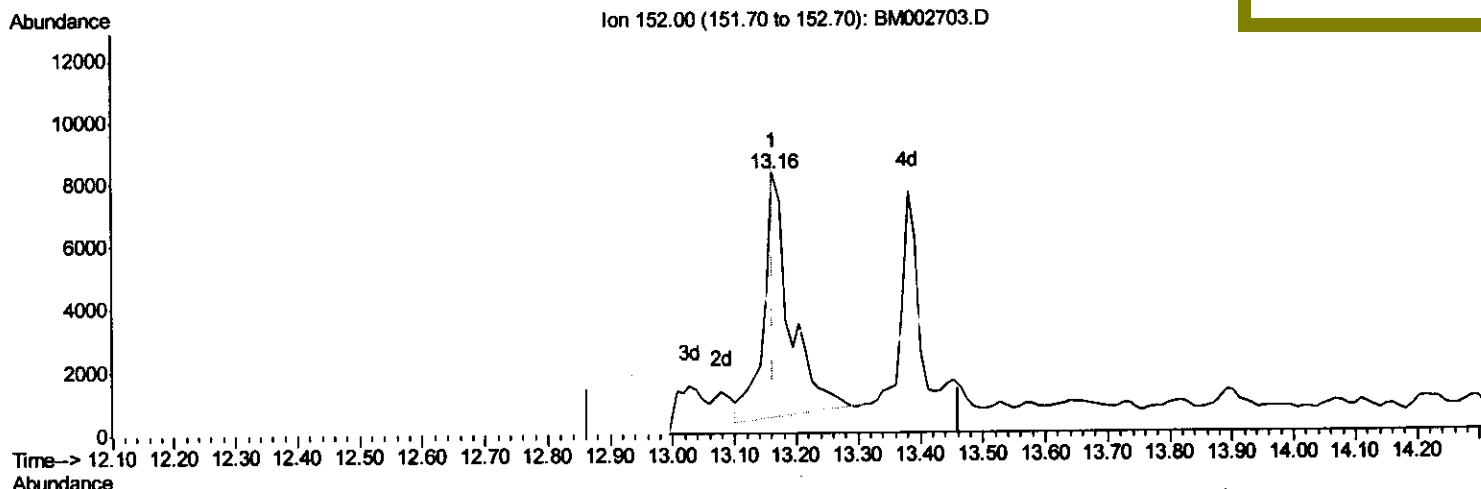

(6) 2-Methylnaphthalene-d10 (SURR)

13.162min (+0.000) 0.44ng/ul

response 22967

Ion	Exp%	Act%
152.00	100	100
151.00	18.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\bm092215\
 Data File : BM002703.D
 Acq On : 22 Sep 2015 20:36
 Operator : UM/IZ
 Sample : G3741-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHAF6

Quant Time: Sep 23 06:04:46 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 03:40:59 2015
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 9/23/2015 4:37:32 PM

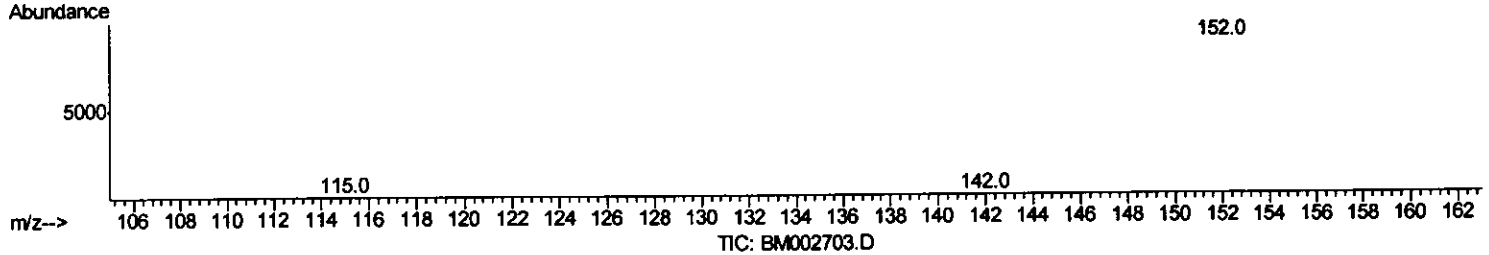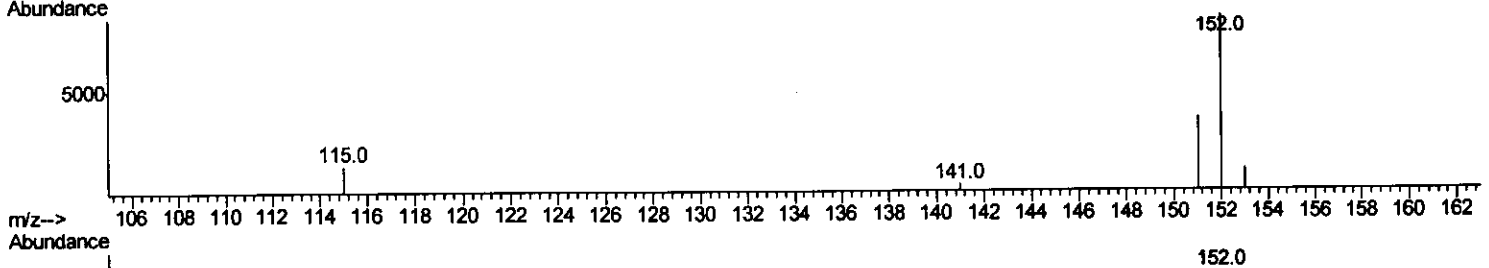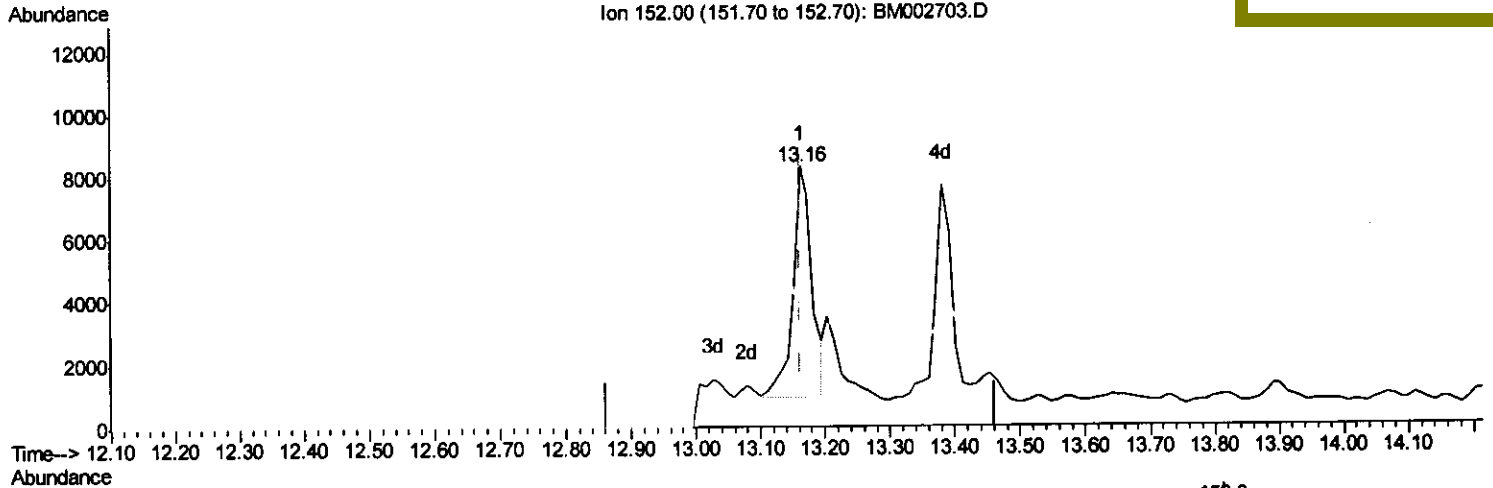

(6) 2-Methylnaphthalene-d10 (SURR)

13.162min (+0.000) 0.29ng/ul m U.M

response 15177

9/24/15

Ion	Exp%	Act%
152.00	100	100
151.00	18.90	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA M\Data\bm092215\
 Data File : BM002703.D
 Acq On : 22 Sep 2015 20:36
 Operator : UM/IZ
 Sample : G3741-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Quant Time: Sep 23 09:08:56 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 03:40:59 2015
 Response via : Initial Calibration

Instrument :
 BNA M
 ClientSampleId :
 JHAF6

Manual Integrations
 APPROVED

MMDadoda
 9/23/2015 4:37:32 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	9853	0.40	ng/ul	0.00
4) Naphthalene-d8	11.64	136	39266	0.40	ng/ul	0.00
8) Acenaphthene-d10	15.35	164	21899	0.40	ng/ul	-0.02
12) Phenanthrene-d10	18.06	188	37090	0.40	ng/ul	0.00
18) Chrysene-d12	22.15	240	28804	0.40	ng/ul	-0.01
22) Perylene-d12	24.77	264	27428	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
6) 2-Methylnaphthalene-d10	13.16	152	15177m	0.29	ng/ul	0.00
16) Fluoranthene-d10	20.03	212	18380	0.22	ng/ul	0.00
Target Compounds						
19) Pvrene	20.42	202	4991	0.05	ng/ul#	Ovalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M.
 09/24/15