

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092215\
 Data File : BM002704.D
 Acq On : 22 Sep 2015 21:12
 Operator : UM/IZ
 Sample : G3741-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHAF8

Quant Time: Sep 23 06:07:55 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM90315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 03:40:59 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.78	152	8212	0.40	ng/ul	0.00
4) Naphthalene-d8	11.64	136	29343	0.40	ng/ul	0.00
8) Acenaphthene-d10	15.36	164	13790	0.40	ng/ul	0.00
12) Phenanthrene-d10	18.06	188	28958	0.40	ng/ul	0.00
18) Chrysene-d12	22.15	240	25494	0.40	ng/ul	0.00
22) Perylene-d12	24.78	264	24258	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL	
6) 2-Methylnaphthalene-d10	13.16	152	13105	0.33	ng/ul	0.00
16) Fluoranthene-d10	20.04	212	22934	0.35	ng/ul	0.00
Target Compounds						
5) Naphthalene	11.69	128	949	0.01	ng/ul#	68
14) Phenanthrene	18.11	178	1047	0.01	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092215\
Data File : BM002704.D
Acq On : 22 Sep 2015 21:12
Operator : UM/IZ
Sample : G3741-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHAF8

Quant Time: Sep 23 06:07:55 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 03:40:59 2015
Response via : Initial Calibration

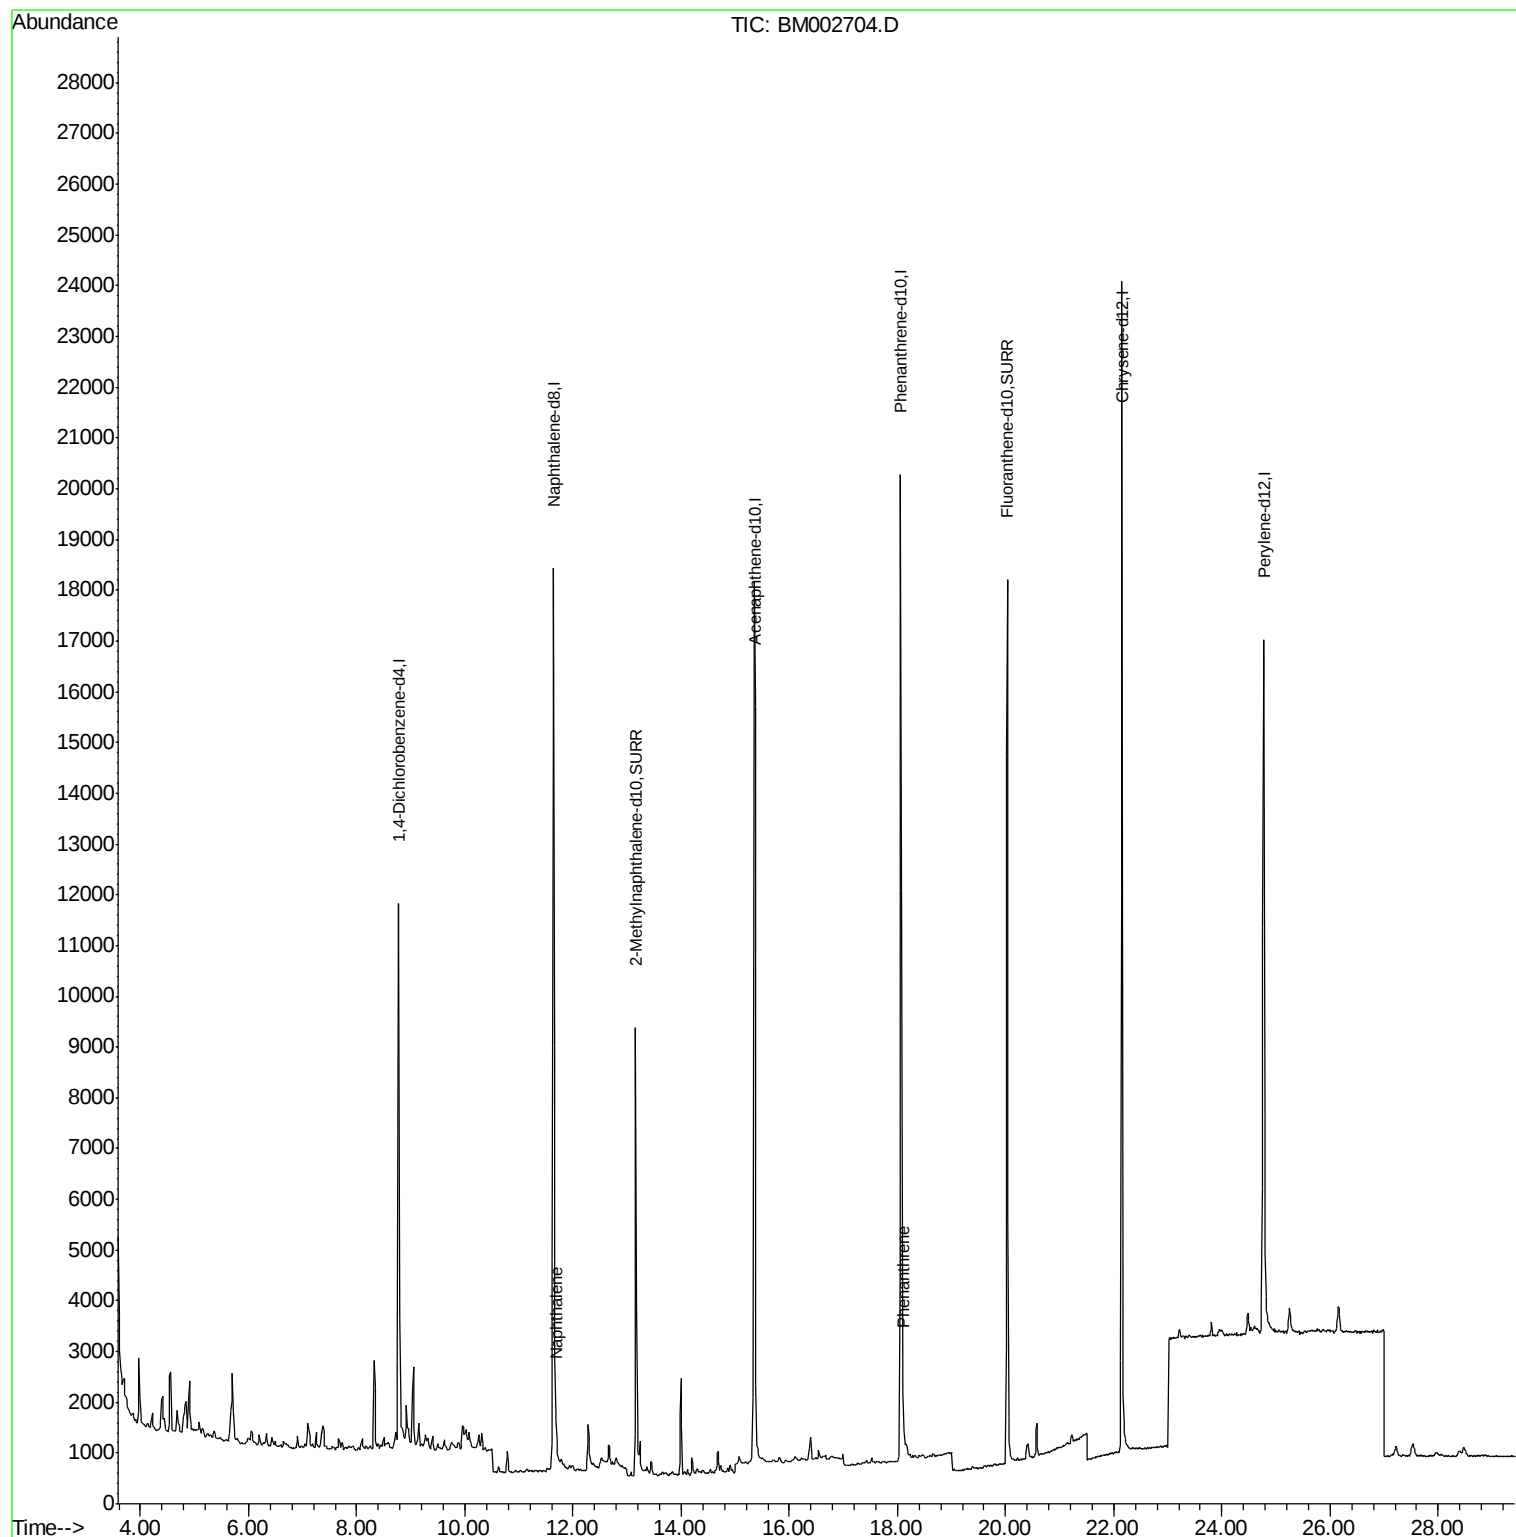

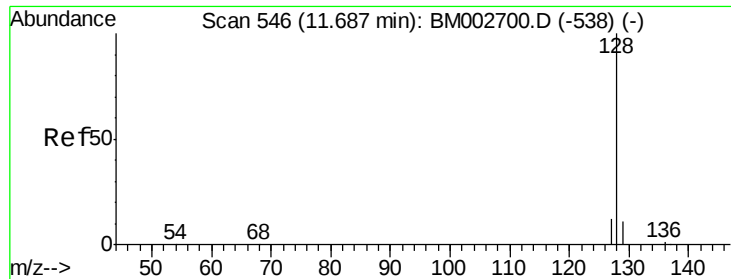

#5

Naphthalene

Concen: 0.01 ng/ul

RT: 11.69 min Scan# 546

Delta R.T. 0.00 min

Lab File: BM002704.D

Acq: 22 Sep 2015 21:12

Instrument :

BNA_M

ClientSampleId :

JHAF8


Tot Ion:128 Resp: 949

Ion Ratio Lower Upper

128 100

129 26.9 9.8 14.8#


127 24.4 10.7 16.1#

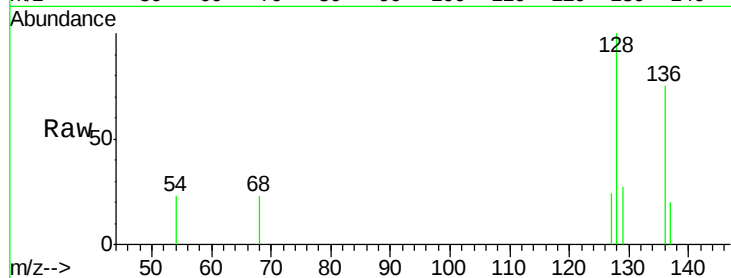



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

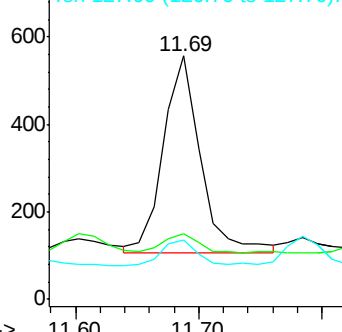

Time-->

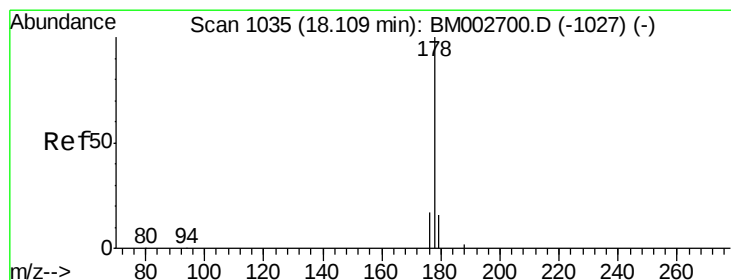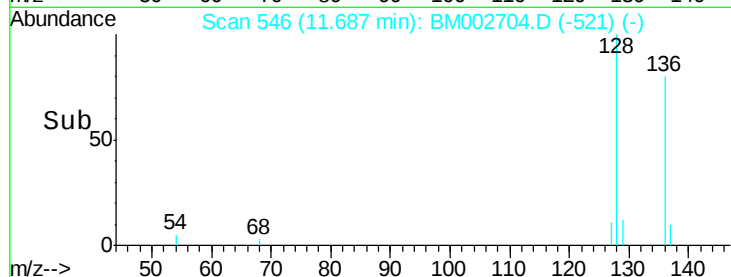

#14

Phenanthrene

Concen: 0.01 ng/ul

RT: 18.11 min Scan# 1035

Delta R.T. -0.00 min

Lab File: BM002704.D

Acq: 22 Sep 2015 21:12


Tgt Ion:178 Resp: 1047

Ion Ratio Lower Upper

178 100

176 28.9 16.2 24.4#


179 32.3 12.8 19.2#

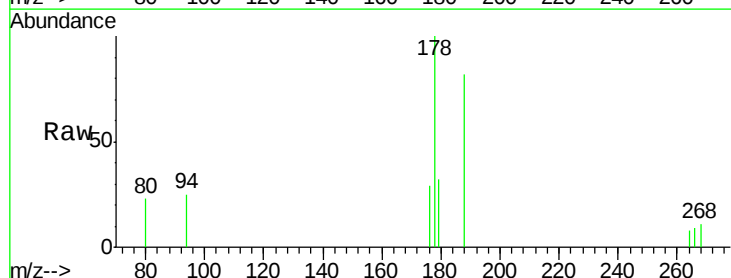

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

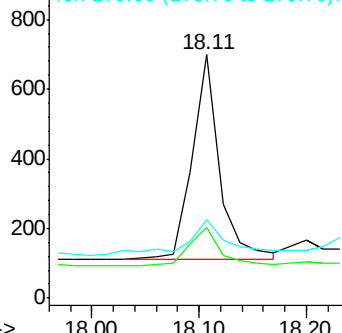

Time-->

