


Data Path : Z:\HPCHEM1\BNA M\DATA\BM092215\
Data File : BM002699.D
Acq On : 22 Sep 2015 16:52
Operator : UM/IZ
Sample : DFTPP14
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP14

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM90315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 23 03:40:59 2015

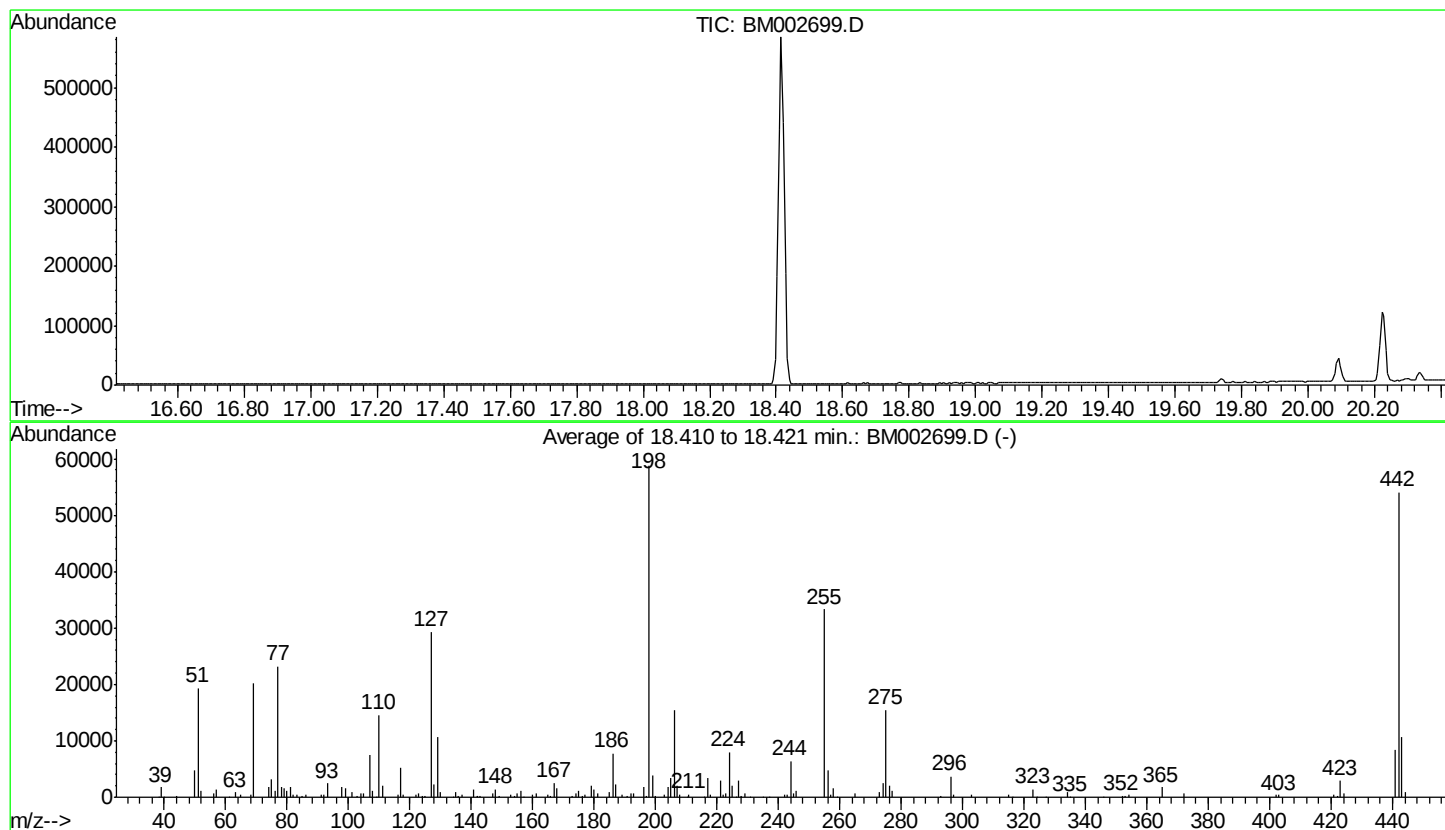

AutoFind: Scans 2605, 2606, 2607; Background Corrected with Scan 2599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	19398	PASS
68	69	0.00	2	1.8	374	PASS
69	198	0.00	100	34.4	20238	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	29293	PASS
197	198	0.00	1	0.3	153	PASS
198	198	100	100	100.0	58781	PASS
199	198	5	9	6.8	3970	PASS
275	198	10	60	26.3	15451	PASS
365	198	1	100	3.0	1773	PASS
441	443	0.01	100	79.6	8476	PASS
442	198	50	100	92.0	54093	PASS
443	442	15	24	19.7	10643	PASS

m/z	Abundance
39.90	352.0
44.00	1787.0
207.00	439.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14

m/z	Abundance
39.00	1751.0
40.00	460.0
44.00	1863.0
50.00	4933.0
51.00	20384.0
52.00	1024.0
55.90	573.0
57.00	1588.0
63.00	833.0
65.00	391.0
68.00	373.0
69.00	20752.0
74.00	2026.0
75.00	3322.0
76.00	1027.0
77.10	23592.0
78.10	1865.0
79.00	1619.0
80.00	1234.0
81.00	1653.0
82.00	368.0
83.00	420.0
85.00	394.0
85.90	526.0
91.00	453.0
91.90	401.0
93.00	2616.0
98.00	1929.0
99.00	1623.0
101.00	934.0
104.00	680.0
105.00	560.0
107.00	7458.0
108.00	1243.0
110.00	14447.0
111.00	2118.0
115.90	350.0
117.00	4941.0
117.90	378.0
121.90	512.0
123.00	779.0
123.90	323.0
127.00	28296.0
128.00	2207.0
129.00	10257.0
130.00	826.0
134.90	813.0
137.00	564.0
140.90	1353.0
141.90	458.0
143.00	315.0
147.00	669.0
148.00	1532.0
152.90	406.0
153.90	405.0
155.00	678.0
156.00	1122.0
160.00	455.0
161.00	516.0
164.90	510.0
167.00	2461.0
168.00	1476.0
172.90	317.0
173.90	499.0
175.00	1019.0
176.90	514.0
178.90	1799.0
180.00	1365.0
181.00	596.0
185.00	911.0
186.00	6754.0
187.00	2284.0
189.00	378.0
190.80	380.0
192.00	568.0
193.00	596.0
196.00	1926.0
197.90	52744.0
199.00	3866.0
202.90	355.0
204.00	1692.0
205.00	2937.0
206.00	13645.0
207.00	2344.0
207.90	552.0
211.10	495.0
217.00	3040.0
217.90	509.0
221.00	2317.0
221.80	463.0
222.90	672.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14

224.00	7153.0
225.00	1741.0
227.00	2575.0
227.80	341.0
228.90	630.0
242.00	302.0
242.90	334.0
244.00	5269.0
245.00	684.0
246.00	910.0
255.00	28096.0
256.00	4305.0
257.00	322.0
258.00	1334.0
264.90	528.0
273.00	733.0
274.00	2149.0
275.00	12647.0
276.00	1892.0
277.00	896.0
296.00	3123.0
296.90	400.0
302.90	312.0
314.90	430.0
323.00	1117.0
334.00	719.0
354.00	415.0
364.90	1342.0
372.00	634.0
401.90	390.0
421.00	308.0
423.00	2038.0
424.00	598.0
441.00	5802.0
442.00	36376.0
443.00	7315.0
444.00	765.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14

m/z	Abundance
38.00	320.0
39.00	1983.0
39.90	476.0
44.00	1964.0
50.10	5636.0
51.00	22728.0
52.00	1269.0
56.00	733.0
57.00	1576.0
61.00	352.0
63.00	1013.0
65.00	518.0
68.00	443.0
69.00	24384.0
74.00	2204.0
75.00	3633.0
76.10	1351.0
77.10	28176.0
78.00	2159.0
79.00	1791.0
80.00	1471.0
81.00	2100.0
82.00	501.0
83.00	527.0
84.90	355.0
86.00	411.0
91.00	466.0
91.90	372.0
93.00	2922.0
98.00	2029.0
99.00	2007.0
101.00	1161.0
103.00	386.0
104.00	843.0
105.00	694.0
107.00	8826.0
108.00	1529.0
109.00	315.0
110.00	17632.0
111.00	2591.0
116.00	383.0
117.00	6345.0
118.00	526.0
121.90	519.0
123.00	746.0
124.00	379.0
125.00	373.0
127.00	34968.0
128.00	2791.0
129.00	12798.0
130.00	1089.0
134.90	1071.0
135.90	401.0
137.00	575.0
140.90	1602.0
141.90	585.0
143.00	395.0
146.90	787.0
148.00	1688.0
148.90	456.0
152.90	564.0
153.90	371.0
155.00	792.0
156.00	1331.0
157.00	319.0
159.90	579.0
161.00	740.0
164.90	597.0
165.90	365.0
167.00	3198.0
168.00	1761.0
173.00	425.0
174.00	696.0
175.00	1267.0
176.00	492.0
176.90	582.0
179.00	2280.0
180.00	1590.0
181.00	733.0
185.00	1220.0
186.00	9175.0
187.00	2703.0
188.90	512.0
192.00	778.0
193.00	909.0
196.00	2173.0
197.00	461.0
197.90	71352.0
198.90	4531.0
199.90	403.0
202.90	461.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14

204.00	2322.0
205.00	4109.0
206.00	17880.0
207.00	2812.0
208.00	625.0
210.20	308.0
210.90	693.0
215.90	323.0
217.00	4139.0
218.00	478.0
221.00	3620.0
221.80	617.0
222.90	887.0
224.00	9474.0
225.00	2349.0
226.00	316.0
227.00	3789.0
228.00	577.0
229.00	767.0
230.90	343.0
235.00	324.0
237.00	341.0
242.00	587.0
243.00	486.0
244.00	7999.0
245.00	1011.0
245.90	1468.0
255.00	39672.0
256.00	5691.0
257.00	478.0
257.90	2041.0
259.00	300.0
265.00	817.0
273.00	1185.0
274.00	3031.0
275.00	18536.0
276.00	2586.0
277.00	1308.0
292.80	386.0
296.00	4285.0
297.00	668.0
302.90	548.0
314.90	511.0
316.00	349.0
323.00	1598.0
324.10	340.0
326.90	306.0
334.00	1114.0
335.00	324.0
345.90	318.0
351.90	507.0
353.00	316.0
354.00	439.0
365.00	2022.0
372.00	776.0
402.00	374.0
403.00	547.0
421.00	422.0
422.00	464.0
423.00	3432.0
423.90	872.0
441.00	10182.0
442.00	63952.0
443.00	12716.0
444.00	1240.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14

m/z	Abundance
39.00	1414.0
39.90	414.0
44.00	1955.0
50.00	3451.0
51.00	15082.0
52.00	810.0
55.90	495.0
57.00	1057.0
63.00	578.0
65.10	387.0
68.00	306.0
69.00	15580.0
74.00	1419.0
75.00	2621.0
76.10	826.0
77.00	17848.0
78.00	1377.0
79.00	1252.0
79.90	1003.0
81.00	1455.0
81.90	383.0
83.00	349.0
85.90	363.0
91.00	334.0
91.90	351.0
93.00	1853.0
98.00	1468.0
99.00	1413.0
101.00	792.0
103.90	626.0
105.00	566.0
107.00	6004.0
108.00	959.0
110.00	11704.0
111.00	1779.0
116.00	314.0
117.00	4139.0
118.00	370.0
121.90	379.0
123.00	574.0
127.00	24616.0
128.00	2022.0
129.00	9216.0
129.90	769.0
133.90	347.0
135.00	797.0
135.90	342.0
136.90	436.0
140.90	1101.0
142.10	419.0
147.00	597.0
147.90	1131.0
152.90	341.0
155.00	739.0
156.00	1002.0
160.10	338.0
160.90	564.0
164.90	554.0
165.90	307.0
167.00	1955.0
168.00	1226.0
173.90	549.0
175.00	957.0
177.00	403.0
179.00	1779.0
180.00	1258.0
181.00	642.0
184.90	814.0
186.00	7304.0
187.00	1805.0
188.90	438.0
191.90	562.0
192.90	675.0
195.90	1563.0
197.90	52248.0
198.90	3513.0
202.90	390.0
203.90	1714.0
205.00	3173.0
206.00	14474.0
207.00	2302.0
207.90	491.0
210.90	488.0
216.90	2970.0
217.80	372.0
221.00	2655.0
222.90	654.0
224.00	7205.0
225.00	1925.0
227.00	2671.0
228.90	594.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14

241.90	364.0
243.00	456.0
244.00	5814.0
244.90	705.0
245.90	1157.0
255.00	32216.0
256.00	4658.0
256.90	370.0
258.00	1623.0
264.90	598.0
272.90	978.0
274.00	2431.0
275.00	15171.0
276.00	1890.0
277.00	1284.0
296.00	3633.0
296.90	477.0
303.00	443.0
314.90	426.0
323.00	1425.0
334.00	842.0
352.00	421.0
352.90	355.0
354.00	458.0
365.00	1955.0
372.00	878.0
401.80	359.0
403.00	592.0
420.90	526.0
422.10	427.0
423.00	3244.0
424.00	658.0
441.00	9444.0
442.00	61952.0
443.00	11898.0
444.00	843.0

Instrument :
BNA_M
ClientSampleId :
DFTPP14