

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
 Data File : BM007516.D
 Acq On : 22 Sep 2016 18:04
 Operator : UM/SJ
 Sample : H4830-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VH4

Quant Time: Sep 23 04:01:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 23 04:00:23 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	1381	0.40	ng/ul	0.00
2) Naphthalene-d8	10.57	136	5619	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.42	164	3985	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	674230	0.40	ng/ul	0.10
16) Chrysene-d12	21.35	240	8853	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	642373	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	2835	0.43	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	8957	0.01	ng/ul	0.00
Target Compounds						
						Qvalue
9) Fluorene	15.41	166	1208	0.07	ng/ul#	16
17) Pyrene	19.56	202	1634	0.06	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
 Data File : BM007516.D
 Acq On : 22 Sep 2016 18:04
 Operator : UM/SJ
 Sample : H4830-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VH4

Quant Time: Sep 23 04:01:59 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 23 04:00:23 2016
 Response via : Initial Calibration




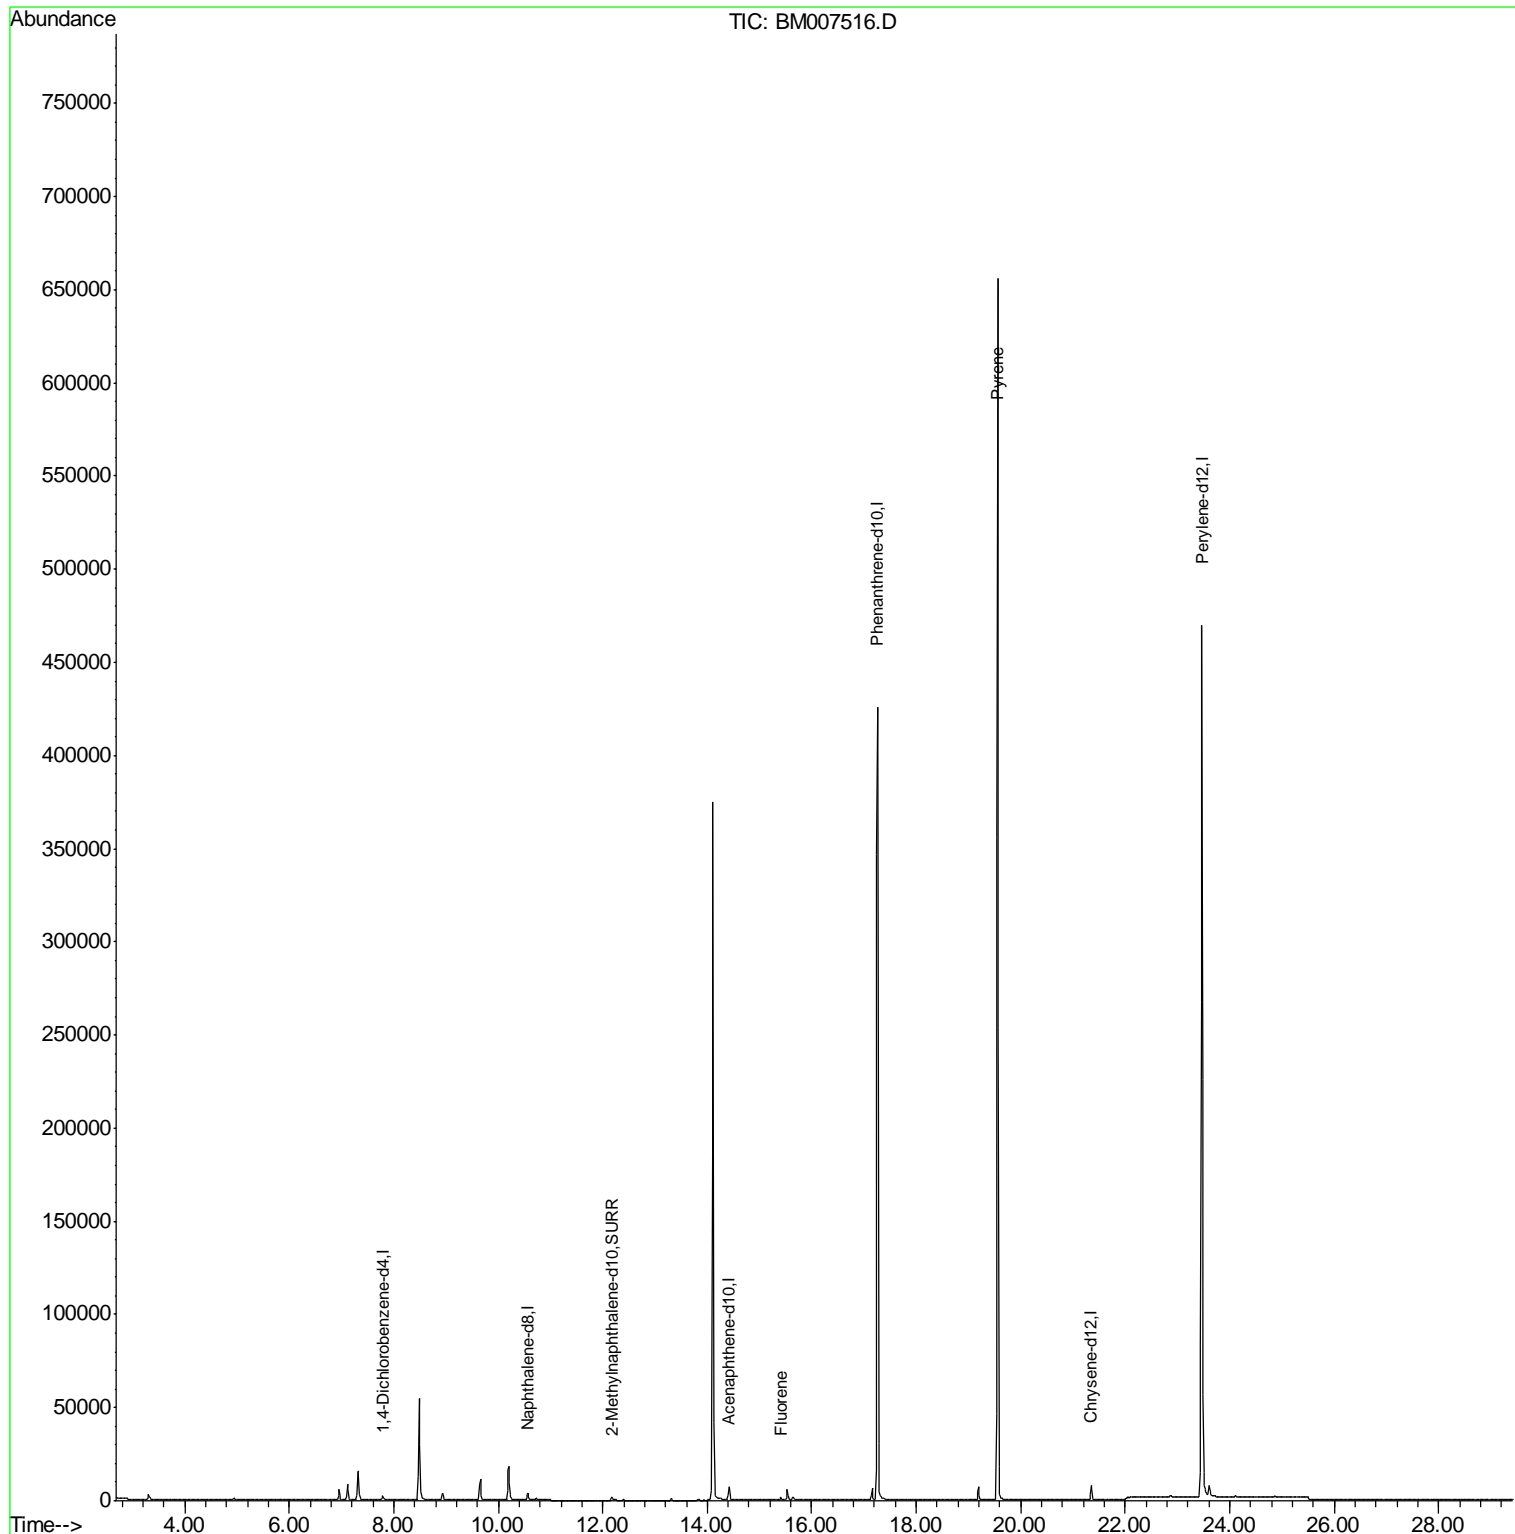


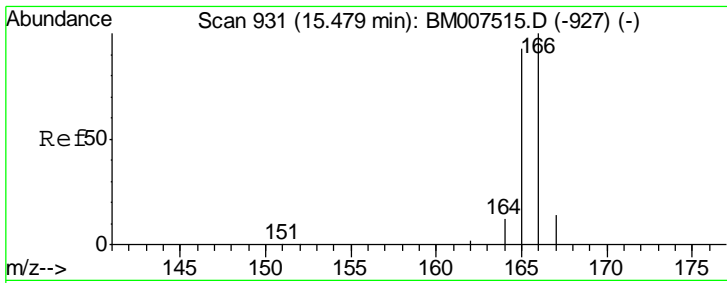

#9
 Fluorene
 Concen: 0.07 ng/ul
 RT: 15.41 min Scan# 927
 Delta R.T. -0.07 min
 Lab File: BM007516.D
 Acq: 22 Sep 2016 18:04

Instrument :
 BNA_M
 ClientSampleID :
 A4VH4

Tgt Ion	Resp	Lower	Upper
166	1208		
165	10.2	79.8	119.8#
167	32.9	11.5	17.3#

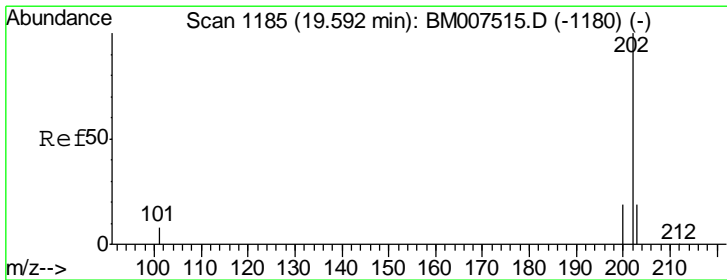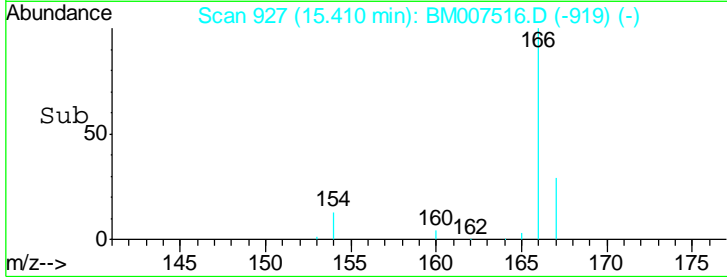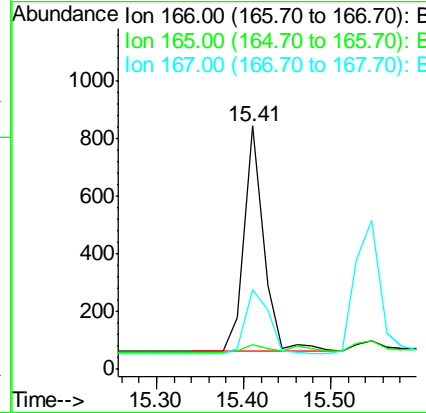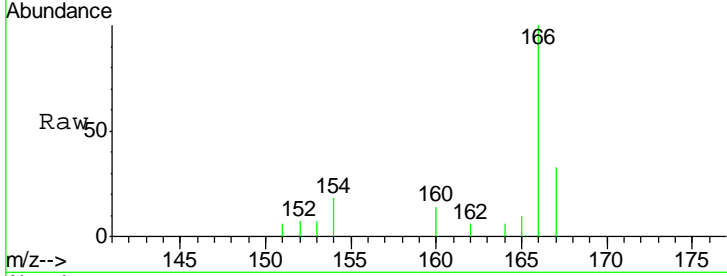

#17
 Pyrene
 Concen: 0.06 ng/ul
 RT: 19.56 min Scan# 1182
 Delta R.T. -0.04 min
 Lab File: BM007516.D
 Acq: 22 Sep 2016 18:04

Tgt Ion	Resp	Lower	Upper
202	1634		
200	8.5	15.9	23.9#
203	185.4	15.0	22.4#

