

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
 Data File : BM007519.D
 Acq On : 22 Sep 2016 19:52
 Operator : UM/SJ
 Sample : H4830-15
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4VI3

Quant Time: Sep 23 04:02:26 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 23 04:00:23 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	1378	0.40	ng/ul	0.00
2) Naphthalene-d8	10.57	136	5538	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.42	164	3950	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.26	188	619783	0.40	ng/ul	0.10
16) Chrysene-d12	21.35	240	8678	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	572222	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	2723	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	8206	0.01	ng/ul	0.00
Target Compounds						
9) Fluorene	15.41	166	1149	0.07	ng/ul#	16
17) Pyrene	19.56	202	2087	0.07	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007519.D
Acq On : 22 Sep 2016 19:52
Operator : UM/SJ
Sample : H4830-15
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4VI3

Quant Time: Sep 23 04:02:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 23 04:00:23 2016
Response via : Initial Calibration

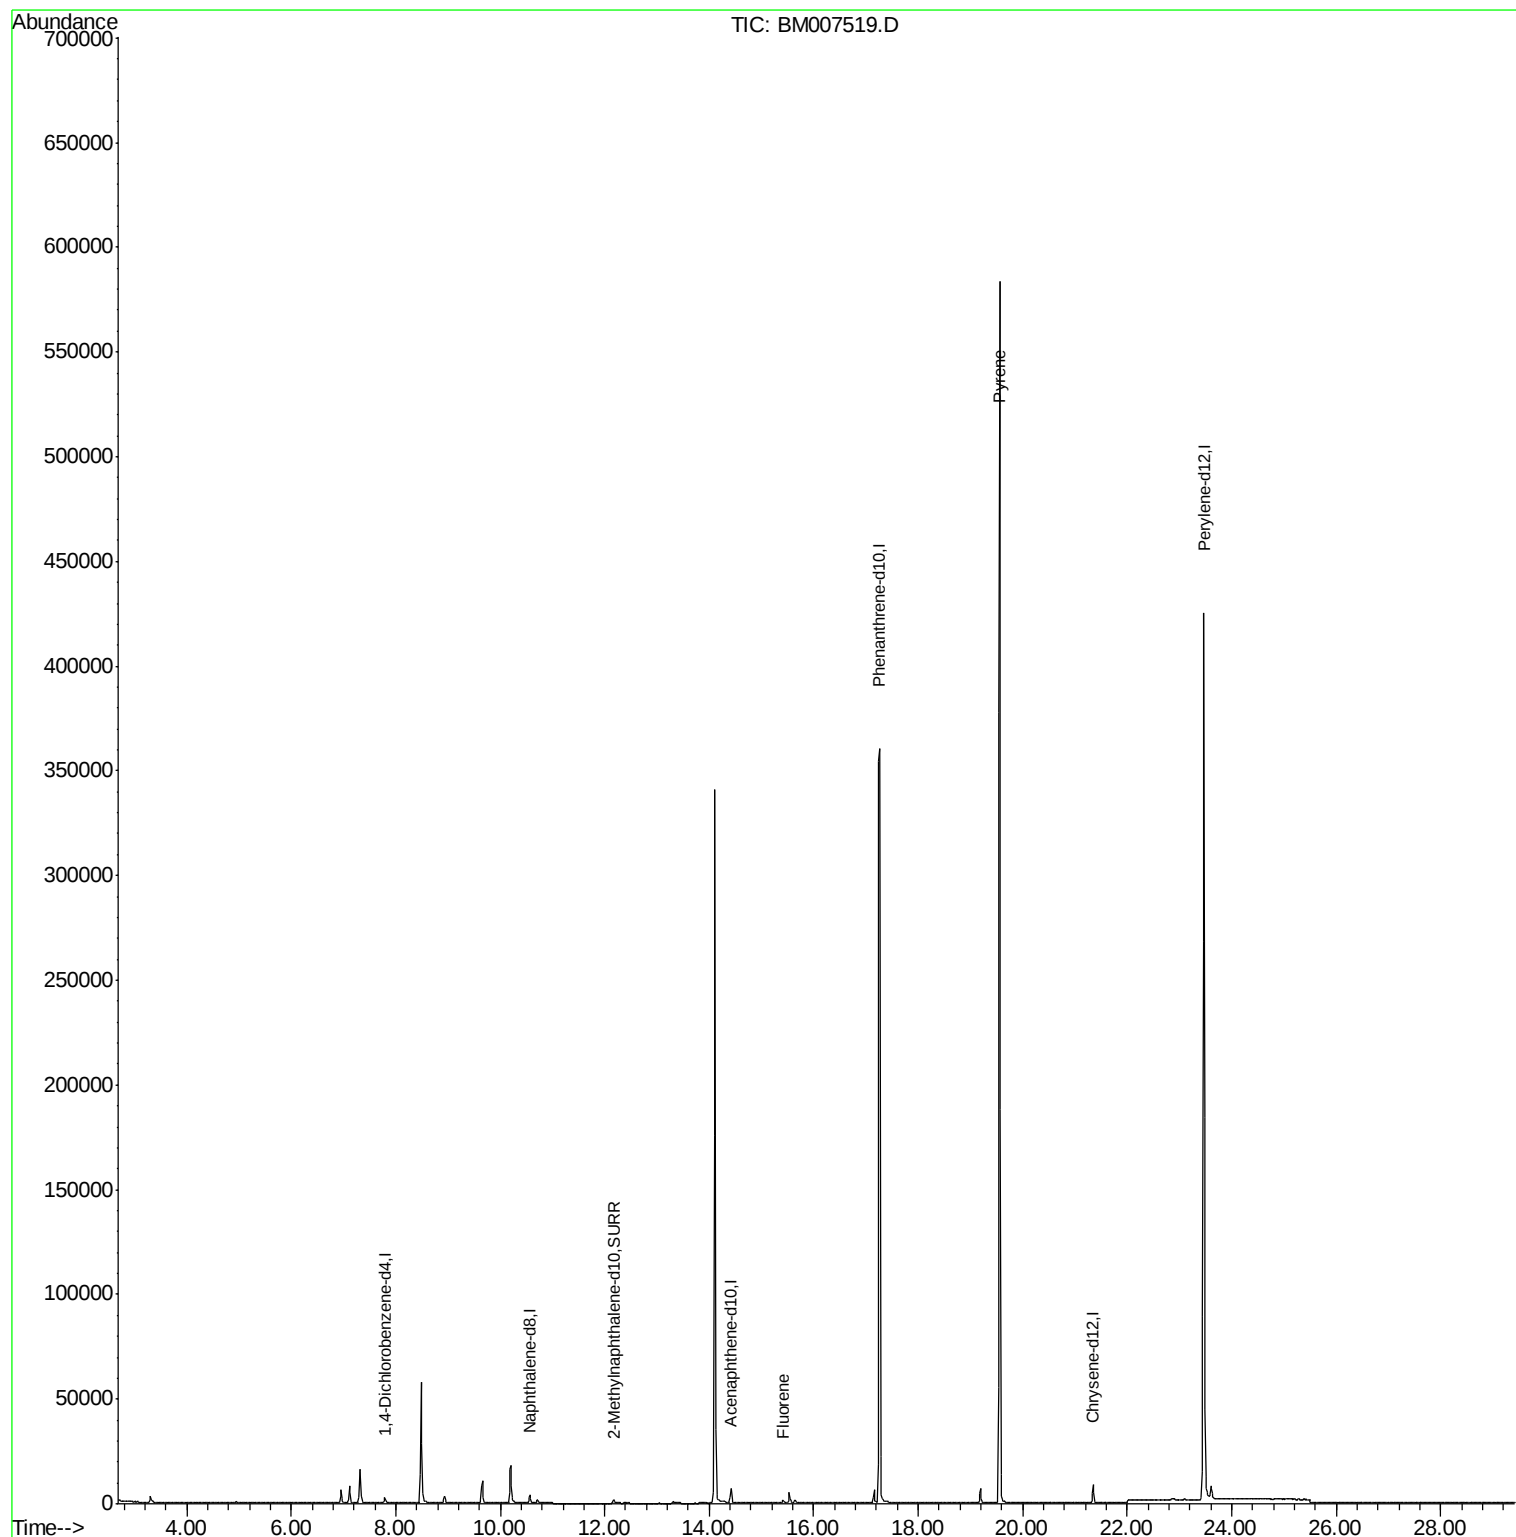


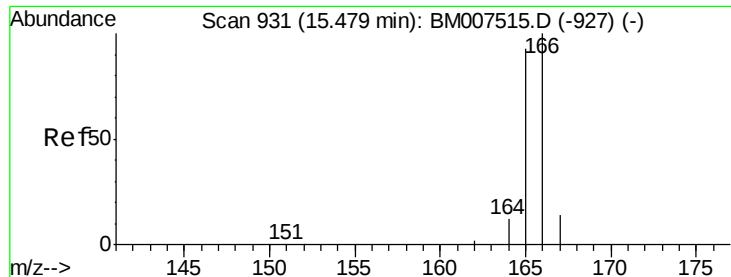




#9
Fluorene
 Concen: 0.07 ng/ul
 RT: 15.41 min Scan# 927
 Delta R.T. -0.07 min
 Lab File: BM007519.D
 Acq: 22 Sep 2016 19:52

Instrument :
 BNA_M
 ClientSampleId :
 A4VI3

Tgt Ion:166 Resp: 1149
 Ion Ratio Lower Upper
 166 100
 165 10.9 79.8 119.8#
 167 33.8 11.5 17.3#

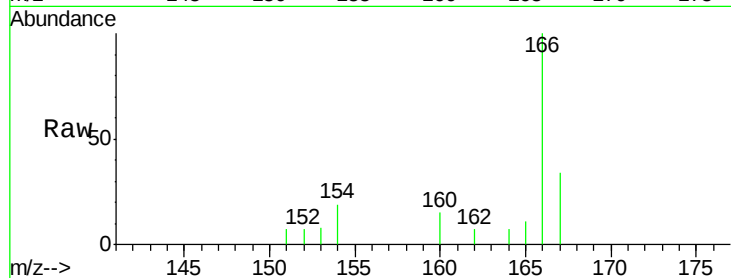


Abundance Ion 166.00 (165.70 to 166.70): E
 Ion 165.00 (164.70 to 165.70): E
 Ion 167.00 (166.70 to 167.70): E

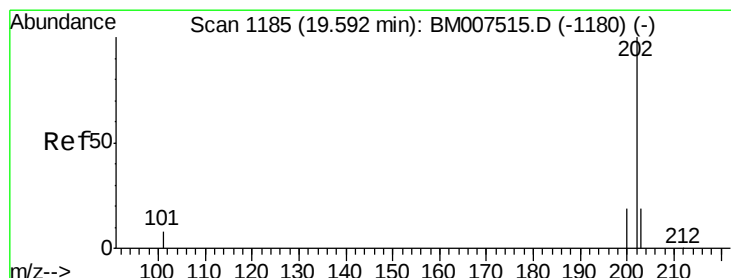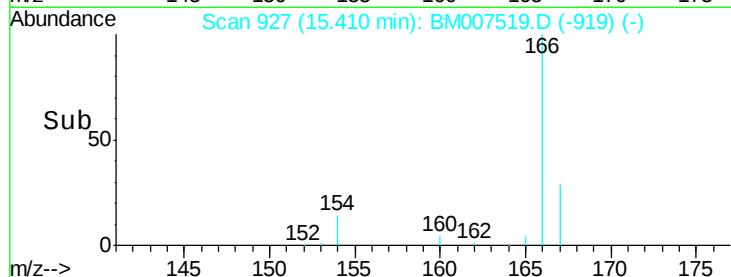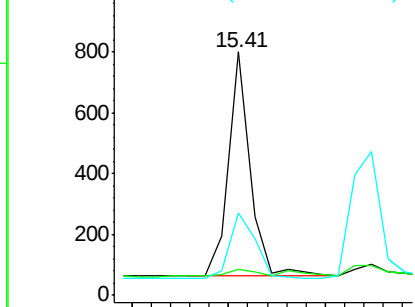

#17
Pyrene
 Concen: 0.07 ng/ul
 RT: 19.56 min Scan# 1182
 Delta R.T. -0.04 min
 Lab File: BM007519.D
 Acq: 22 Sep 2016 19:52

Tgt Ion:202 Resp: 2087
 Ion Ratio Lower Upper
 202 100
 200 9.6 15.9 23.9#
 203 195.4 15.0 22.4#

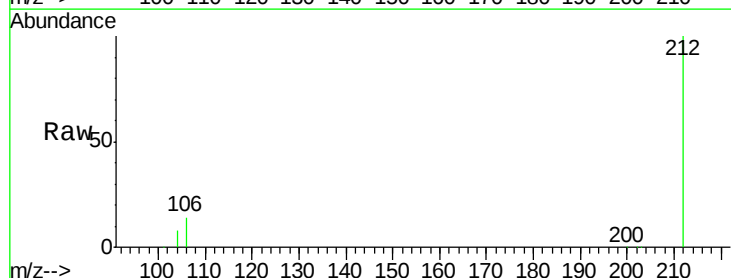

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 200.00 (199.70 to 200.70): E
 Ion 203.00 (202.70 to 203.70): E

