




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007505.D
Acq On : 22 Sep 2016 09:57
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTD0.440

Manual Integrations
APPROVED

umangi
9/23/2016 6:52:06 PM

Quant Time: Sep 22 16:12:09 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 01:26:49 2016
Response via : Initial Calibration

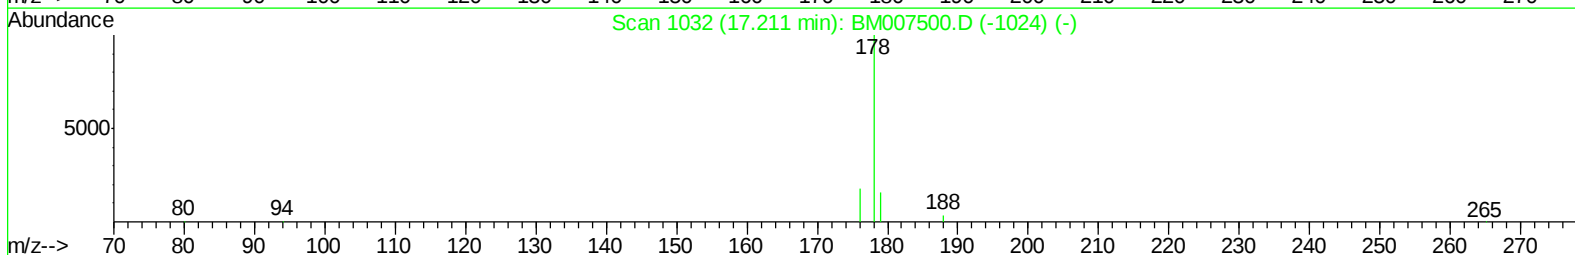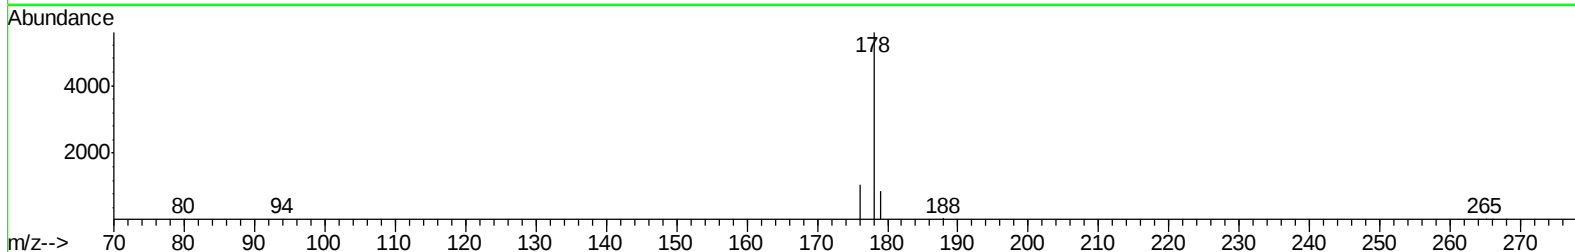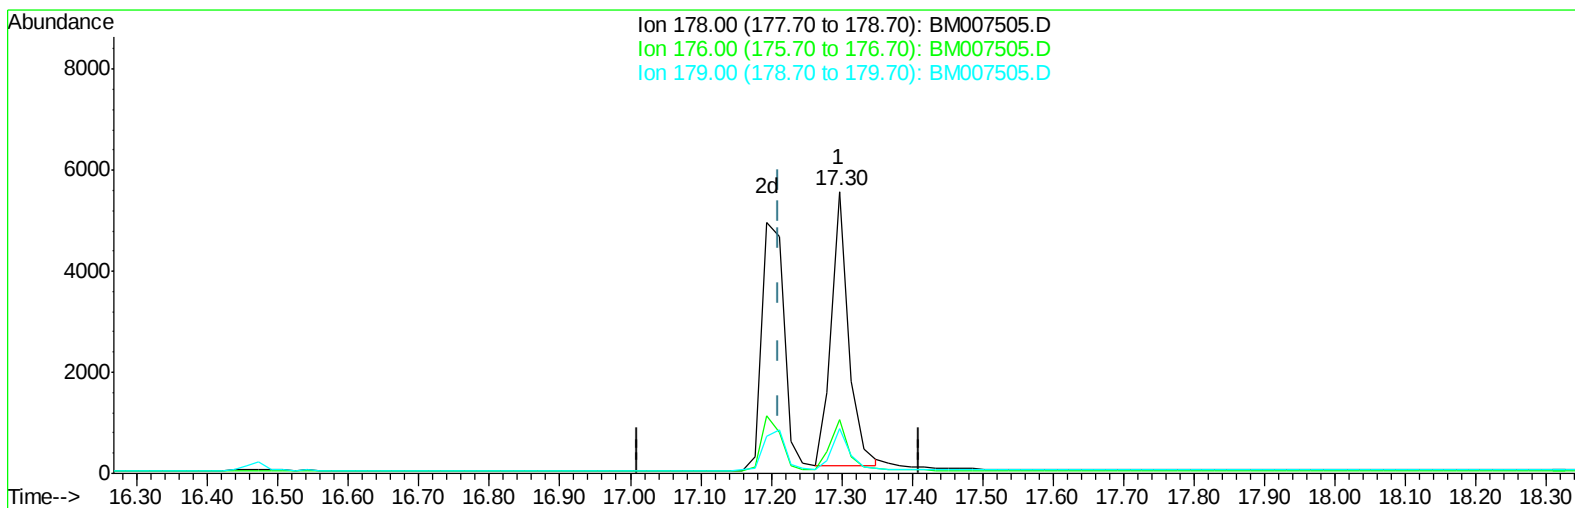

TIC: BM007505.D

(12) Phenanthrene

17.297min (+0.086) 0.33ng/ul

response 9240

Ion	Exp%	Act%
178.00	100	100
176.00	18.60	18.95
179.00	17.10	16.11
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007505.D
Acq On : 22 Sep 2016 09:57
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTD0.440

Manual Integrations
APPROVED

umangi
9/23/2016 6:52:06 PM

Quant Time: Sep 22 17:26:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 01:26:49 2016
Response via : Initial Calibration

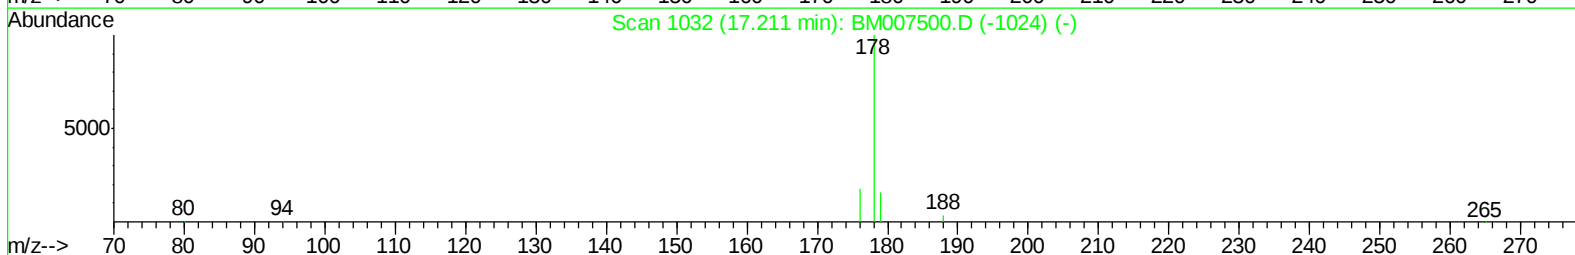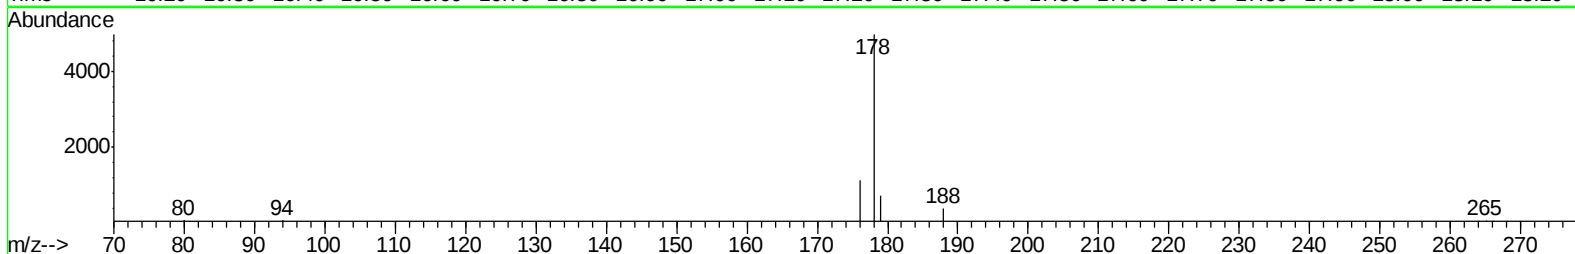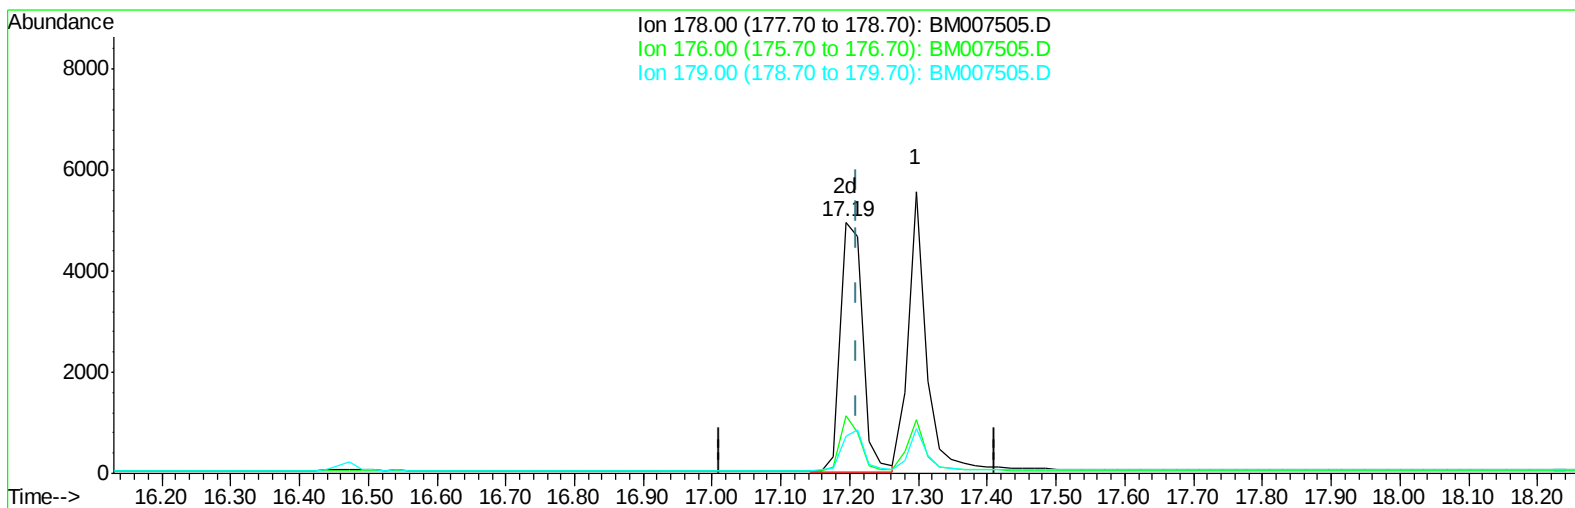

TIC: BM007505.D

(12) Phenanthrene

17.194min (-0.017) 0.40ng/ul m

response 11141

Ion	Exp%	Act%
178.00	100	100
176.00	18.60	22.87#
179.00	17.10	14.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
 Data File : BM007505.D
 Acq On : 22 Sep 2016 09:57
 Operator : UM/SJ
 Sample : SSTDC00.4
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTD0.440

Manual Integrations
 APPROVED

umangi
 9/23/2016 6:52:06 PM

Quant Time: Sep 22 17:26:51 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 01:26:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	1696	0.40	ng/ul	0.00
2) Naphthalene-d8	10.58	136	6516	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.42	164	3934	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.16	188	10346	0.40	ng/ul	0.00
16) Chrysene-d12	21.35	240	10422	0.40	ng/ul	0.00
20) Perylene-d12	23.62	264	9246	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.17	152	3003	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	9351	0.39	ng/ul	0.00
Target Compounds						Qvalue
3) Naphthalene	10.62	128	6067	0.40	ng/ul	97
5) 2-Methylnaphthalene	12.25	142	4094	0.40	ng/ul	99
7) Acenaphthylene	14.14	152	6425	0.39	ng/ul	98
8) Acenaphthene	14.49	153	5158	0.40	ng/ul	98
9) Fluorene	15.48	166	6335	0.40	ng/ul	93
11) Pentachlorophenol	16.83	266	1035	0.37	ng/ul	97
12) Phenanthrene	17.19	178	11141m	0.40	ng/ul	
13) Anthracene	17.30	178	9818	0.39	ng/ul	97
15) Fluoranthene	19.22	202	13808	0.39	ng/ul	91
17) Pyrene	19.58	202	14862	0.43	ng/ul	94
18) Benzo(a)anthracene	21.33	228	12608	0.41	ng/ul	94
19) Chrysene	21.38	228	13329	0.41	ng/ul	99
21) Benzo(b)fluoranthene	22.93	252	13232	0.43	ng/ul	99
22) Benzo(k)fluoranthene	22.97	252	12301	0.39	ng/ul	100
23) Benzo(a)pyrene	23.51	252	11585	0.40	ng/ul	100
24) Indeno(1,2,3-cd)pyrene	25.91	276	11562	0.39	ng/ul	99
25) Dibenzo(a,h)anthracene	25.92	278	8746	0.39	ng/ul	100
26) Benzo(g,h,i)perylene	26.61	276	10501	0.40	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007505.D
Acq On : 22 Sep 2016 09:57
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTD0.440

Manual Integrations
APPROVED

umangi
9/23/2016 6:52:06 PM

Quant Time: Sep 22 17:26:51 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 01:26:49 2016
Response via : Initial Calibration

