




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007506.D
Acq On : 22 Sep 2016 10:33
Operator : UM/SJ
Sample : PB93452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK52

Manual Integrations
APPROVED

umangi
9/23/2016 6:52:04 PM

Quant Time: Sep 22 16:14:39 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 01:26:49 2016
Response via : Initial Calibration

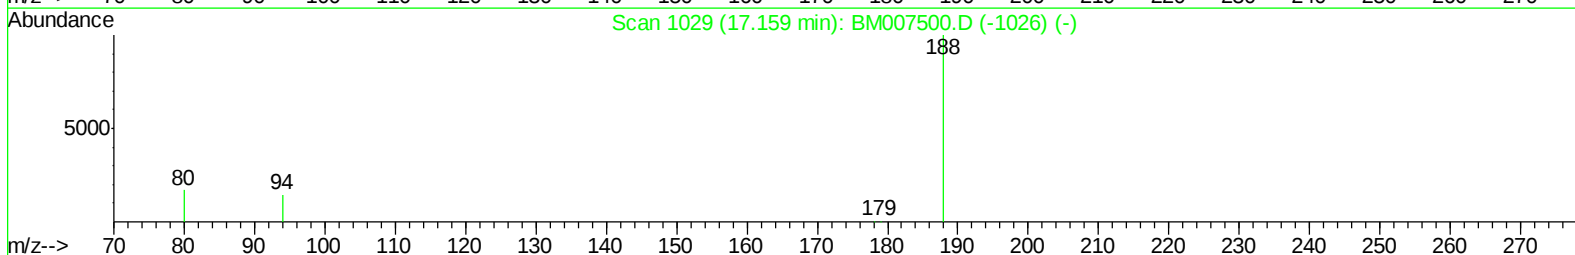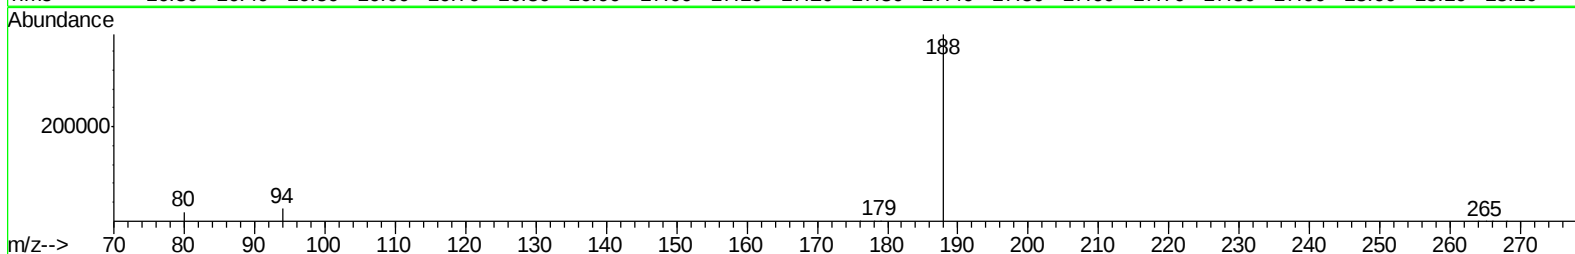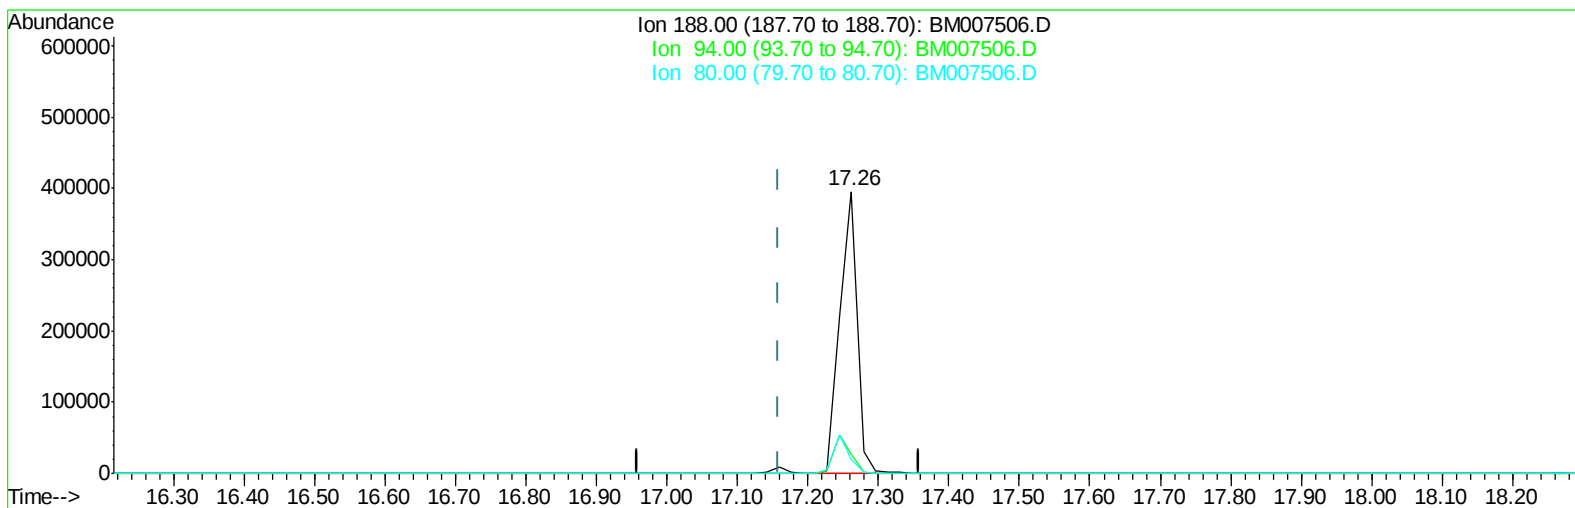

TIC: BM007506.D

(10) Phenanthrene-d10 (I)

17.262min (+0.103) 0.40ng/ul

response 673401

Ion	Exp%	Act%
188.00	100	100
94.00	15.90	6.82#
80.00	18.30	5.13#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007506.D
Acq On : 22 Sep 2016 10:33
Operator : UM/SJ
Sample : PB93452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK52

Manual Integrations
APPROVED

umangi
9/23/2016 6:52:04 PM

Quant Time: Sep 22 16:08:35 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 01:26:49 2016
Response via : Initial Calibration

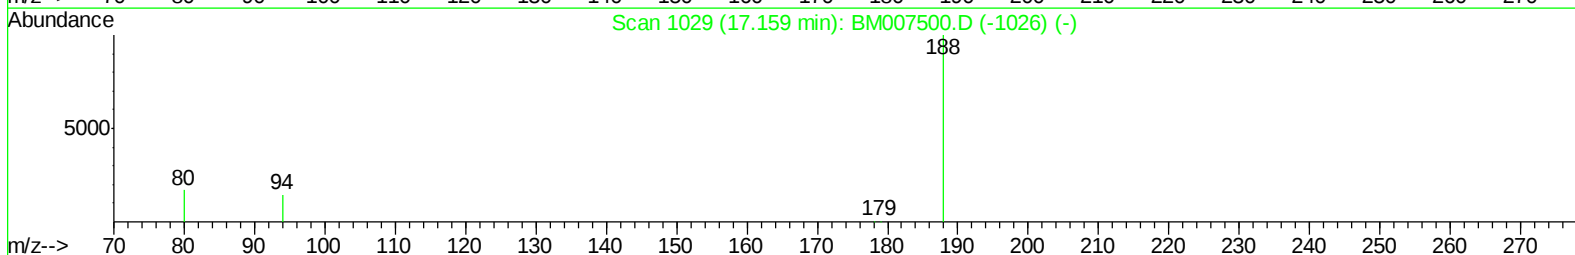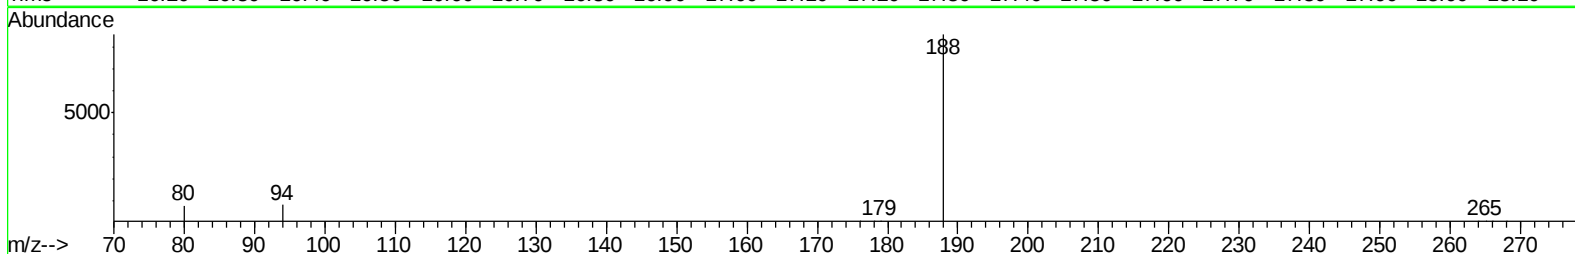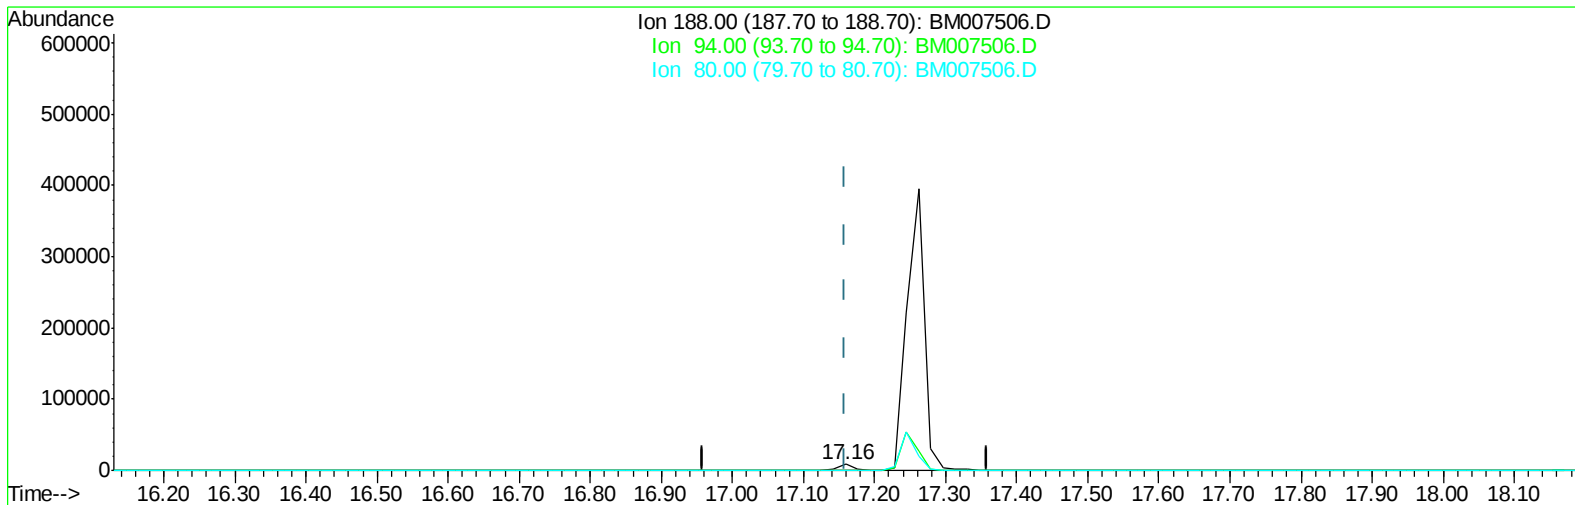

TIC: BM007506.D

(10) Phenanthrene-d10 (I)

17.159min (-0.000) 0.40ng/ul m

response 12416

Ion	Exp%	Act%
188.00	100	100
94.00	15.90	9.14#
80.00	18.30	9.02#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
 Data File : BM007506.D
 Acq On : 22 Sep 2016 10:33
 Operator : UM/SJ
 Sample : PB93452BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK52

Manual Integrations
 APPROVED

umangi
 9/23/2016 6:52:04 PM

Quant Time: Sep 22 17:31:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 22 01:26:49 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	2026	0.40	ng/ul	0.00
2) Naphthalene-d8	10.57	136	8492	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.42	164	5213	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.16	188	12416m	0.40	ng/ul	0.00
16) Chrysene-d12	21.36	240	12641	0.40	ng/ul	0.01
20) Perylene-d12	23.61	264	15113	0.40	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.17	152	3180	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.19	212	8633	0.30	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092216\
Data File : BM007506.D
Acq On : 22 Sep 2016 10:33
Operator : UM/SJ
Sample : PB93452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK52

Manual Integrations
APPROVED

umangi
9/23/2016 6:52:04 PM

Quant Time: Sep 22 17:31:18 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM092116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 22 01:26:49 2016
Response via : Initial Calibration

