

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
 Data File : BM007543.D
 Acq On : 24 Sep 2016 03:01
 Operator : UM/SJ
 Sample : H4855-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H9014

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.957	737	743	753	rVB	166675	286997	3.21%	0.362%
2	7.116	763	770	779	rBV	590414	947872	10.59%	1.194%
3	7.316	797	804	816	rBV	650695	1072467	11.99%	1.351%
4	7.781	876	883	896	rBV	1024995	1694937	18.94%	2.135%
5	8.487	997	1003	1015	rBV	551745	935019	10.45%	1.178%
6	8.934	1072	1079	1094	rBV	828500	1430395	15.99%	1.802%
7	9.651	1194	1201	1213	rBV	732079	1256748	14.04%	1.583%
8	10.192	1286	1293	1315	rBV	896885	1785691	19.96%	2.250%
9	10.563	1348	1356	1366	rBV	1645700	2762019	30.87%	3.480%
10	10.710	1375	1381	1397	rBV2	120208	265306	2.96%	0.334%
11	13.827	1903	1911	1922	rBV	2512969	3716693	41.54%	4.682%
12	14.104	1951	1958	1973	rBV	2681453	3974889	44.42%	5.008%
13	14.416	2003	2011	2017	rBV2	2801269	4475080	50.01%	5.638%
14	14.469	2017	2020	2039	rVV	225634	357453	3.99%	0.450%
15	14.633	2042	2048	2064	rBV2	133736	356877	3.99%	0.450%
16	15.410	2171	2180	2191	rBV	3612720	5441778	60.81%	6.856%
17	15.533	2195	2201	2216	rBV	1318903	1998880	22.34%	2.518%
18	17.157	2470	2477	2486	rBV	4313116	6167687	68.93%	7.770%
19	17.257	2487	2494	2506	rVV	4428661	6403328	71.56%	8.067%
20	19.186	2817	2822	2828	rBV	64986	93568	1.05%	0.118%
21	19.551	2877	2884	2894	rBV	5874281	8180200	91.42%	10.306%
22	21.339	3182	3188	3199	rBV	6883414	8948312	100.00%	11.273%
23	23.462	3541	3549	3559	rBV2	4289805	8361699	93.44%	10.534%
24	23.603	3566	3573	3587	rVB	4219587	8461341	94.56%	10.660%


Sum of corrected areas: 79375236

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
Data File : BM007543.D
Acq On : 24 Sep 2016 03:01
Operator : UM/SJ
Sample : H4855-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H9014

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

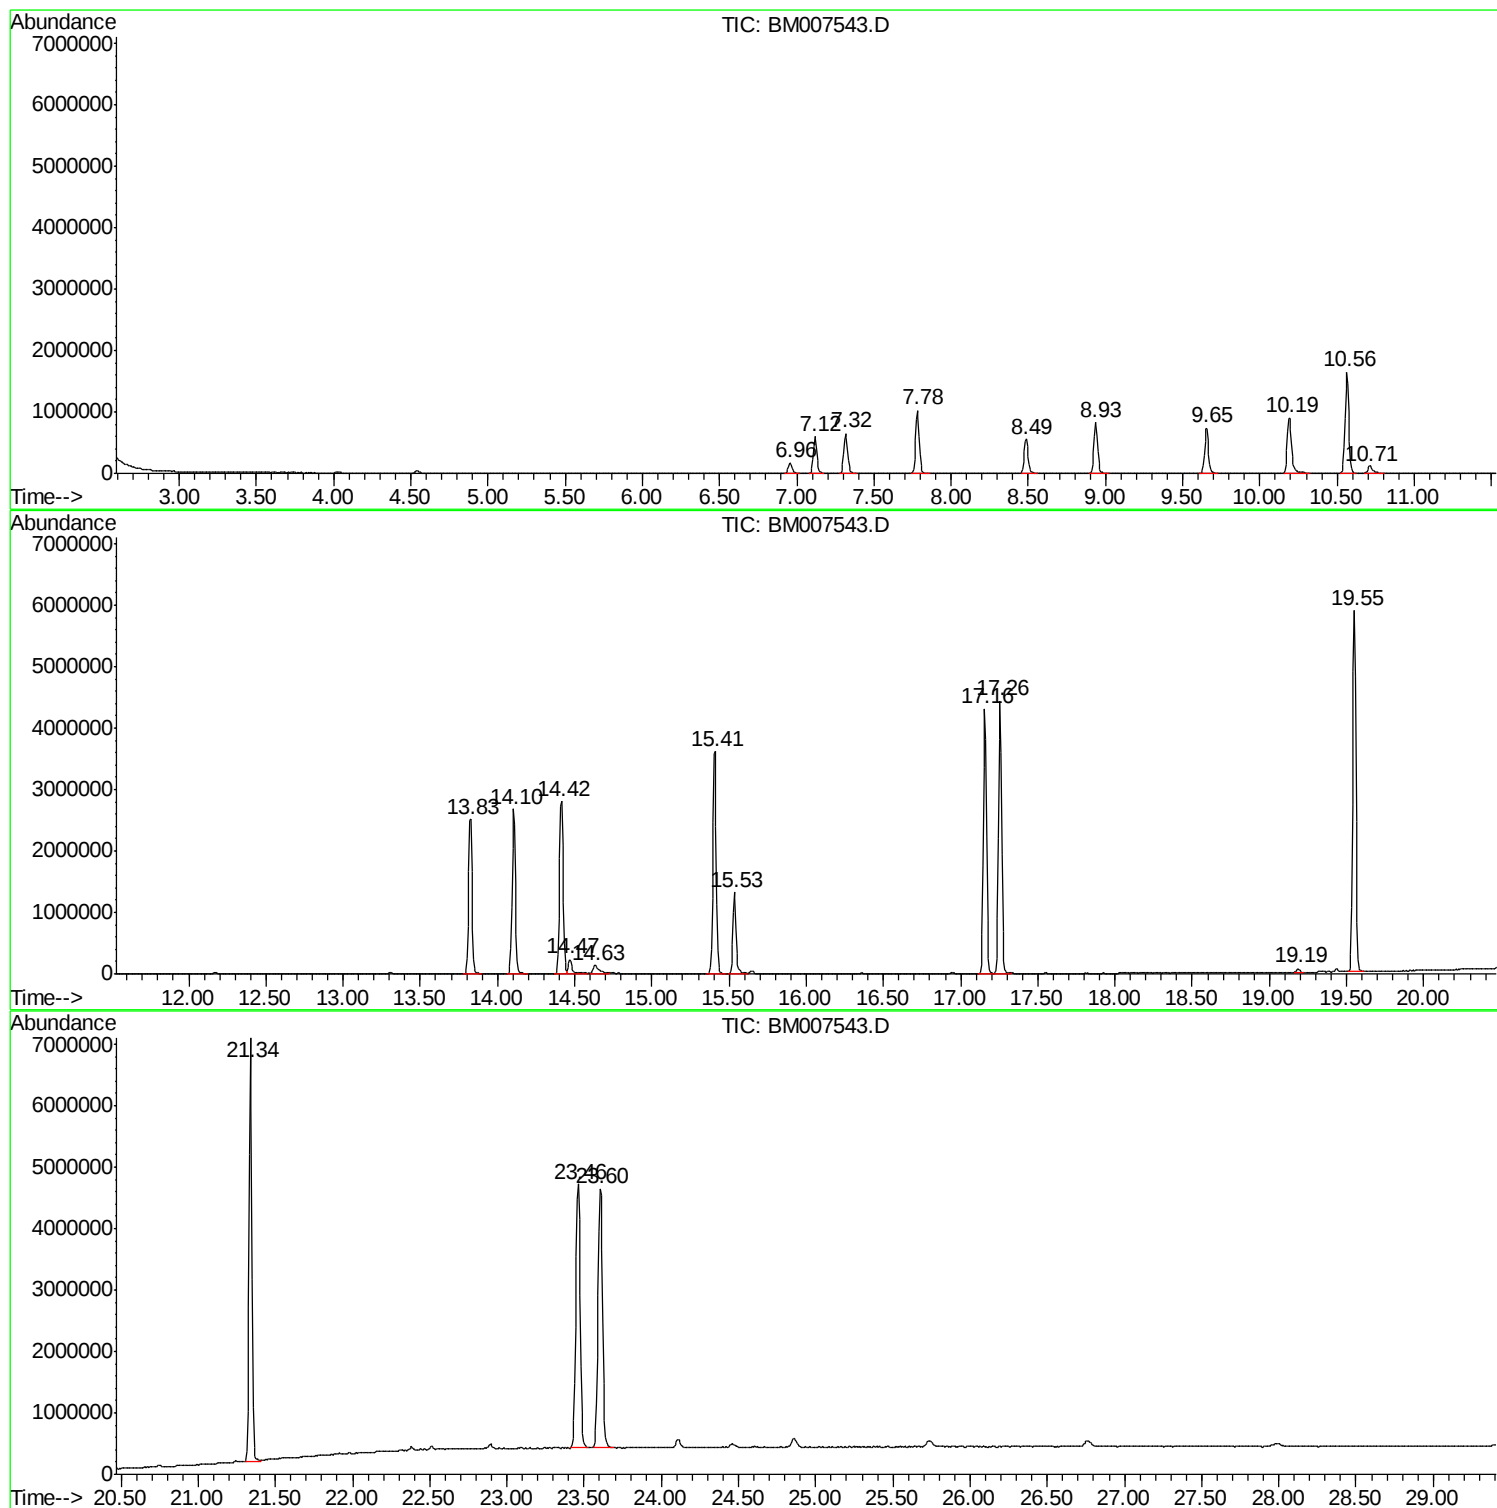

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007543.D
Acq On : 24 Sep 2016 03:01
Operator : UM/SJ
Sample : H4855-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H9014

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007543.D
Acq On : 24 Sep 2016 03:01
Operator : UM/SJ
Sample : H4855-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H9014

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc