

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
 Data File : BM007553.D
 Acq On : 24 Sep 2016 09:00
 Operator : UM/SJ
 Sample : H4866-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43S4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.910	729	735	738	rBV	153498	216770	2.04%	0.256%
2	6.951	738	742	755	rVB	238559	409992	3.86%	0.485%
3	7.116	763	770	781	rBV	748271	1192441	11.22%	1.410%
4	7.316	797	804	816	rBV	828592	1365356	12.85%	1.614%
5	7.781	876	883	892	rBV	746356	1231751	11.59%	1.456%
6	8.481	996	1002	1012	rBV	750483	1291209	12.15%	1.527%
7	8.934	1069	1079	1089	rBV	1067057	1808523	17.02%	2.138%
8	9.651	1194	1201	1216	rBV	942288	1619963	15.24%	1.915%
9	10.187	1285	1292	1312	rBV	1311752	2370064	22.30%	2.802%
10	10.563	1349	1356	1365	rVB	1171155	1984452	18.67%	2.346%
11	10.704	1372	1380	1396	rBV	1269458	2375299	22.35%	2.808%
12	13.822	1904	1910	1928	rBV	3215644	4712574	44.34%	5.572%
13	14.104	1949	1958	1974	rBV	3447298	5086494	47.86%	6.014%
14	14.410	2003	2010	2022	rBV	2140065	3245497	30.54%	3.837%
15	14.627	2042	2047	2065	rBV	203945	524535	4.94%	0.620%
16	15.404	2172	2179	2195	rBV	4526985	6911164	65.03%	8.171%
17	15.533	2195	2201	2211	rBV	1633486	2412581	22.70%	2.852%
18	17.157	2470	2477	2487	rBV	3036409	4297169	40.44%	5.081%
19	17.257	2487	2494	2505	rBV2	5715498	8297739	78.08%	9.811%
20	19.186	2817	2822	2829	rBV	83375	127344	1.20%	0.151%
21	19.551	2877	2884	2896	rBV2	7731213	10627345	100.00%	12.565%
22	21.339	3182	3188	3199	rBV	4632962	6195253	58.30%	7.325%
23	23.462	3541	3549	3561	rVB2	5547241	10597591	99.72%	12.530%
24	23.603	3566	3573	3585	rVB	2904722	5678695	53.43%	6.714%


Sum of corrected areas: 84579801

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
Data File : BM007553.D
Acq On : 24 Sep 2016 09:00
Operator : UM/SJ
Sample : H4866-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43S4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

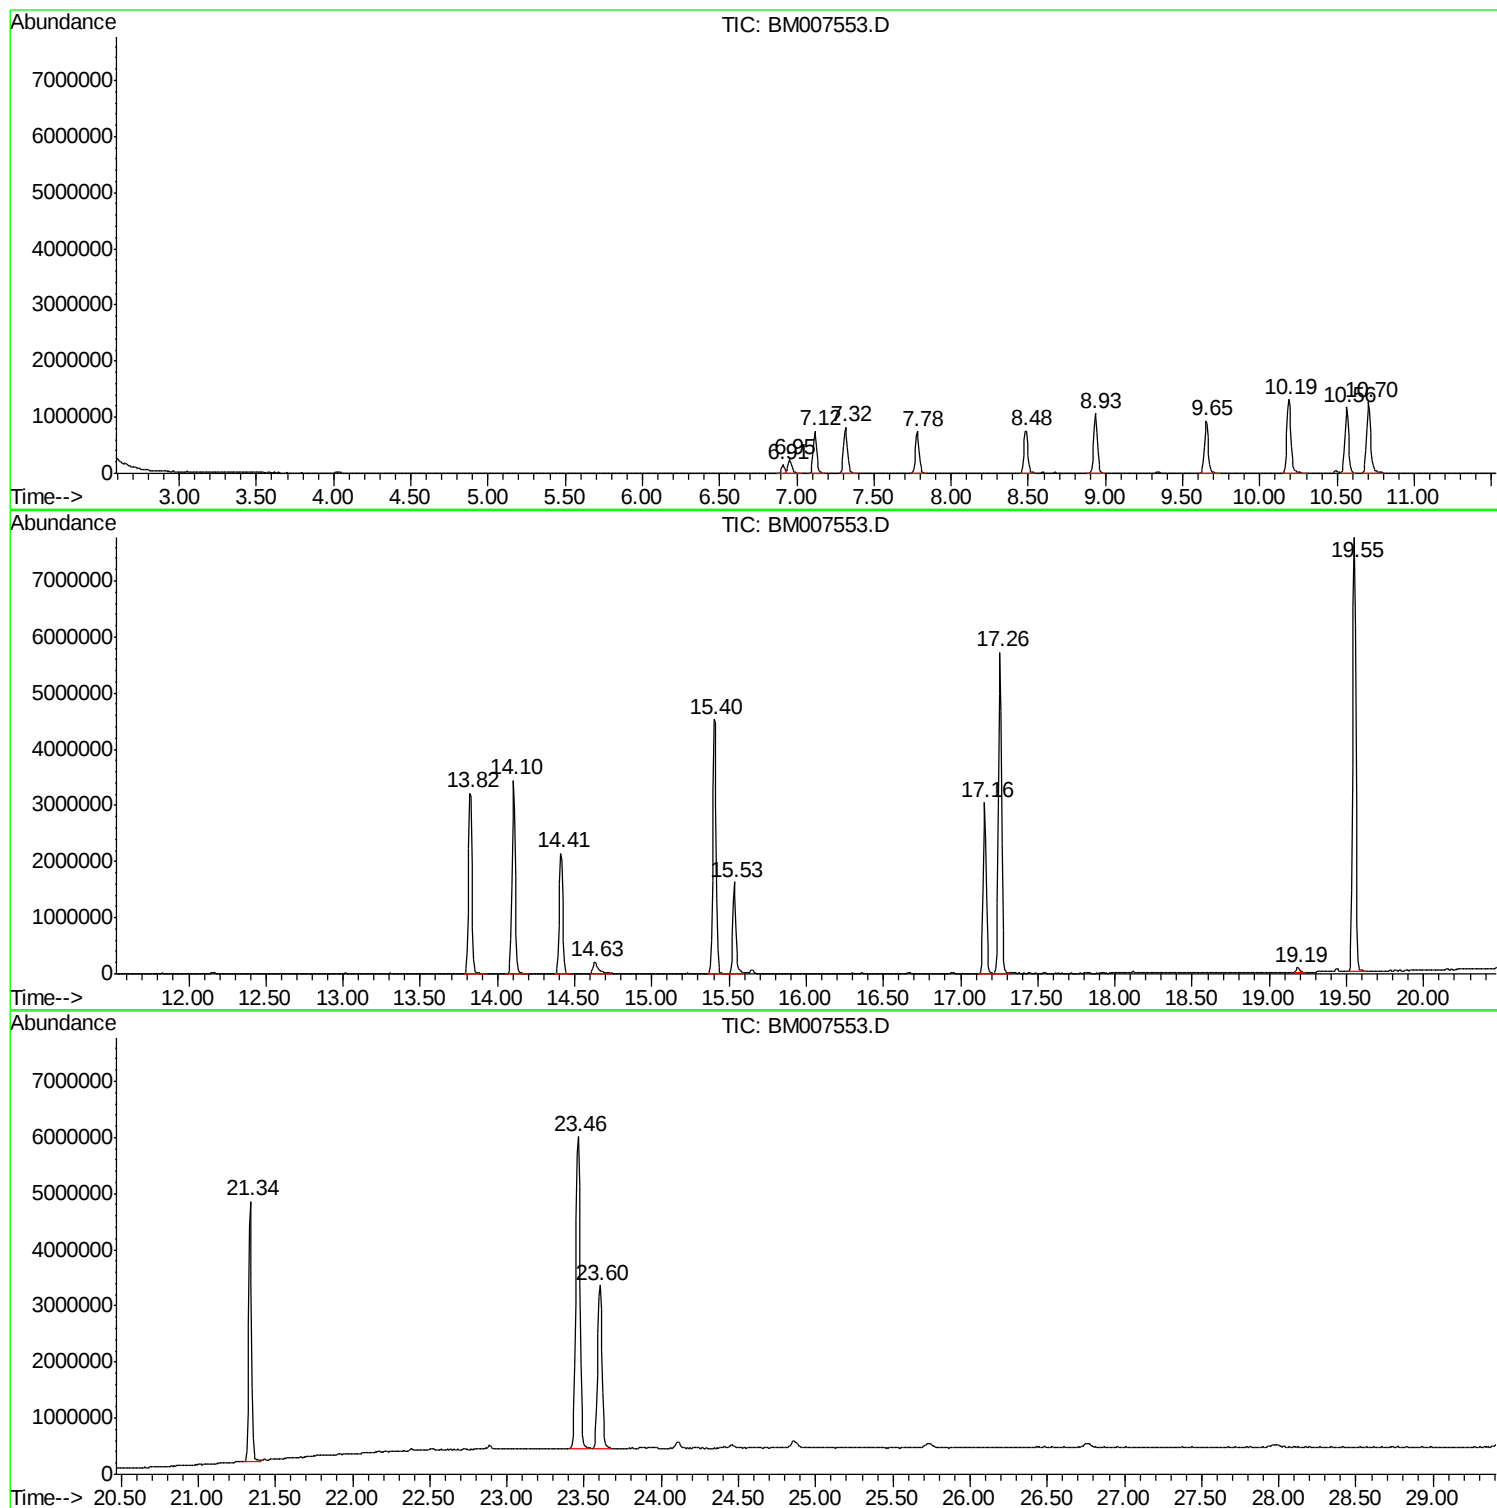

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007553.D
Acq On : 24 Sep 2016 09:00
Operator : UM/SJ
Sample : H4866-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43S4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007553.D
Acq On : 24 Sep 2016 09:00
Operator : UM/SJ
Sample : H4866-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43S4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc