

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
 Data File : BM007559.D
 Acq On : 24 Sep 2016 12:36
 Operator : UM/SJ
 Sample : H4866-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43T0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.951	737	742	752	rVB	308822	516809	3.72%	0.473%
2	7.116	764	770	782	rBV	1024913	1600809	11.53%	1.465%
3	7.316	797	804	816	rBV	1122842	1836134	13.22%	1.680%
4	7.781	876	883	891	rBV	976413	1596960	11.50%	1.461%
5	8.481	996	1002	1014	rBV	977693	1672901	12.05%	1.531%
6	8.934	1072	1079	1094	rBV	1435125	2460320	17.72%	2.251%
7	9.651	1193	1201	1214	rBV	1318658	2217414	15.97%	2.029%
8	10.186	1285	1292	1310	rBV	1734814	3157176	22.74%	2.889%
9	10.563	1349	1356	1365	rVB	1529557	2567425	18.49%	2.349%
10	10.704	1373	1380	1397	rBV	318222	642651	4.63%	0.588%
11	13.827	1904	1911	1925	rBV	4277595	6194189	44.61%	5.668%
12	14.104	1951	1958	1969	rBV	4566340	6754650	48.65%	6.180%
13	14.410	2003	2010	2024	rBV	2773552	4143003	29.84%	3.791%
14	14.627	2041	2047	2069	rBV	292503	678595	4.89%	0.621%
15	15.410	2172	2180	2193	rBV	5966388	9094549	65.50%	8.321%
16	15.533	2195	2201	2215	rVV	2328205	3448911	24.84%	3.156%
17	17.157	2470	2477	2487	rBV	3960928	5598017	40.32%	5.122%
18	17.257	2487	2494	2507	rBV	7347793	10756310	77.46%	9.842%
19	19.186	2817	2822	2828	rBV	111153	159909	1.15%	0.146%
20	19.551	2877	2884	2899	rBV	9744325	13633124	98.18%	12.474%
21	19.780	2919	2923	2929	rBV	159185	183140	1.32%	0.168%
22	21.339	3182	3188	3200	rBV	5948320	7956344	57.30%	7.280%
23	23.462	3541	3549	3561	rVB2	7153418	13885408	100.00%	12.705%
24	23.603	3566	3573	3583	rVB	3812478	7435471	53.55%	6.803%
25	24.103	3654	3658	3666	rVB3	267931	515132	3.71%	0.471%
26	24.856	3782	3786	3794	rVB	288507	586468	4.22%	0.537%


Sum of corrected areas: 109291819

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
Data File : BM007559.D
Acq On : 24 Sep 2016 12:36
Operator : UM/SJ
Sample : H4866-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
E43T0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

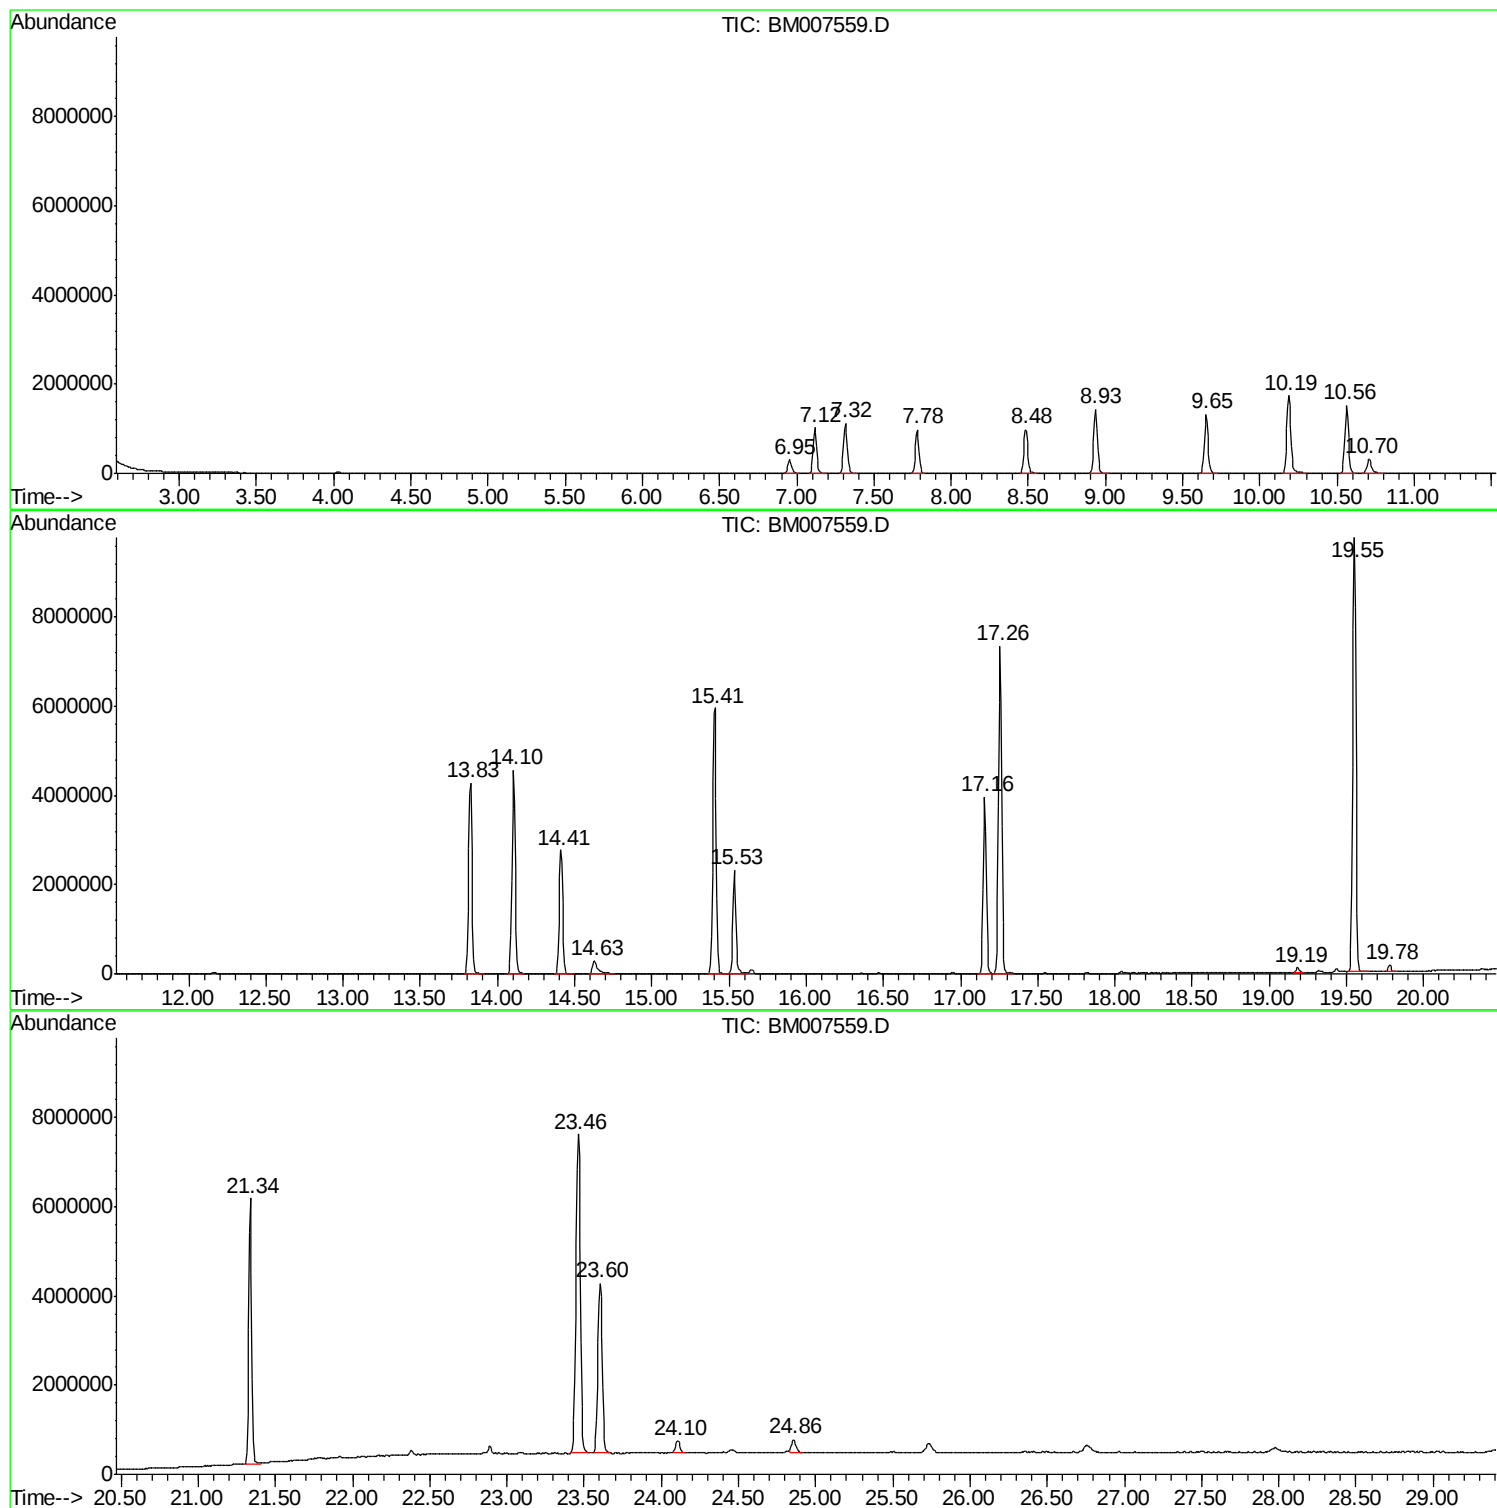

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007559.D
Acq On : 24 Sep 2016 12:36
Operator : UM/SJ
Sample : H4866-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007559.D
Acq On : 24 Sep 2016 12:36
Operator : UM/SJ
Sample : H4866-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc