

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
 Data File : BM007560.D
 Acq On : 24 Sep 2016 13:12
 Operator : UM/SJ
 Sample : H4866-08
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43T4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.951	737	742	755	rVB	229396	391822	3.56%	0.444%
2	7.116	763	770	783	rBV	836643	1310307	11.91%	1.486%
3	7.316	797	804	815	rBV	885213	1455658	13.23%	1.651%
4	7.781	874	883	891	rBV	804686	1319726	12.00%	1.497%
5	8.481	995	1002	1015	rBV	749611	1273349	11.58%	1.444%
6	8.933	1071	1079	1094	rBV	1153622	1978651	17.99%	2.244%
7	9.651	1194	1201	1211	rBV	1045759	1761198	16.01%	1.997%
8	10.186	1285	1292	1312	rBV	1345354	2494555	22.68%	2.829%
9	10.563	1348	1356	1365	rVB	1245743	2117100	19.25%	2.401%
10	10.710	1374	1381	1393	rBV	161945	335929	3.05%	0.381%
11	13.821	1903	1910	1927	rBV	3440540	5007807	45.53%	5.679%
12	14.104	1950	1958	1970	rBV	3645529	5514317	50.13%	6.253%
13	14.410	2003	2010	2022	rBV	2381161	3461471	31.47%	3.925%
14	14.633	2039	2048	2066	rBV2	167823	458703	4.17%	0.520%
15	15.404	2172	2179	2193	rBV	4986895	7389002	67.17%	8.379%
16	15.533	2195	2201	2216	rVV	1754167	2657469	24.16%	3.014%
17	17.156	2470	2477	2487	rBV	3269300	4633637	42.12%	5.255%
18	17.256	2487	2494	2506	rBV	5953740	8726931	79.34%	9.896%
19	19.186	2817	2822	2828	rBV	82445	126714	1.15%	0.144%
20	19.550	2877	2884	2897	rBV	7723937	10999806	100.00%	12.474%
21	21.244	3168	3172	3178	rBV	1135530	1232218	11.20%	1.397%
22	21.339	3182	3188	3198	rVV	4985994	6561135	59.65%	7.440%
23	23.462	3541	3549	3557	rBV2	5735956	10871412	98.83%	12.328%
24	23.603	3566	3573	3587	rVB	3077110	6104915	55.50%	6.923%


Sum of corrected areas: 88183832

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
Data File : BM007560.D
Acq On : 24 Sep 2016 13:12
Operator : UM/SJ
Sample : H4866-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T4

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

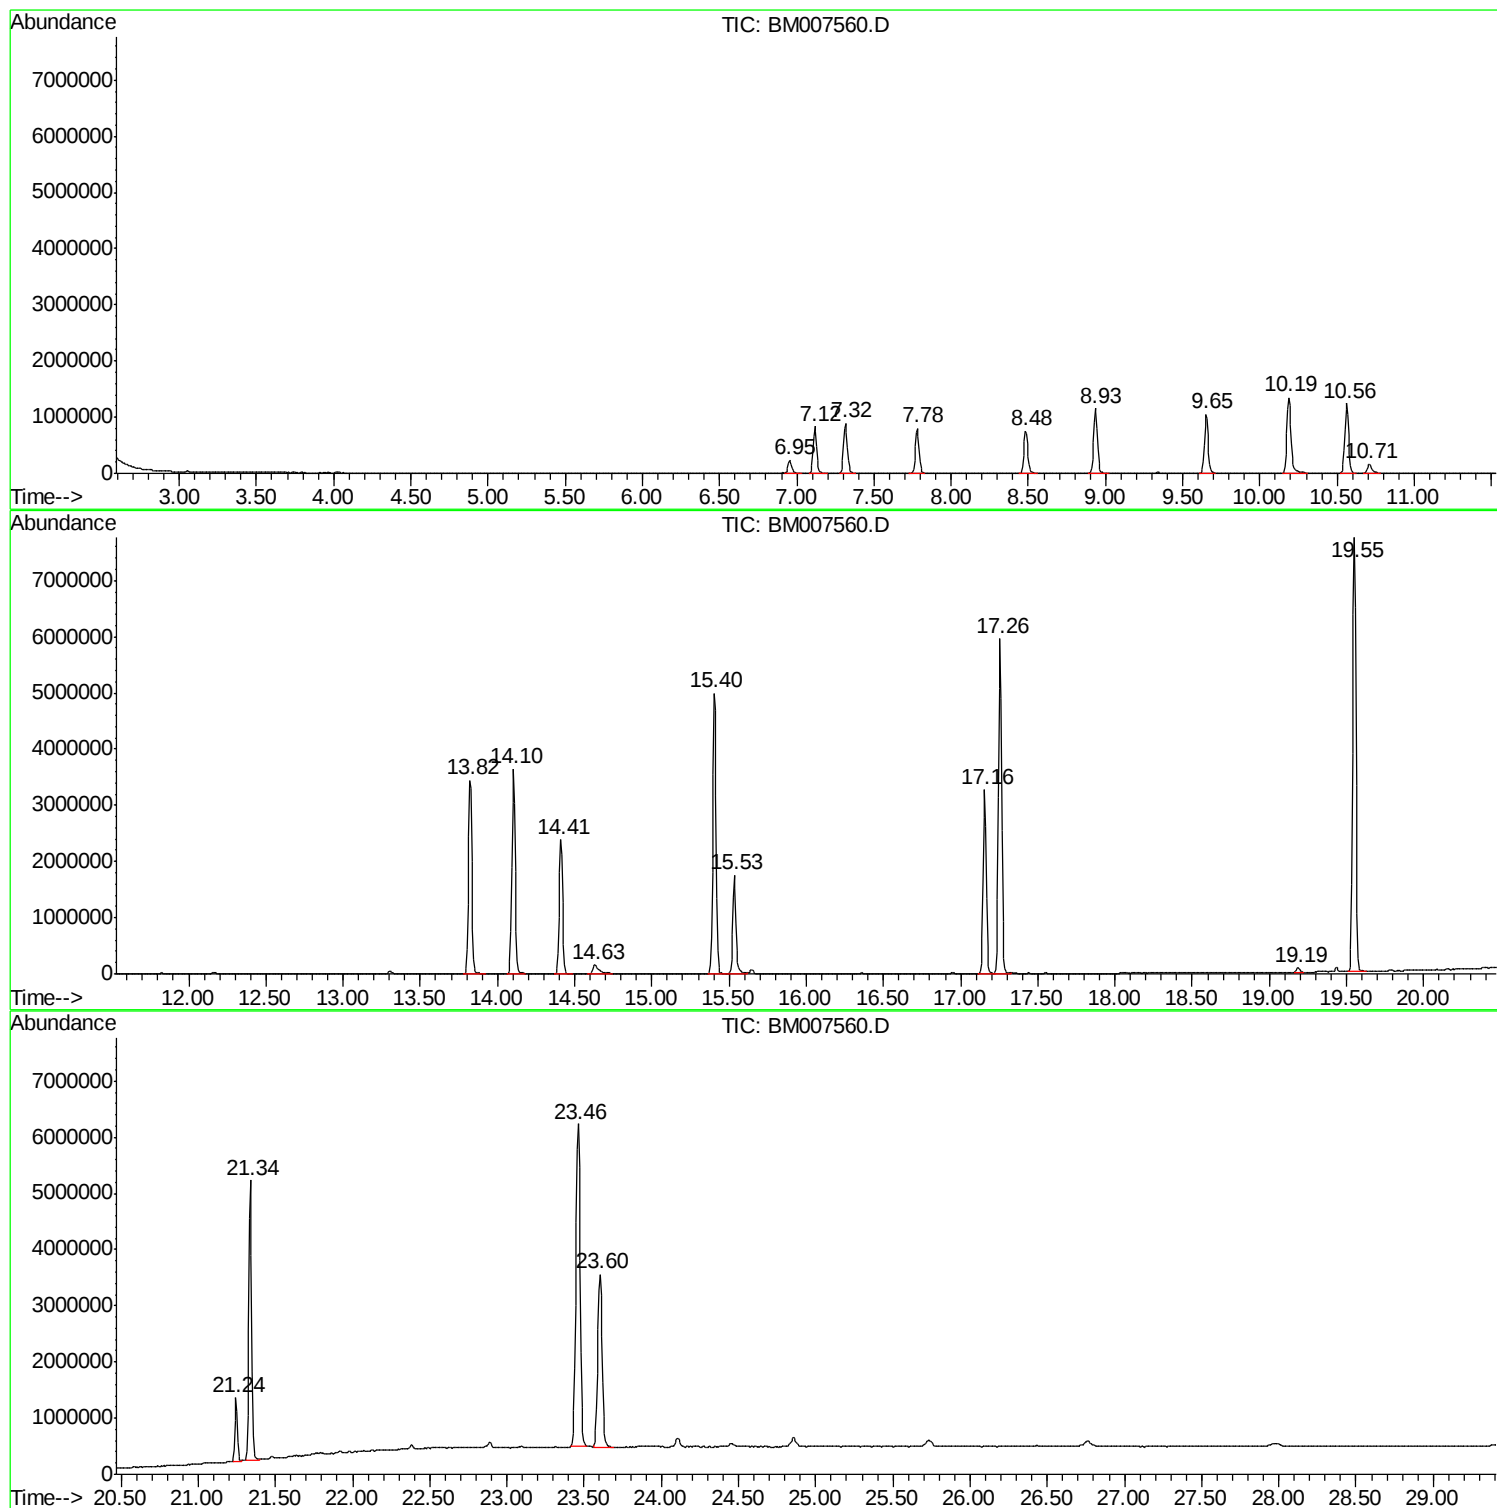

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007560.D
Acq On : 24 Sep 2016 13:12
Operator : UM/SJ
Sample : H4866-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007560.D
Acq On : 24 Sep 2016 13:12
Operator : UM/SJ
Sample : H4866-08
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T4

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc