

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
 Data File : BM007561.D
 Acq On : 24 Sep 2016 13:48
 Operator : UM/SJ
 Sample : H4866-09
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43T5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.951	738	742	753	rVB	242996	404536	3.48%	0.450%
2	7.116	763	770	782	rBV	899619	1422039	12.24%	1.582%
3	7.316	797	804	815	rBV	949290	1565169	13.47%	1.741%
4	7.781	876	883	893	rBV	800400	1314539	11.31%	1.462%
5	8.480	996	1002	1014	rBV	780642	1332410	11.47%	1.482%
6	8.933	1072	1079	1091	rBV	1273965	2130178	18.33%	2.370%
7	9.339	1142	1148	1155	rVB	97841	146645	1.26%	0.163%
8	9.651	1194	1201	1216	rBV	1079572	1880869	16.19%	2.092%
9	10.186	1284	1292	1308	rBV	1437350	2660543	22.90%	2.960%
10	10.563	1349	1356	1364	rVB	1234114	2090976	17.99%	2.326%
11	10.710	1374	1381	1397	rBV	221285	459351	3.95%	0.511%
12	13.821	1903	1910	1924	rBV	3590547	5311619	45.71%	5.909%
13	14.104	1951	1958	1970	rBV	3874680	5787660	49.81%	6.438%
14	14.409	2002	2010	2020	rBV	2258996	3350948	28.84%	3.728%
15	14.627	2041	2047	2071	rBV	169690	460258	3.96%	0.512%
16	15.404	2172	2179	2191	rBV	5103111	7794263	67.07%	8.670%
17	15.533	2195	2201	2216	rVV	1835355	2778264	23.91%	3.091%
18	17.156	2469	2477	2487	rBV	3103216	4438707	38.20%	4.938%
19	17.256	2487	2494	2510	rVV	6330380	9136146	78.62%	10.163%
20	19.186	2817	2822	2827	rBV	82541	116415	1.00%	0.130%
21	19.550	2877	2884	2896	rBV2	8042946	11544625	99.35%	12.842%
22	21.338	3182	3188	3197	rBV	4809527	6302084	54.23%	7.010%
23	23.462	3541	3549	3564	rBV2	6033240	11620355	100.00%	12.926%
24	23.603	3566	3573	3585	rVB	2990495	5847079	50.32%	6.504%


Sum of corrected areas: 89895678

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
Data File : BM007561.D
Acq On : 24 Sep 2016 13:48
Operator : UM/SJ
Sample : H4866-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T5

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

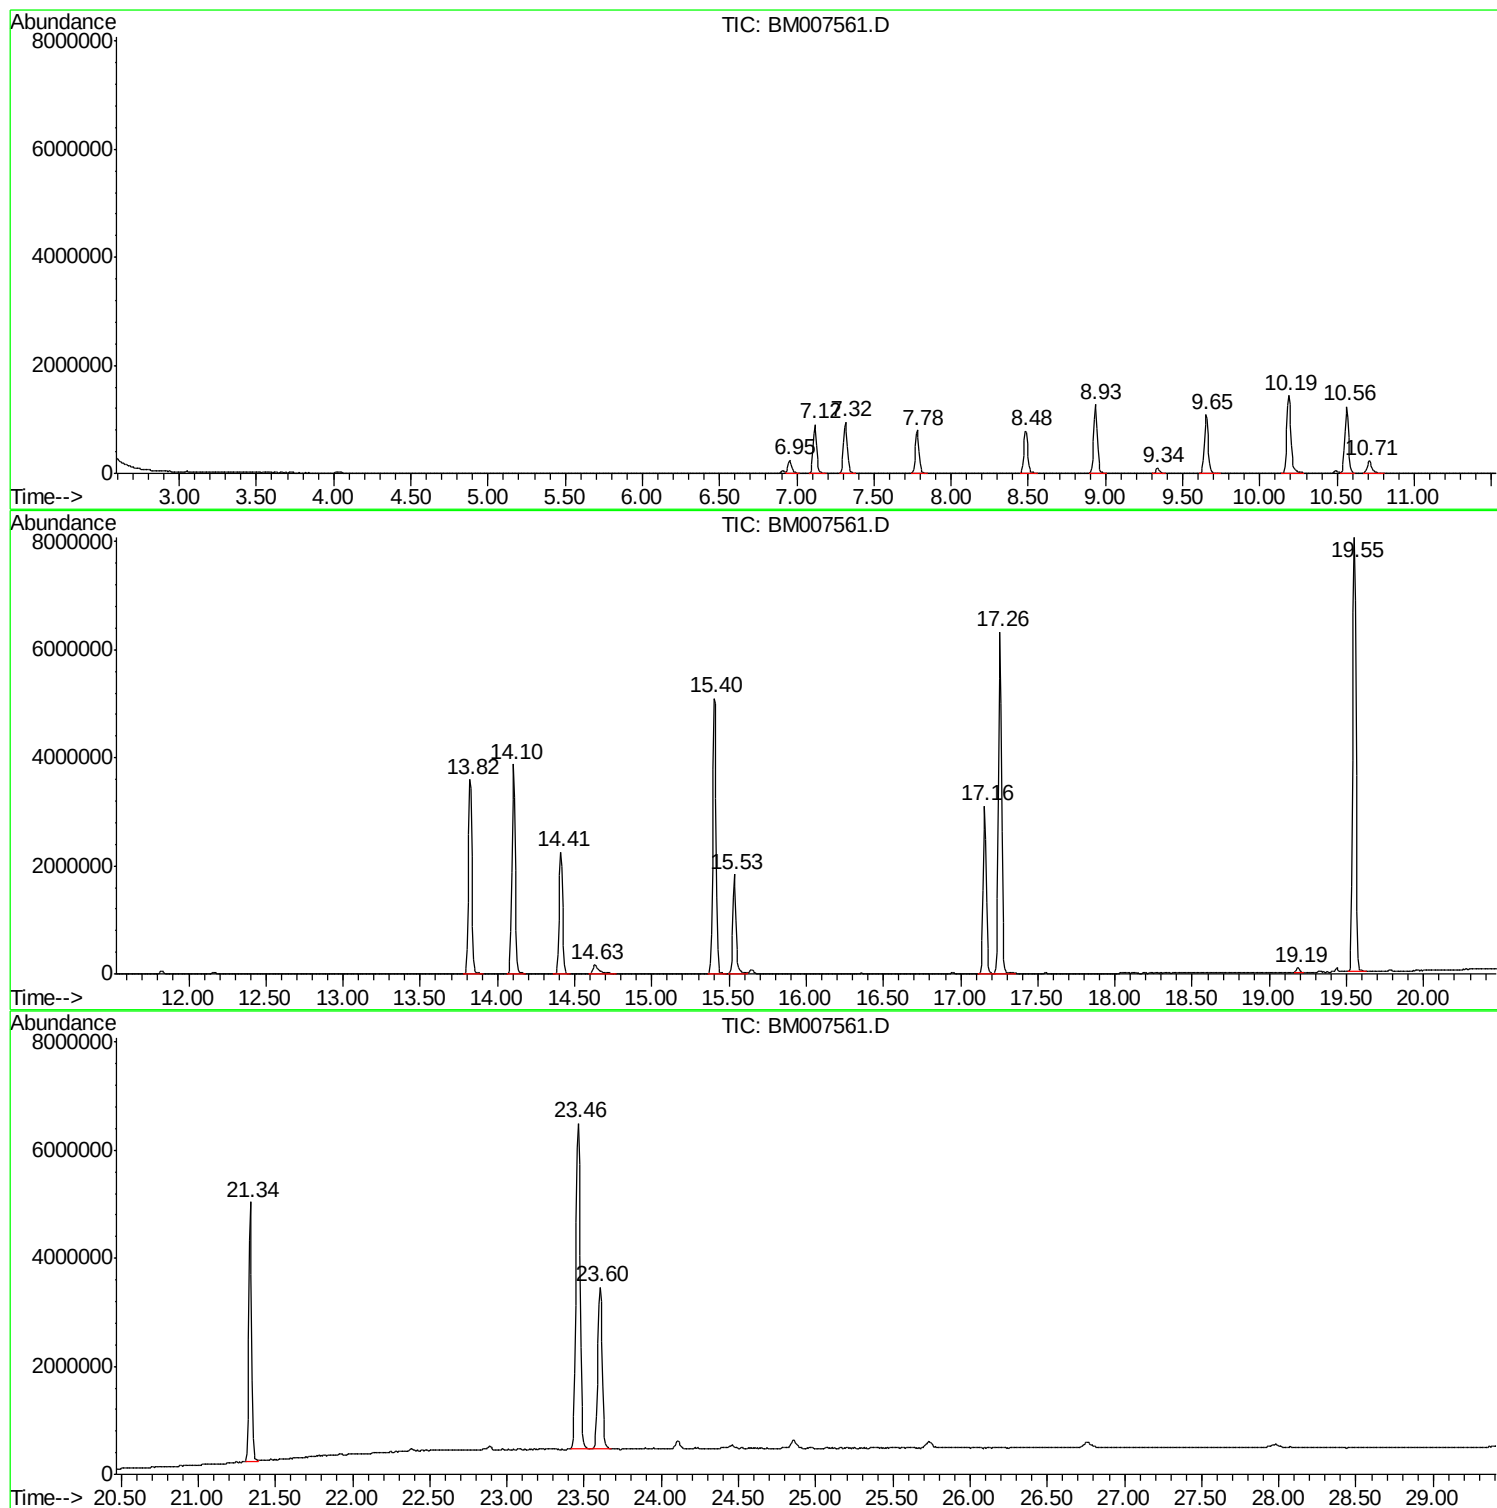

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007561.D
Acq On : 24 Sep 2016 13:48
Operator : UM/SJ
Sample : H4866-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007561.D
Acq On : 24 Sep 2016 13:48
Operator : UM/SJ
Sample : H4866-09
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43T5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc