

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
 Data File : BM007562.D
 Acq On : 24 Sep 2016 14:24
 Operator : UM/SJ
 Sample : H4866-10
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E43S0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.951	738	742	753	rVB	248090	422529	3.78%	0.484%
2	7.116	763	770	783	rBV	744235	1184614	10.61%	1.356%
3	7.316	797	804	814	rBV	847761	1400044	12.53%	1.602%
4	7.781	876	883	892	rBV	821112	1345805	12.05%	1.540%
5	8.480	996	1002	1013	rBV	805656	1356467	12.14%	1.552%
6	8.933	1072	1079	1094	rBV	1046092	1822849	16.32%	2.086%
7	9.651	1194	1201	1210	rBV	956346	1619488	14.50%	1.853%
8	10.186	1284	1292	1316	rBV	1319808	2553945	22.86%	2.923%
9	10.563	1349	1356	1367	rVB	1270399	2160824	19.34%	2.473%
10	10.716	1374	1382	1393	rBV	75643	167209	1.50%	0.191%
11	13.821	1903	1910	1924	rBV	3138582	4647064	41.60%	5.318%
12	14.104	1947	1958	1970	rBV	3408335	5087715	45.55%	5.822%
13	14.410	2003	2010	2023	rBV	2320725	3464900	31.02%	3.965%
14	14.633	2042	2048	2066	rBV	232357	552076	4.94%	0.632%
15	15.404	2172	2179	2194	rBV	4713685	6863774	61.45%	7.855%
16	15.533	2194	2201	2215	rVV	1734487	2545217	22.79%	2.913%
17	17.156	2470	2477	2487	rBV	3255721	4672498	41.83%	5.347%
18	17.256	2487	2494	2507	rVV	5644110	8218997	73.58%	9.406%
19	18.045	2623	2628	2633	rBV2	88627	129517	1.16%	0.148%
20	19.180	2817	2821	2827	rBV	85117	130821	1.17%	0.150%
21	19.321	2841	2845	2853	rBV	158707	243979	2.18%	0.279%
22	19.550	2877	2884	2890	rBV	7701953	10726219	96.02%	12.275%
23	21.244	3169	3172	3176	rBV	115597	125886	1.13%	0.144%
24	21.338	3182	3188	3195	rBV	5099733	6852375	61.34%	7.842%
25	21.827	3269	3271	3276	rBV3	92675	127297	1.14%	0.146%
26	22.074	3309	3313	3318	rBV	262480	332900	2.98%	0.381%
27	23.462	3541	3549	3558	rVB2	5852116	11170310	100.00%	12.783%
28	23.603	3566	3573	3586	rVB	3330700	6491221	58.11%	7.429%
29	24.109	3655	3659	3668	rVB	230518	409183	3.66%	0.468%
30	24.856	3782	3786	3795	rVB2	261018	556892	4.99%	0.637%


Sum of corrected areas: 87382615

Data Path : Z:\HPCHEM1\BNA M\DATA\BM092316\
Data File : BM007562.D
Acq On : 24 Sep 2016 14:24
Operator : UM/SJ
Sample : H4866-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
E43S0

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

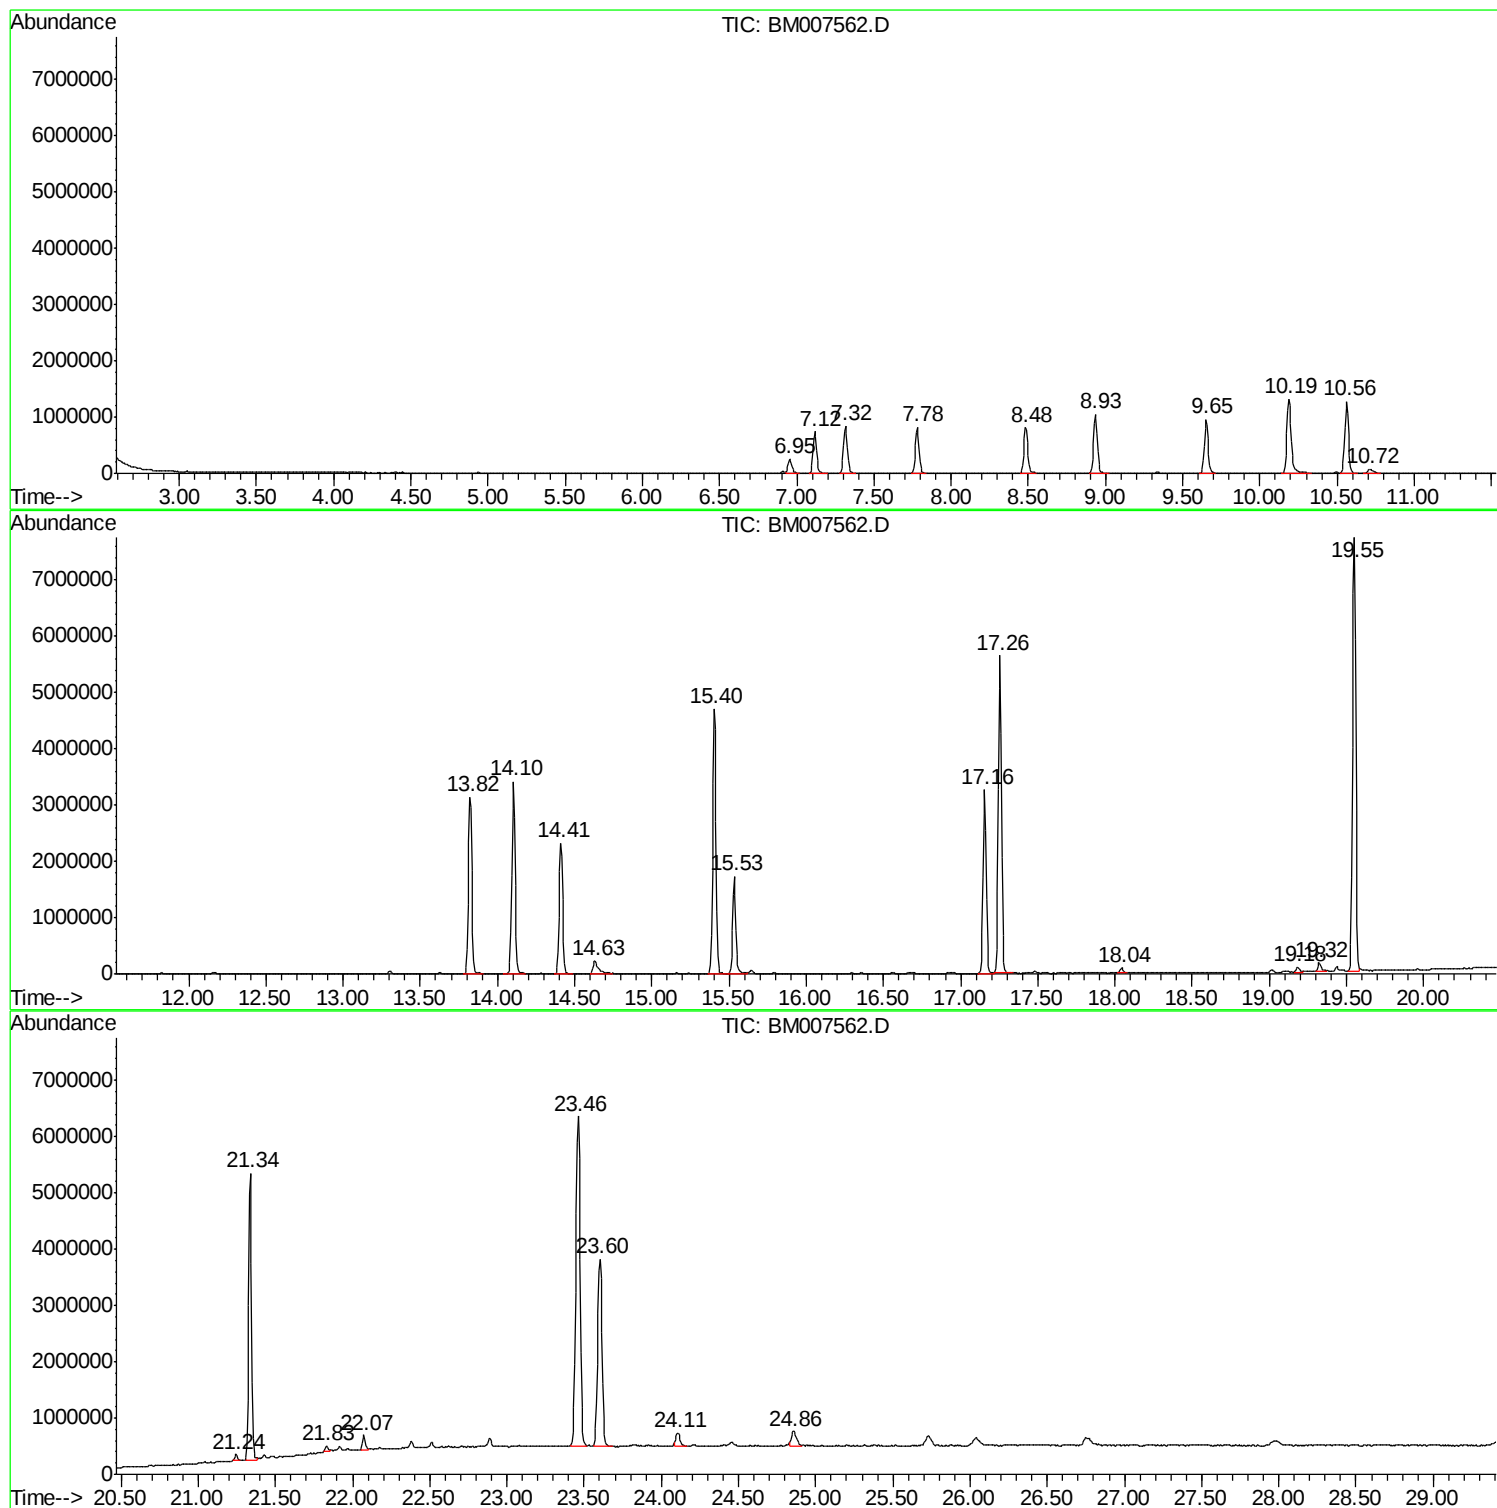

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007562.D
Acq On : 24 Sep 2016 14:24
Operator : UM/SJ
Sample : H4866-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43S0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092316\
Data File : BM007562.D
Acq On : 24 Sep 2016 14:24
Operator : UM/SJ
Sample : H4866-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E43S0

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM092316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc