

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011708.D
 Acq On : 23 Sep 2017 16:44
 Operator : SJ/JU
 Sample : I5324-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	12	16	24	rVB	60135	81221	1.57%	0.177%
2	4.128	140	143	147	rVB5	7272	9104	0.18%	0.020%
3	5.263	330	336	342	rVB5	13065	23919	0.46%	0.052%
4	6.157	485	488	493	rVB6	7585	11603	0.22%	0.025%
5	6.557	551	556	559	rBV6	2577	5671	0.11%	0.012%
6	6.610	562	565	569	rBV4	3531	5519	0.11%	0.012%
7	7.057	634	641	643	rBV7	4910	7969	0.15%	0.017%
8	7.104	643	649	657	rVB	192782	325374	6.28%	0.711%
9	7.275	671	678	689	rBV	772280	1205178	23.27%	2.633%
10	7.363	691	693	699	rVB5	6012	9436	0.18%	0.021%
11	7.481	706	713	725	rBV	796582	1321666	25.52%	2.887%
12	7.951	785	793	806	rBV	717860	1190926	23.00%	2.601%
13	8.304	850	853	859	rVV5	8056	11546	0.22%	0.025%
14	8.645	905	911	924	rBV	524897	889044	17.17%	1.942%
15	9.110	982	990	1004	rBV	898041	1607757	31.04%	3.512%
16	9.498	1053	1056	1064	rVB4	11065	21755	0.42%	0.048%
17	9.834	1106	1113	1126	rBV	773861	1328095	25.64%	2.901%
18	10.369	1196	1204	1218	rBV	994497	1724311	33.30%	3.767%
19	10.757	1263	1270	1281	rVB	894300	1560828	30.14%	3.409%
20	10.892	1288	1293	1301	rBV6	12779	27220	0.53%	0.059%
21	11.569	1405	1408	1414	rBV6	6481	11498	0.22%	0.025%
22	11.992	1477	1480	1485	rVB5	9488	15233	0.29%	0.033%
23	12.339	1535	1539	1548	rVB4	14505	25534	0.49%	0.056%
24	13.980	1812	1818	1832	rVB	1724767	2530269	48.86%	5.527%
25	14.216	1855	1858	1861	rBV4	3295	5242	0.10%	0.011%
26	14.274	1861	1868	1879	rVV	1887444	2924946	56.48%	6.389%
27	14.416	1883	1892	1900	rBV2	34732	91737	1.77%	0.200%
28	14.580	1914	1920	1930	rVB2	1163890	1837417	35.48%	4.014%
29	14.774	1947	1953	1964	rBV2	90068	216299	4.18%	0.472%
30	14.980	1983	1988	1991	rBV6	4347	8550	0.17%	0.019%
31	15.257	2028	2035	2039	rBV8	7073	15574	0.30%	0.034%
32	15.339	2044	2049	2051	rBV6	5114	7485	0.14%	0.016%
33	15.574	2082	2089	2102	rVV	2440084	3619461	69.89%	7.906%
34	15.686	2102	2108	2121	rVV	916255	1326773	25.62%	2.898%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
Data File : BM011708.D
Acq On : 23 Sep 2017 16:44
Operator : SJ/JU
Sample : I5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT8

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Title : SVOA CALIBRATION

35	15.810	2125	2129	2133	rVB2	30893	42479	0.82%	0.093%
36	16.139	2181	2185	2188	rBV5	5415	7467	0.14%	0.016%
37	16.621	2260	2267	2269	rBV6	8688	9845	0.19%	0.022%
38	16.715	2278	2283	2284	rBV5	4031	5393	0.10%	0.012%
39	17.115	2346	2351	2358	rBV3	21998	35197	0.68%	0.077%
40	17.233	2364	2371	2376	rBV	20219	30655	0.59%	0.067%
41	17.321	2380	2386	2395	rVV2	1487580	2147448	41.47%	4.691%
42	17.421	2395	2403	2414	rVV	2875266	4009054	77.41%	8.757%
43	17.509	2417	2418	2423	rVB5	8811	7532	0.15%	0.016%
44	17.927	2485	2489	2494	rBV6	14288	21689	0.42%	0.047%
45	18.157	2524	2528	2529	rBV4	4818	6230	0.12%	0.014%
46	18.192	2529	2534	2544	rVV2	58458	113130	2.18%	0.247%
47	18.274	2544	2548	2551	rVB2	14872	21265	0.41%	0.046%
48	19.345	2726	2730	2736	rVB	36962	48288	0.93%	0.105%
49	19.462	2746	2750	2758	rBV3	87839	146546	2.83%	0.320%
50	19.598	2770	2773	2779	rVB3	30383	51038	0.99%	0.111%
51	19.709	2785	2792	2802	rBV	3472427	4752246	91.76%	10.381%
52	21.486	3089	3094	3102	rBV	1983310	2584546	49.91%	5.646%
53	23.697	3463	3470	3482	rVB2	2528784	5178815	100.00%	11.313%
54	23.850	3489	3496	3503	rBV	1296184	2556404	49.36%	5.584%


Sum of corrected areas: 45779427

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
Data File : BM011708.D
Acq On : 23 Sep 2017 16:44
Operator : SJ/JU
Sample : I5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

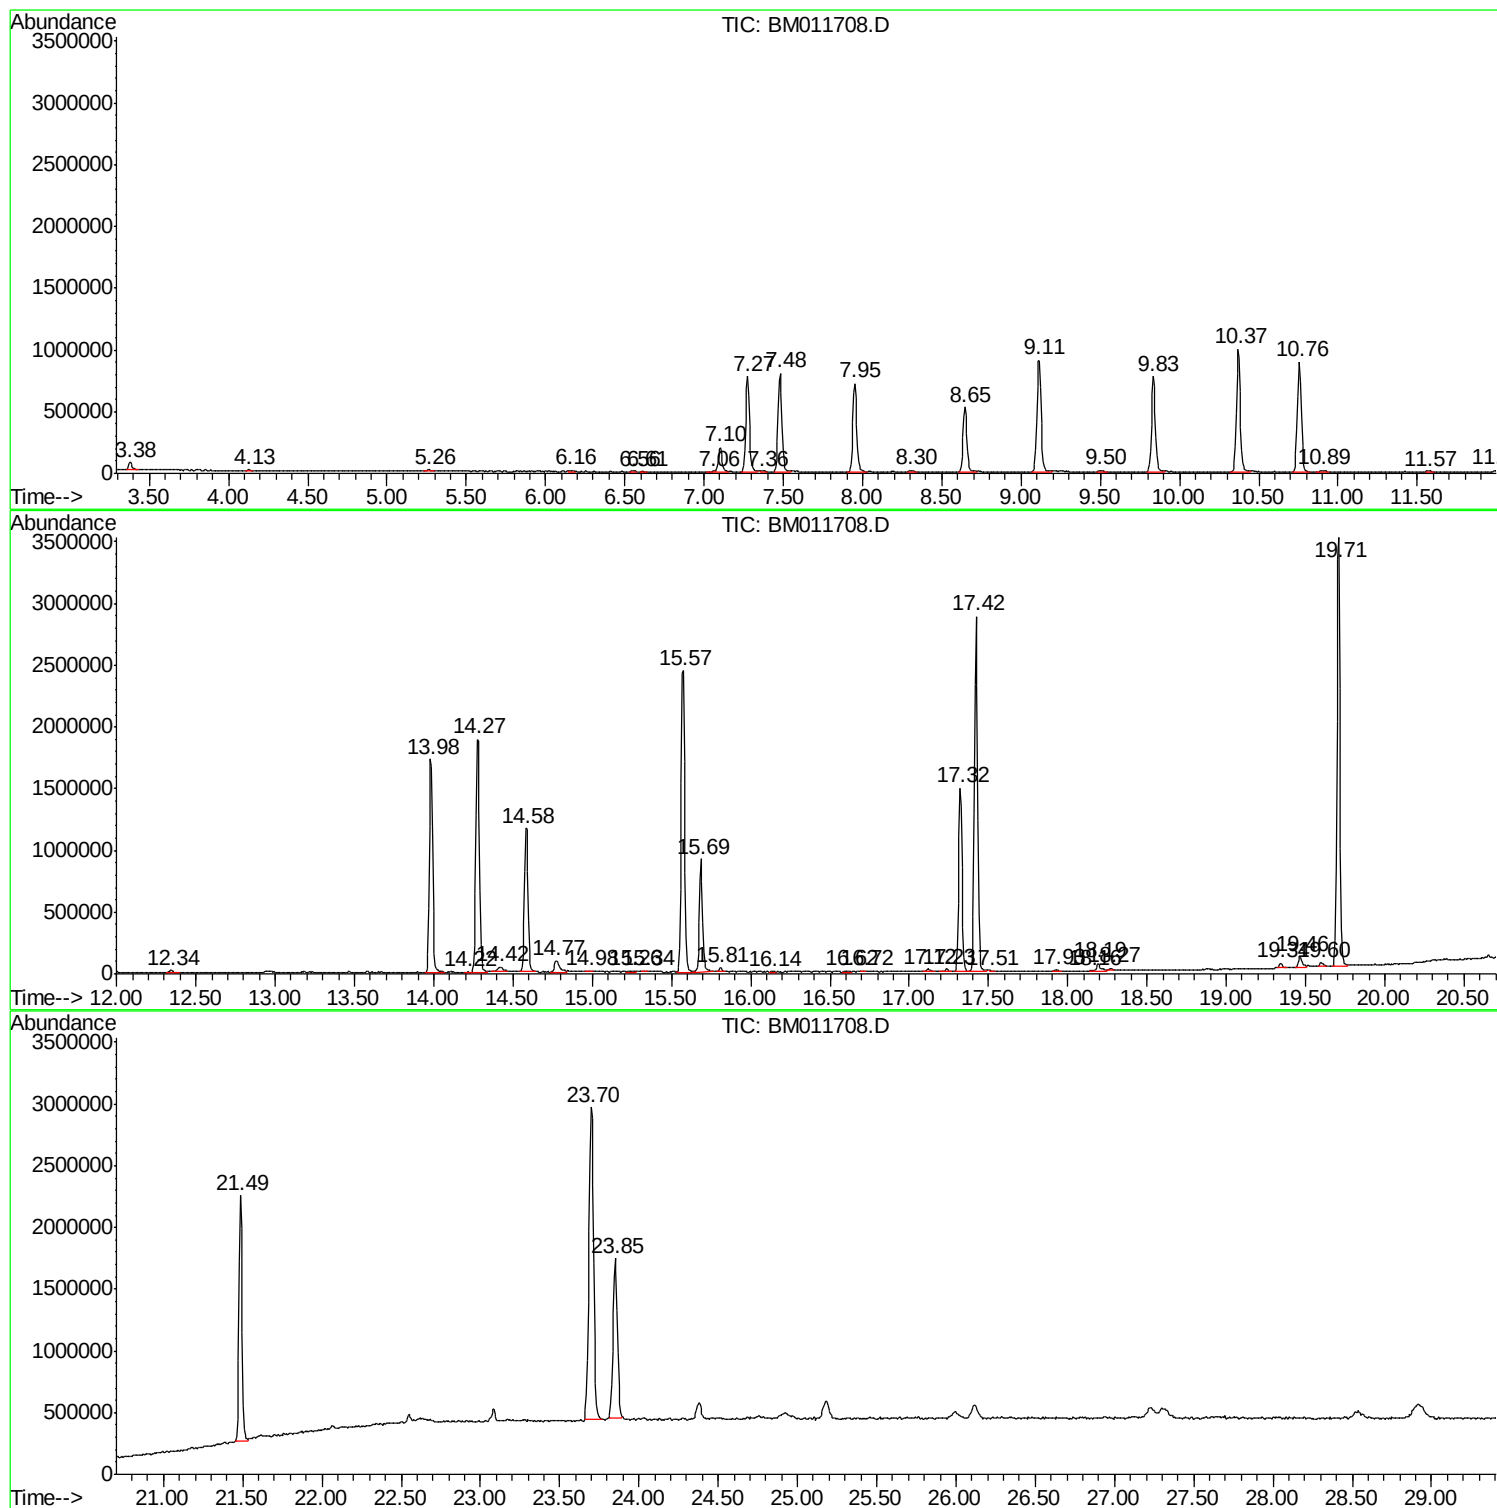

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
Data File : BM011708.D
Acq On : 23 Sep 2017 16:44
Operator : SJ/JU
Sample : I5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
Data File : BM011708.D
Acq On : 23 Sep 2017 16:44
Operator : SJ/JU
Sample : I5324-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT8

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc