

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011716.D
 Acq On : 23 Sep 2017 21:37
 Operator : SJ/JU
 Sample : I5324-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	65	67	69	rVB3	4577	3504	0.15%	0.024%
2	4.128	141	143	147	rBV5	5863	6561	0.27%	0.045%
3	4.393	186	188	191	rVB2	3218	3015	0.13%	0.021%
4	4.498	204	206	208	rBV3	3477	2735	0.11%	0.019%
5	4.963	282	285	289	rBV5	2974	4090	0.17%	0.028%
6	5.010	291	293	296	rVB4	2960	2692	0.11%	0.019%
7	5.193	320	324	326	rVB5	3533	4215	0.18%	0.029%
8	5.328	345	347	350	rBV4	2924	2838	0.12%	0.020%
9	5.422	360	363	367	rBV5	2897	3964	0.16%	0.027%
10	5.698	406	410	412	rVB4	2245	2634	0.11%	0.018%
11	5.751	418	419	423	rVB4	3103	2675	0.11%	0.019%
12	6.510	546	548	552	rVB5	2024	2537	0.11%	0.018%
13	6.669	572	575	578	rBV4	3062	4463	0.19%	0.031%
14	6.922	617	618	620	rBV2	3274	2470	0.10%	0.017%
15	7.104	645	649	655	rBV5	12588	23143	0.96%	0.160%
16	7.204	662	666	669	rBV5	2257	3973	0.17%	0.028%
17	7.275	673	678	690	rVB2	56456	101164	4.21%	0.701%
18	7.481	708	713	721	rVV	60479	112960	4.70%	0.783%
19	7.951	785	793	807	rBV	657776	1120341	46.59%	7.764%
20	8.498	884	886	891	rVB5	2539	3359	0.14%	0.023%
21	8.651	907	912	922	rVV2	31904	66313	2.76%	0.460%
22	8.998	965	971	973	rBV7	2430	4898	0.20%	0.034%
23	9.116	985	991	1000	rBV2	65181	125875	5.23%	0.872%
24	9.504	1056	1057	1063	rVV4	2294	3275	0.14%	0.023%
25	9.545	1063	1064	1070	rVB4	2703	4019	0.17%	0.028%
26	9.839	1106	1114	1124	rBV2	50330	102673	4.27%	0.711%
27	9.957	1132	1134	1135	rBV2	3249	2745	0.11%	0.019%
28	9.975	1135	1137	1140	rVB4	2459	2883	0.12%	0.020%
29	10.092	1153	1157	1159	rBV4	1829	3117	0.13%	0.022%
30	10.375	1198	1205	1215	rBV	58419	123448	5.13%	0.855%
31	10.439	1215	1216	1220	rVB2	4922	3624	0.15%	0.025%
32	10.622	1245	1247	1250	rVB4	2358	2681	0.11%	0.019%
33	10.651	1250	1252	1253	rBV	3151	2608	0.11%	0.018%
34	10.751	1262	1269	1279	rBV	804124	1448630	60.24%	10.038%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011716.D
 Acq On : 23 Sep 2017 21:37
 Operator : SJ/JU
 Sample : I5324-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

35	10.822	1279	1281	1283	rVB3	3416	2704	0.11%	0.019%
36	11.180	1340	1342	1346	rBV3	2005	2490	0.10%	0.017%
37	11.251	1349	1354	1356	rBV4	2373	4043	0.17%	0.028%
38	11.427	1381	1384	1389	rBV6	2529	4607	0.19%	0.032%
39	11.580	1407	1410	1411	rBV3	2724	2742	0.11%	0.019%
40	12.186	1509	1513	1515	rVB4	2359	3389	0.14%	0.023%
41	12.216	1515	1518	1521	rBV4	2243	3158	0.13%	0.022%
42	12.521	1566	1570	1571	rBV4	1992	2437	0.10%	0.017%
43	12.657	1590	1593	1596	rVB3	2337	3307	0.14%	0.023%
44	12.686	1596	1598	1603	rBV3	1946	2945	0.12%	0.020%
45	12.980	1644	1648	1650	rBV4	2921	4429	0.18%	0.031%
46	13.057	1656	1661	1665	rBV5	2462	5594	0.23%	0.039%
47	13.186	1681	1683	1686	rVB4	4616	4250	0.18%	0.029%
48	13.986	1812	1819	1830	rBV	146885	233091	9.69%	1.615%
49	14.180	1850	1852	1855	rBV3	2052	2661	0.11%	0.018%
50	14.274	1863	1868	1876	rBV	153116	232351	9.66%	1.610%
51	14.421	1887	1893	1901	rBV3	21588	55494	2.31%	0.385%
52	14.580	1913	1920	1939	rVB2	1058993	1685393	70.09%	11.679%
53	14.827	1958	1962	1963	rVV4	1865	2829	0.12%	0.020%
54	15.174	2019	2021	2024	rVB3	2432	2480	0.10%	0.017%
55	15.204	2024	2026	2030	rBV5	2495	3012	0.13%	0.021%
56	15.262	2035	2036	2039	rVB2	3748	3141	0.13%	0.022%
57	15.339	2043	2049	2051	rVV5	2330	3693	0.15%	0.026%
58	15.357	2051	2052	2059	rVB6	4584	5315	0.22%	0.037%
59	15.568	2082	2088	2097	rBV	209493	319229	13.28%	2.212%
60	15.686	2103	2108	2115	rBV3	47239	74845	3.11%	0.519%
61	15.798	2126	2127	2129	rBV2	2818	2643	0.11%	0.018%
62	15.815	2129	2130	2134	rVV4	4247	3988	0.17%	0.028%
63	15.862	2137	2138	2140	rVV2	2800	2577	0.11%	0.018%
64	16.015	2163	2164	2167	rVB3	4414	3910	0.16%	0.027%
65	16.239	2199	2202	2205	rBV4	2549	2685	0.11%	0.019%
66	16.392	2225	2228	2230	rBV4	2456	2488	0.10%	0.017%
67	16.439	2234	2236	2241	rVB5	3056	3175	0.13%	0.022%
68	16.474	2241	2242	2245	rBV3	2211	2542	0.11%	0.018%
69	16.533	2250	2252	2255	rBV4	2819	2875	0.12%	0.020%
70	16.609	2264	2265	2267	rBV	2852	2578	0.11%	0.018%
71	16.939	2318	2321	2323	rBV4	2721	2529	0.11%	0.018%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011716.D
 Acq On : 23 Sep 2017 21:37
 Operator : SJ/JU
 Sample : I5324-02DL 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT7DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

72	17.115	2348	2351	2353	rBV4	5390	7427	0.31%	0.051%
73	17.233	2368	2371	2376	rBV2	9192	11669	0.49%	0.081%
74	17.321	2380	2386	2397	rBV2	1366197	1981534	82.40%	13.731%
75	17.421	2397	2403	2415	rVB	241279	367381	15.28%	2.546%
76	17.698	2447	2450	2451	rBV2	2609	2527	0.11%	0.018%
77	17.839	2473	2474	2477	rBV3	2877	2674	0.11%	0.019%
78	17.862	2477	2478	2483	rVV5	2686	2960	0.12%	0.021%
79	17.933	2485	2490	2492	rBV5	2504	3203	0.13%	0.022%
80	18.127	2520	2523	2524	rVB3	3299	2838	0.12%	0.020%
81	18.145	2524	2526	2528	rBV2	2543	2762	0.11%	0.019%
82	18.192	2528	2534	2543	rBV8	20960	44391	1.85%	0.308%
83	18.274	2545	2548	2551	rBV5	2926	4636	0.19%	0.032%
84	18.356	2556	2562	2563	rBV6	3410	6941	0.29%	0.048%
85	18.398	2567	2569	2572	rBV4	4131	4546	0.19%	0.032%
86	18.609	2602	2605	2606	rBV3	2670	2422	0.10%	0.017%
87	18.774	2628	2633	2636	rBV5	3530	5919	0.25%	0.041%
88	18.798	2636	2637	2639	rBV2	3352	2651	0.11%	0.018%
89	18.886	2650	2652	2656	rBV5	4096	5119	0.21%	0.035%
90	19.315	2723	2725	2727	rBV3	4355	4162	0.17%	0.029%
91	19.462	2746	2750	2758	rBV8	31160	58076	2.42%	0.402%
92	19.703	2786	2791	2798	rBV	302117	433139	18.01%	3.001%
93	21.486	3089	3094	3100	rBV	1865237	2385188	99.19%	16.528%
94	23.691	3464	3469	3477	rVB3	338887	672230	27.96%	4.658%
95	23.844	3489	3495	3505	rVB	1211324	2404685	100.00%	16.664%


Sum of corrected areas: 14430821

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
Data File : BM011716.D
Acq On : 23 Sep 2017 21:37
Operator : SJ/JU
Sample : I5324-02DL 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT7DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

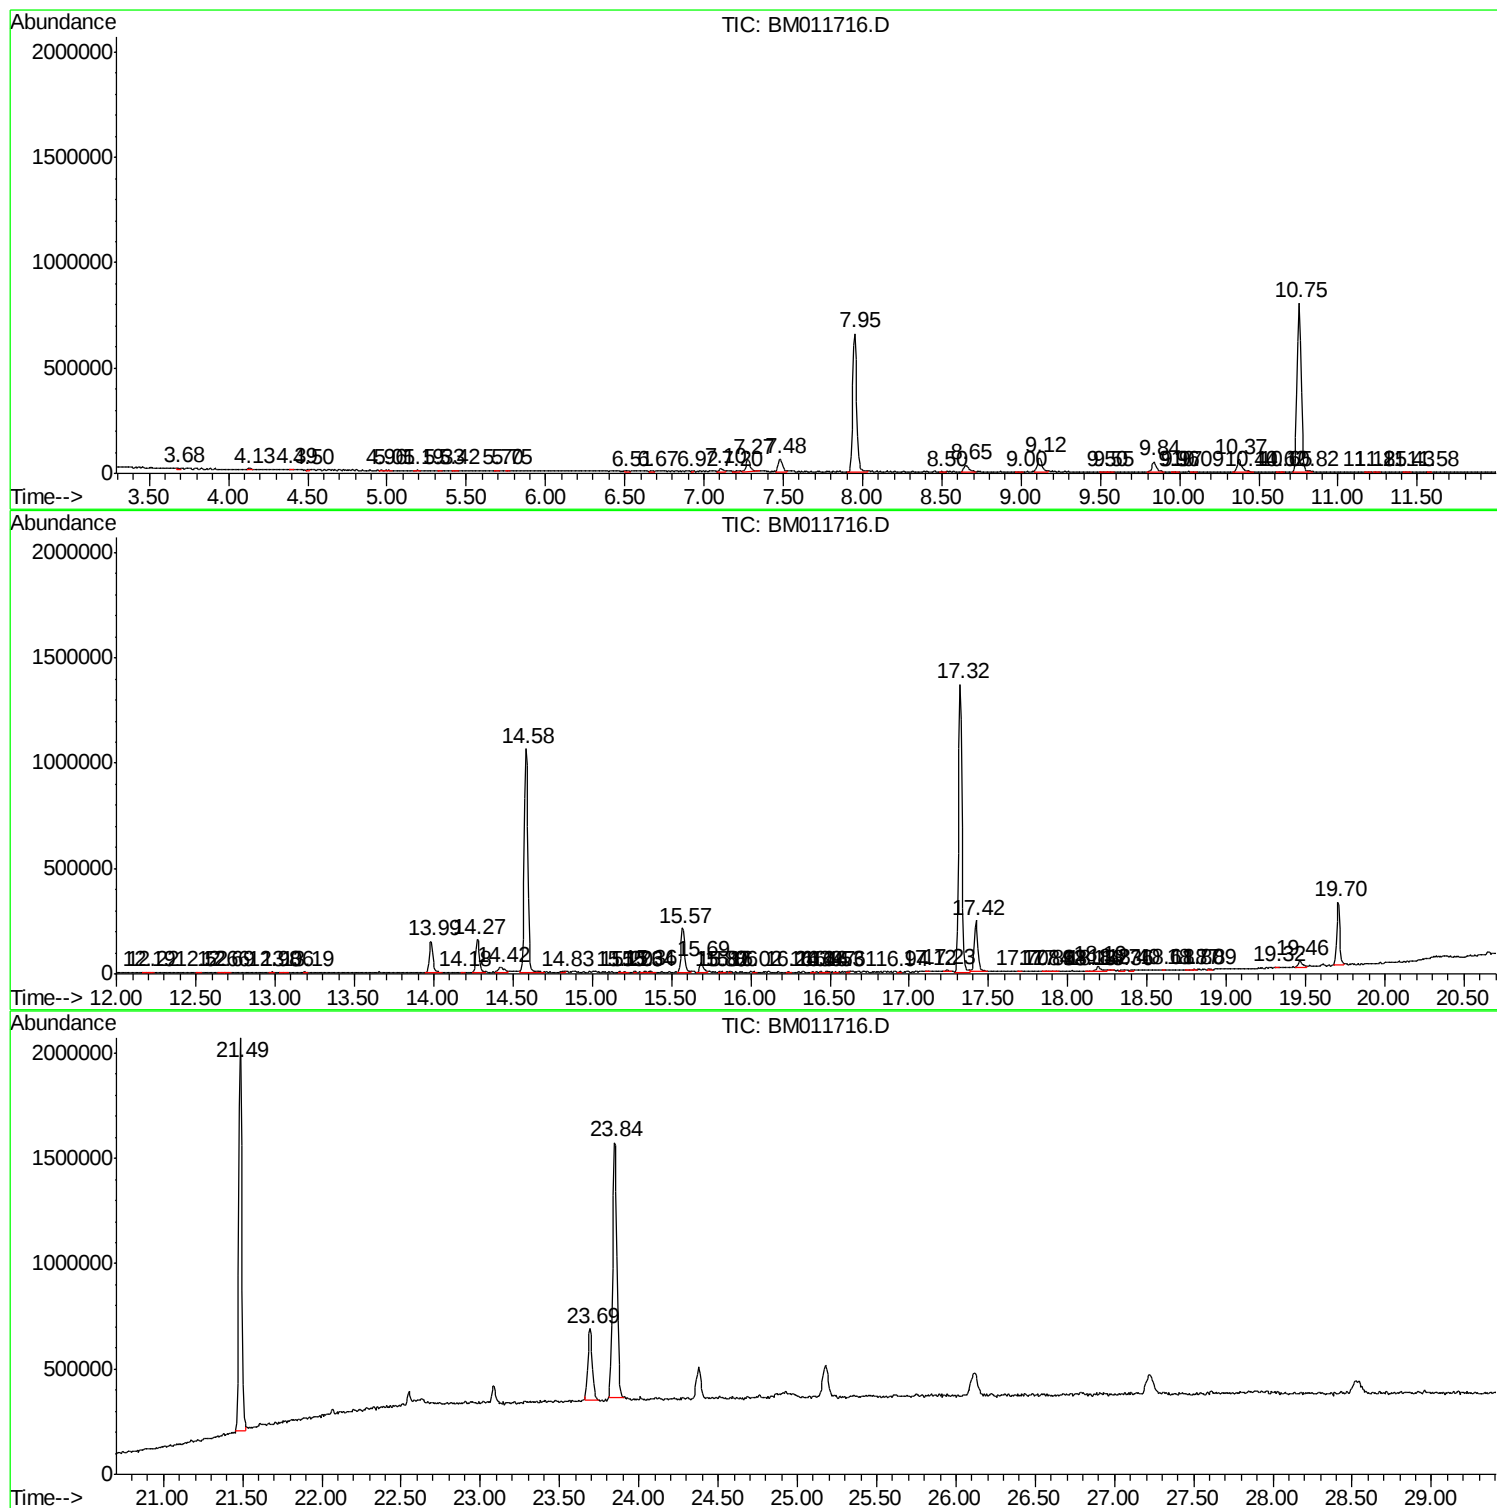

DbaaaPathh::ZZ\NRPBHHM1BBAAMMDAAABBB0023IX\
 DbaaaFile::BBB017766DD
 Aeqq00n ::233Spp2007 221337
 Oppaaaor ::SSJJUU
 Samplee ::I5324000DL100X
 Misc ::
 AASSVaal ::188 SampleeMMuifppler:11

Instrument :
 BNA_M
 ClientSampleId :
 C0AT7DL

QqaabtMebbdd::ZZ\NRPBHHM1BBAAMMMEH00SS00MEPRABBB00087MMAMM
 QqaabtTillee ::S00ACSAIBBATION

TICCLibbaayy ::CC\DATAABASSEN0SS002LL
 TICInteggaafionPaaaaaess:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
