

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011717.D
 Acq On : 23 Sep 2017 22:13
 Operator : SJ/JU
 Sample : I5324-03DL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.822	89	91	94	rBV4	4270	4773	0.20%	0.035%
2	4.081	134	135	139	rBV4	2511	2780	0.12%	0.021%
3	4.116	139	141	142	rVV2	5154	2780	0.12%	0.021%
4	4.134	142	144	147	rVV3	4485	4710	0.20%	0.035%
5	4.193	151	154	156	rBV4	3035	2812	0.12%	0.021%
6	4.228	158	160	162	rVB2	3729	2931	0.13%	0.022%
7	4.528	209	211	213	rVB3	3672	2467	0.11%	0.018%
8	4.587	220	221	224	rBV3	3117	3197	0.14%	0.024%
9	4.793	254	256	258	rBV2	2993	2576	0.11%	0.019%
10	4.963	284	285	288	rBV3	2113	2404	0.10%	0.018%
11	5.140	311	315	318	rBV5	3023	4312	0.18%	0.032%
12	5.752	417	419	422	rBV3	2622	2692	0.12%	0.020%
13	7.057	638	641	644	rBV5	2847	4136	0.18%	0.031%
14	7.110	644	650	654	rVB3	15095	22913	0.98%	0.170%
15	7.275	672	678	685	rBV	56416	101710	4.36%	0.756%
16	7.481	707	713	722	rBV	68289	117049	5.02%	0.870%
17	7.951	786	793	803	rBV	640716	1062224	45.51%	7.899%
18	8.234	839	841	845	rVB4	2646	2344	0.10%	0.017%
19	8.651	905	912	922	rBV2	31605	66838	2.86%	0.497%
20	8.834	940	943	946	rVB4	3700	4024	0.17%	0.030%
21	9.116	982	991	1005	rBV	64485	139823	5.99%	1.040%
22	9.510	1055	1058	1063	rVB5	3105	4329	0.19%	0.032%
23	9.575	1067	1069	1073	rVB5	1963	2471	0.11%	0.018%
24	9.839	1107	1114	1122	rBV2	47700	95740	4.10%	0.712%
25	10.375	1198	1205	1214	rBV2	59574	124653	5.34%	0.927%
26	10.469	1220	1221	1225	rVB3	2791	2815	0.12%	0.021%
27	10.516	1225	1229	1231	rBV4	2355	2652	0.11%	0.020%
28	10.751	1262	1269	1282	rBV	774356	1359420	58.24%	10.109%
29	10.869	1287	1289	1292	rVB2	2285	2532	0.11%	0.019%
30	11.628	1413	1418	1419	rVB3	1890	2572	0.11%	0.019%
31	12.292	1529	1531	1534	rBV3	2270	2619	0.11%	0.019%
32	12.569	1572	1578	1580	rBV4	2237	3129	0.13%	0.023%
33	12.639	1587	1590	1595	rVB4	1586	2523	0.11%	0.019%
34	12.780	1609	1614	1618	rBV3	2073	3011	0.13%	0.022%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011717.D
 Acq On : 23 Sep 2017 22:13
 Operator : SJ/JU
 Sample : I5324-03DL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

35	12.933	1636	1640	1642	rBV2	2545	2610	0.11%	0.019%
36	13.186	1680	1683	1686	rBV3	2964	3025	0.13%	0.022%
37	13.369	1711	1714	1718	rVB3	1943	2450	0.10%	0.018%
38	13.410	1718	1721	1723	rBV3	2039	2519	0.11%	0.019%
39	13.580	1745	1750	1754	rBV6	2018	3358	0.14%	0.025%
40	13.639	1756	1760	1764	rBV3	1869	3122	0.13%	0.023%
41	13.727	1773	1775	1778	rVB3	2473	2521	0.11%	0.019%
42	13.763	1778	1781	1785	rVV2	2286	2526	0.11%	0.019%
43	13.804	1785	1788	1791	rVV5	3253	3675	0.16%	0.027%
44	13.857	1793	1797	1800	rBV5	3411	4761	0.20%	0.035%
45	13.892	1800	1803	1804	rVV3	3683	2711	0.12%	0.020%
46	13.933	1808	1810	1813	rVV2	2968	3010	0.13%	0.022%
47	13.986	1813	1819	1828	rVV	136684	212408	9.10%	1.579%
48	14.080	1831	1835	1837	rVB4	3368	4210	0.18%	0.031%
49	14.275	1862	1868	1876	rBV	138692	222327	9.53%	1.653%
50	14.422	1885	1893	1906	rBV6	17917	58175	2.49%	0.433%
51	14.580	1913	1920	1929	rVV2	979793	1546661	66.27%	11.501%
52	14.651	1929	1932	1934	rVV3	2686	3119	0.13%	0.023%
53	14.827	1959	1962	1964	rBV4	3124	3991	0.17%	0.030%
54	15.016	1991	1994	1996	rVB4	2246	3006	0.13%	0.022%
55	15.157	2014	2018	2021	rBV4	2331	2742	0.12%	0.020%
56	15.263	2033	2036	2038	rBV3	2297	3415	0.15%	0.025%
57	15.363	2050	2053	2057	rVB4	3076	4645	0.20%	0.035%
58	15.574	2083	2089	2096	rBV	188027	294596	12.62%	2.191%
59	15.686	2104	2108	2118	rBV4	39309	64105	2.75%	0.477%
60	15.792	2123	2126	2127	rBV2	3314	3738	0.16%	0.028%
61	15.916	2144	2147	2149	rBV4	3095	2807	0.12%	0.021%
62	15.986	2155	2159	2161	rBV5	2341	2731	0.12%	0.020%
63	16.057	2168	2171	2172	rBV2	1930	2412	0.10%	0.018%
64	16.151	2186	2187	2190	rVB3	3418	2512	0.11%	0.019%
65	16.174	2190	2191	2195	rBV3	2065	2998	0.13%	0.022%
66	16.274	2205	2208	2215	rVB5	3896	5818	0.25%	0.043%
67	16.521	2249	2250	2253	rVB3	2887	2376	0.10%	0.018%
68	16.939	2320	2321	2324	rVB3	3175	2875	0.12%	0.021%
69	17.021	2332	2335	2336	rBV2	2953	2944	0.13%	0.022%
70	17.121	2344	2352	2358	rBV7	5654	12484	0.53%	0.093%
71	17.168	2358	2360	2362	rVB3	3098	2480	0.11%	0.018%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
 Data File : BM011717.D
 Acq On : 23 Sep 2017 22:13
 Operator : SJ/JU
 Sample : I5324-03DL 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AT8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
 Title : SVOA CALIBRATION

72	17.186	2362	2363	2365	rBV2	3060	2340	0.10%	0.017%
73	17.239	2365	2372	2377	rBV7	7639	13814	0.59%	0.103%
74	17.321	2379	2386	2397	rBV2	1246208	1830338	78.42%	13.611%
75	17.421	2397	2403	2413	rVB	213297	338182	14.49%	2.515%
76	17.663	2443	2444	2447	rBV3	3221	3356	0.14%	0.025%
77	17.815	2467	2470	2471	rBV3	2507	2951	0.13%	0.022%
78	17.927	2486	2489	2492	rVB3	3964	4501	0.19%	0.033%
79	18.051	2508	2510	2513	rBV4	3773	4953	0.21%	0.037%
80	18.192	2531	2534	2537	rBV3	11004	15159	0.65%	0.113%
81	18.268	2546	2547	2550	rBV3	3742	3639	0.16%	0.027%
82	18.310	2552	2554	2558	rBV4	2162	2660	0.11%	0.020%
83	18.380	2561	2566	2568	rBV6	2924	4812	0.21%	0.036%
84	18.533	2590	2592	2598	rBV7	3090	5723	0.25%	0.043%
85	18.804	2636	2638	2642	rBV4	2700	3420	0.15%	0.025%
86	18.986	2666	2669	2671	rBV3	3678	4943	0.21%	0.037%
87	19.057	2678	2681	2682	rBV3	3235	3606	0.15%	0.027%
88	19.462	2746	2750	2754	rBV6	20402	30976	1.33%	0.230%
89	19.704	2786	2791	2800	rBV	272223	396319	16.98%	2.947%
90	21.486	3089	3094	3100	rBV	1744611	2234739	95.75%	16.618%
91	23.692	3464	3469	3478	rVB3	258305	533669	22.87%	3.968%
92	23.850	3489	3496	3508	rVB	1150262	2333978	100.00%	17.356%


Sum of corrected areas: 13447902

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092317\
Data File : BM011717.D
Acq On : 23 Sep 2017 22:13
Operator : SJ/JU
Sample : I5324-03DL 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AT8DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM090817MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

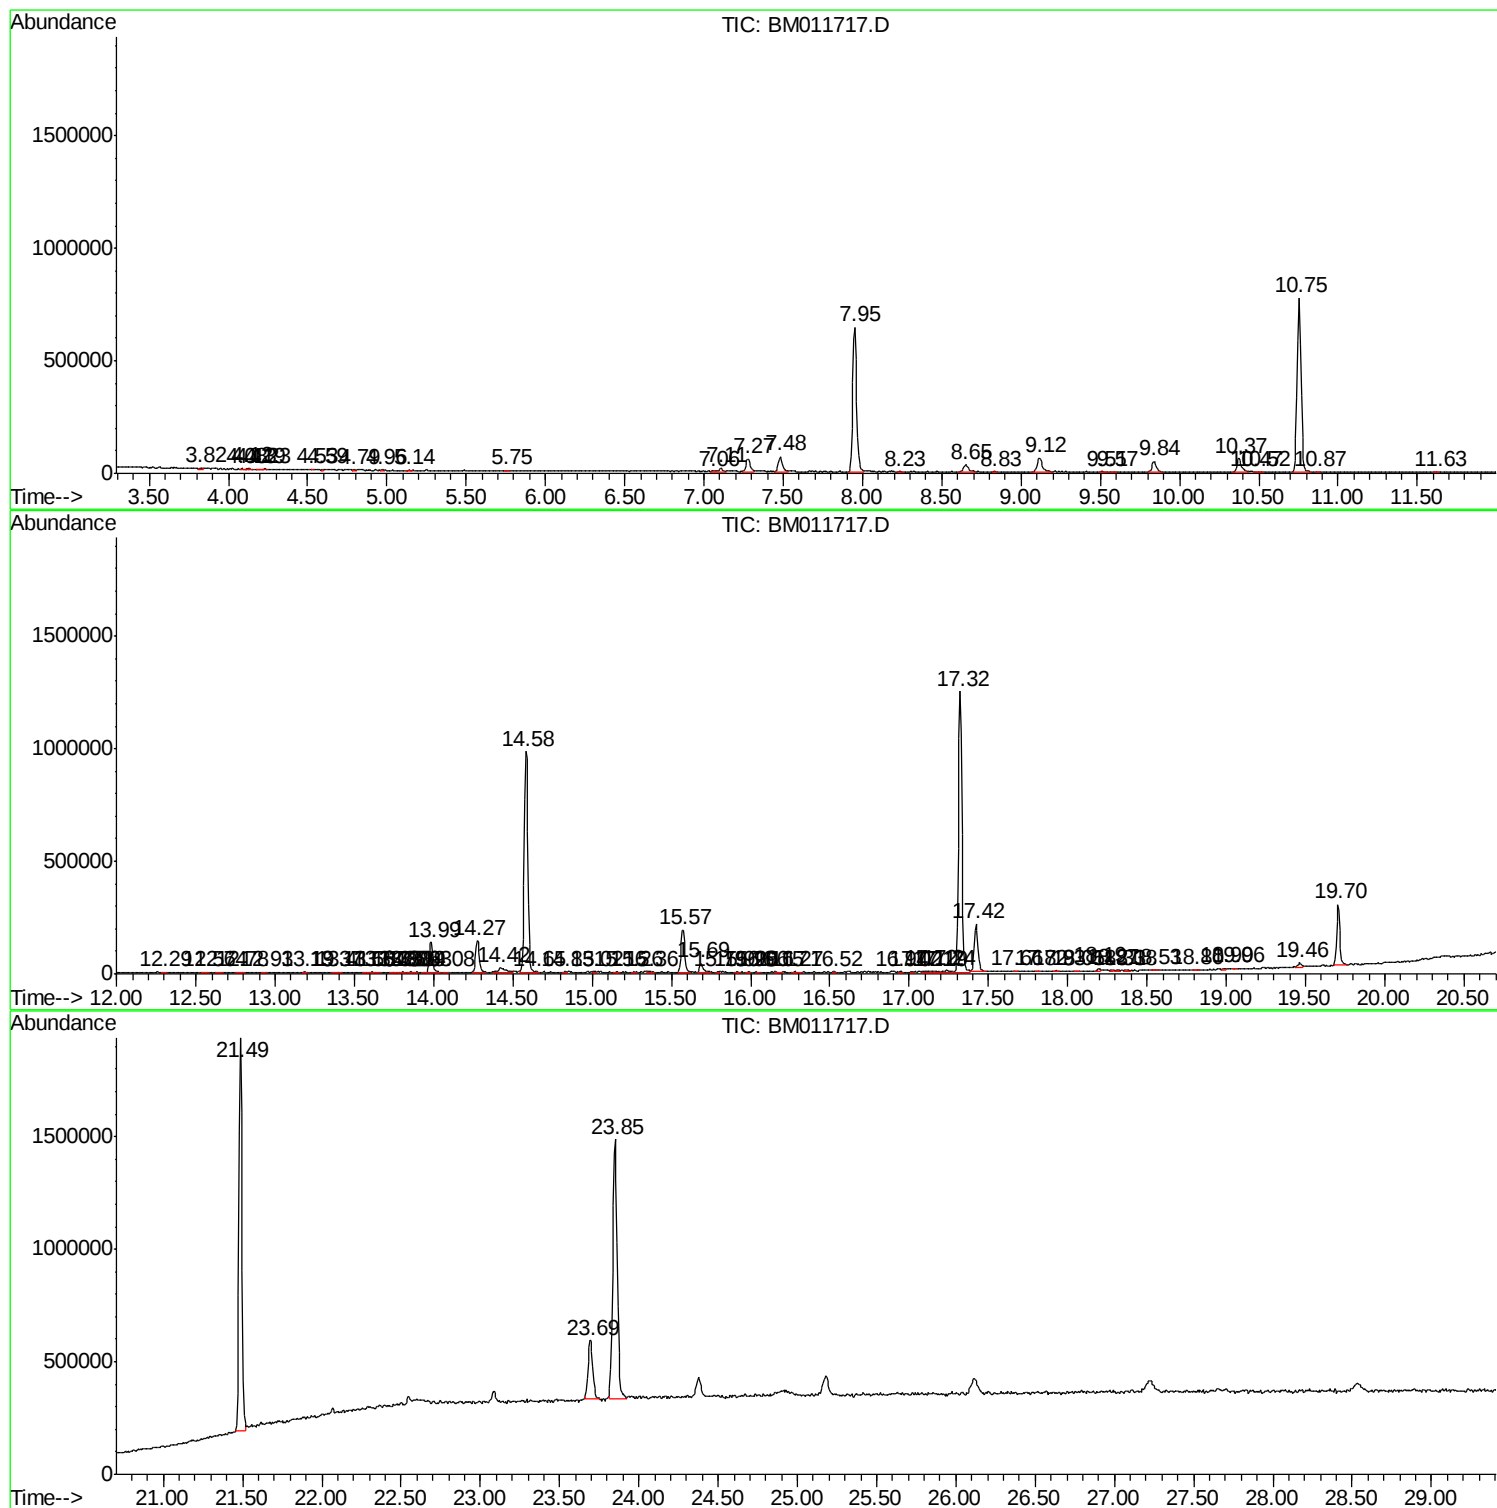

DbaaaPathh::ZZ\NRPBEMM1BBAAMMDAAABEM0023IX\
 DbaaaFile::BEM01777DD
 Aeqq00n ::233Spp2007 222133
 Opeaaor ::SSJUU
 Sample ::I532400DL10X
 Misc ::
 AASSVaal ::199 SampleMMultiplicier:11

Instrument :
 BNA_M
 ClientSampleId :
 C0AT8DL

QqaabMebbdd::ZZ\NRPBEMM1BBAAMMMEH00SS00MEPRABEM0008IMMAMM
 QqaabTitle ::S00ACSAIBRATION

TICLibrary :CC\DATA\BASSEN055002LL
 TICIntegratíonParameters:LS6CNTTP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
