


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092320\
Data File : BM027502.D
Acq On : 23 Sep 2020 15:04
Operator : JU/CG
Sample : PB131671BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Manual Integrations
APPROVED

mohammad
9/24/2020 10:47:53 AM

Quant Time: Sep 23 15:37:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 13:53:59 2020
Response via : Initial Calibration

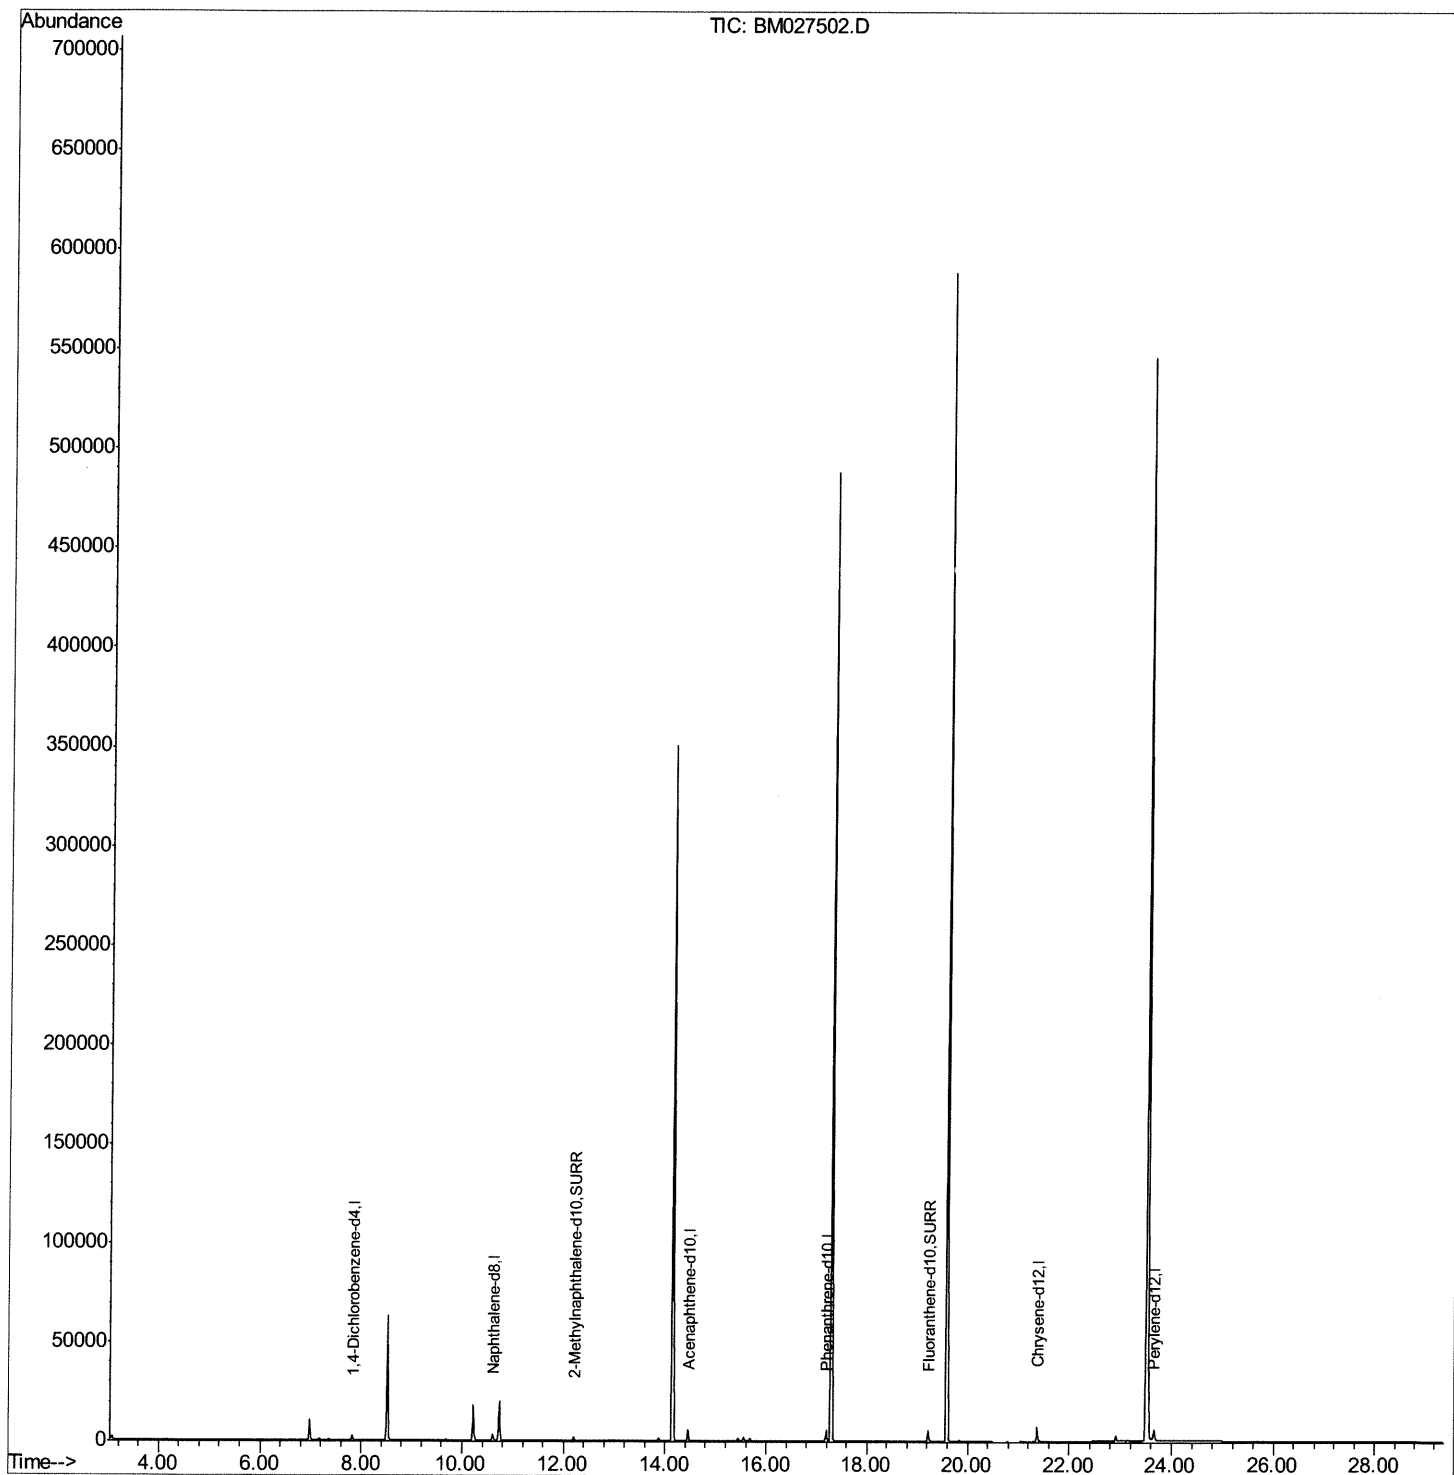

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092320\
 Data File : BM027502.D
 Acq On : 23 Sep 2020 15:04
 Operator : JU/CG
 Sample : PB131671BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 SBLK71

Manual Integrations
APPROVED

mohammad
 9/24/2020 10:47:53 AM

Quant Time: Sep 23 15:36:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 13:53:59 2020
 Response via : Initial Calibration

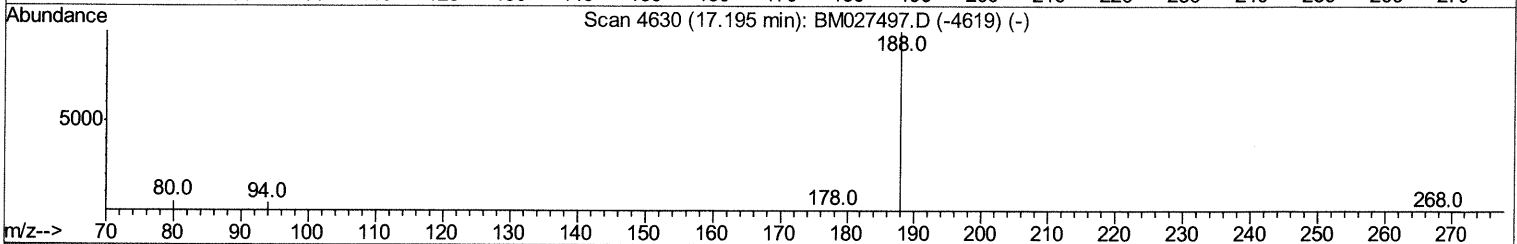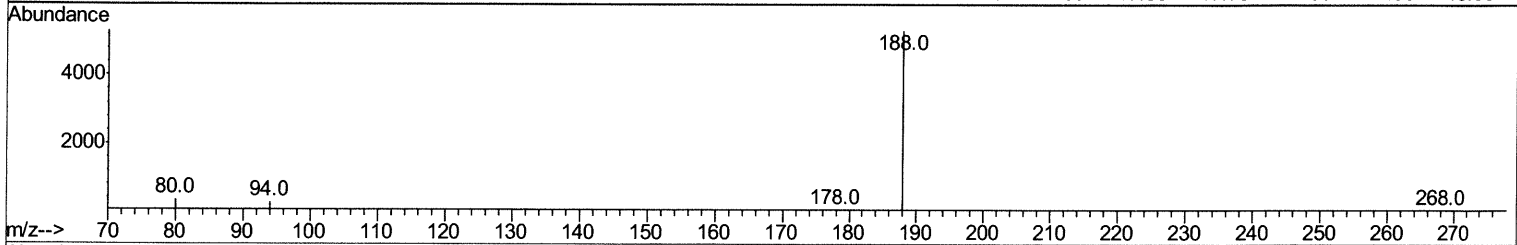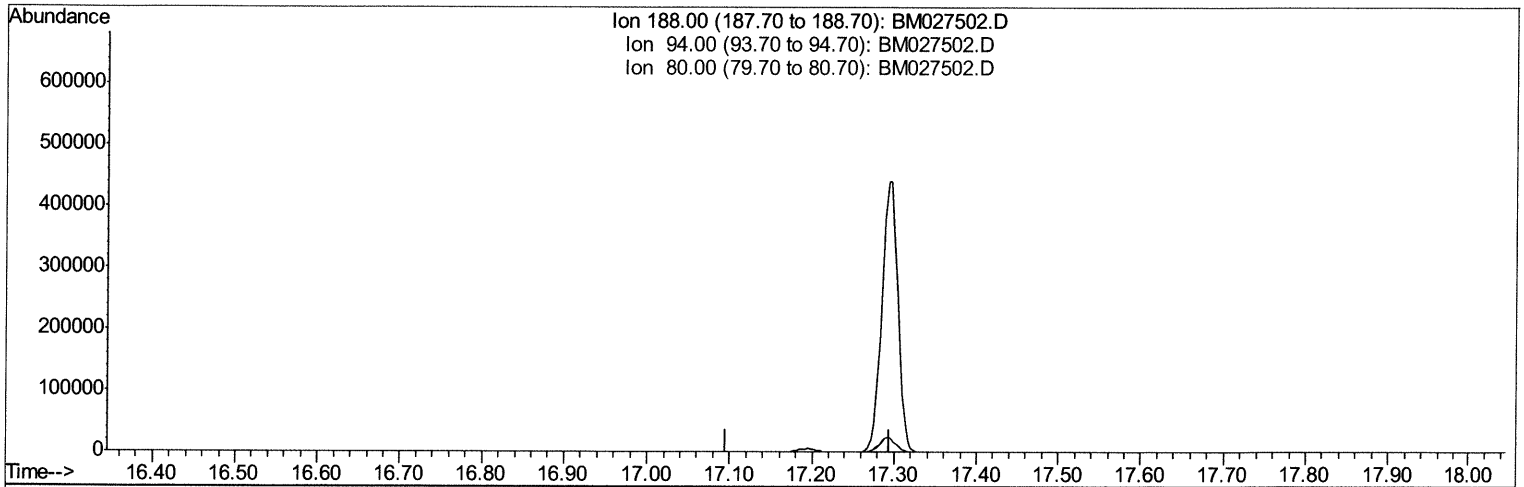

TIC: BM027502.D

(10) Phenanthrene-d10 (I)

17.195min (-17.195) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	5.20	0.00#
80.00	6.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092320\
 Data File : BM027502.D
 Acq On : 23 Sep 2020 15:04
 Operator : JU/CG
 Sample : PB131671BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK71

Manual Integrations
 APPROVED

mohammad
 9/24/2020 10:47:53 AM

Quant Time: Sep 23 15:36:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 13:53:59 2020
 Response via : Initial Calibration

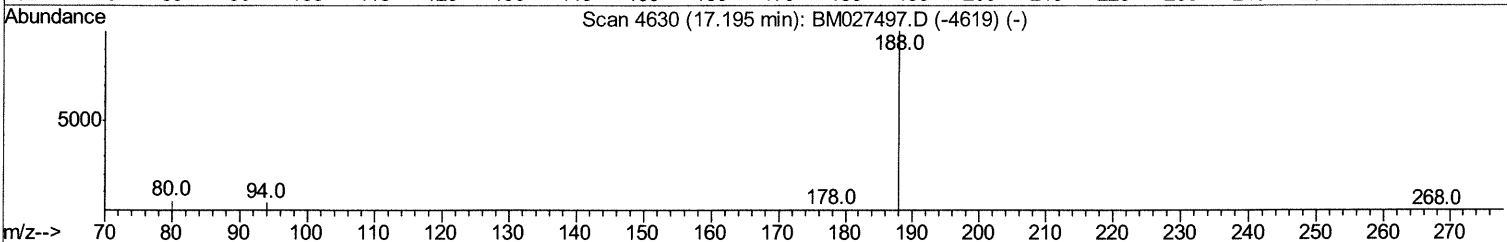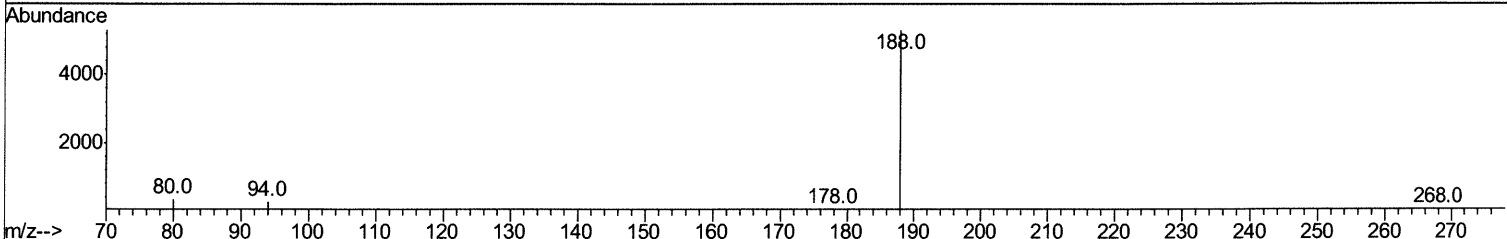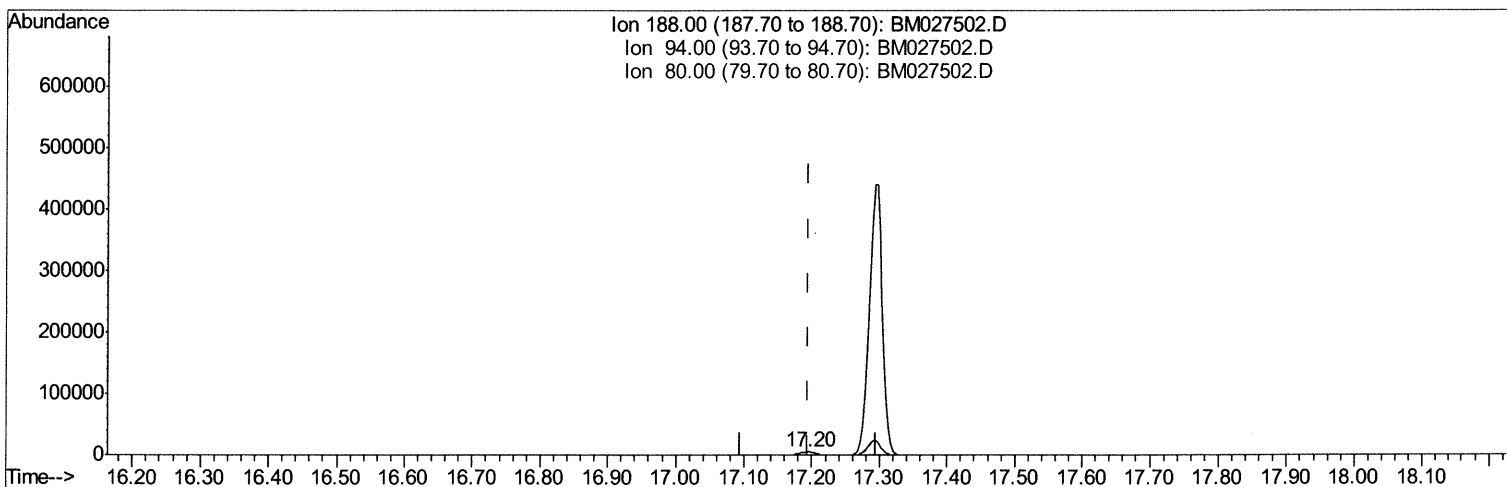

TIC: BM027502.D

(10) Phenanthrene-d10 (I)

17.195min (-0.000) 0.40ng/ul m 9/24/20 JU

response 7725

Ion	Exp%	Act%
188.00	100	100
94.00	5.20	5.16
80.00	6.20	6.60
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092320\
Data File : BM027502.D
Acq On : 23 Sep 2020 15:04
Operator : JU/CG
Sample : PB131671BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK71

Manual Integrations
APPROVED

mohammad
9/24/2020 10:47:53 AM

Quant Time: Sep 23 15:37:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 13:53:59 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1425	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	4364	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.45	164	3184	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.20	188	7725m>	0.40	ng/ul>	0.00
16) Chrysene-d12	21.38	240	7217	0.40	ng/ul	0.00
20) Perylene-d12	23.66	264	8043	0.40	ng/ul	0.00

9/24/20 JU

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.20	152	2295	0.29	ng/ul	0.00
14) Fluoranthene-d10	19.22	212	6751	0.32	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed