

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092320\
 Data File : BM027508.D
 Acq On : 23 Sep 2020 18:42
 Operator : JU/CG
 Sample : L4001-06MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETYP2MSD

Quant Time: Sep 23 19:34:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 23 13:53:59 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	1658	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	4914	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.45	164	3240	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.19	188	7808	0.40	ng/ul	0.00
16) Chrysene-d12	21.37	240	7289	0.40	ng/ul	0.00
20) Perylene-d12	23.64	264	7589	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.20	152	2350	0.26	ng/ul	0.00
14) Fluoranthene-d10	19.21	212	7421	0.35	ng/ul	0.00
Target Compounds				Ovalue		
8) Acenaphthene	14.51	153	2826	0.240	ng/ul	99
11) Pentachlorophenol	16.84	266	672	0.316	ng/ul	99
17) Pyrene	19.61	202	9143	0.275	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM092320\
Data File : BM027508.D
Acq On : 23 Sep 2020 18:42
Operator : JU/CG
Sample : L4001-06MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETYP2MSD

Quant Time: Sep 23 19:34:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM092320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 23 13:53:59 2020
Response via : Initial Calibration

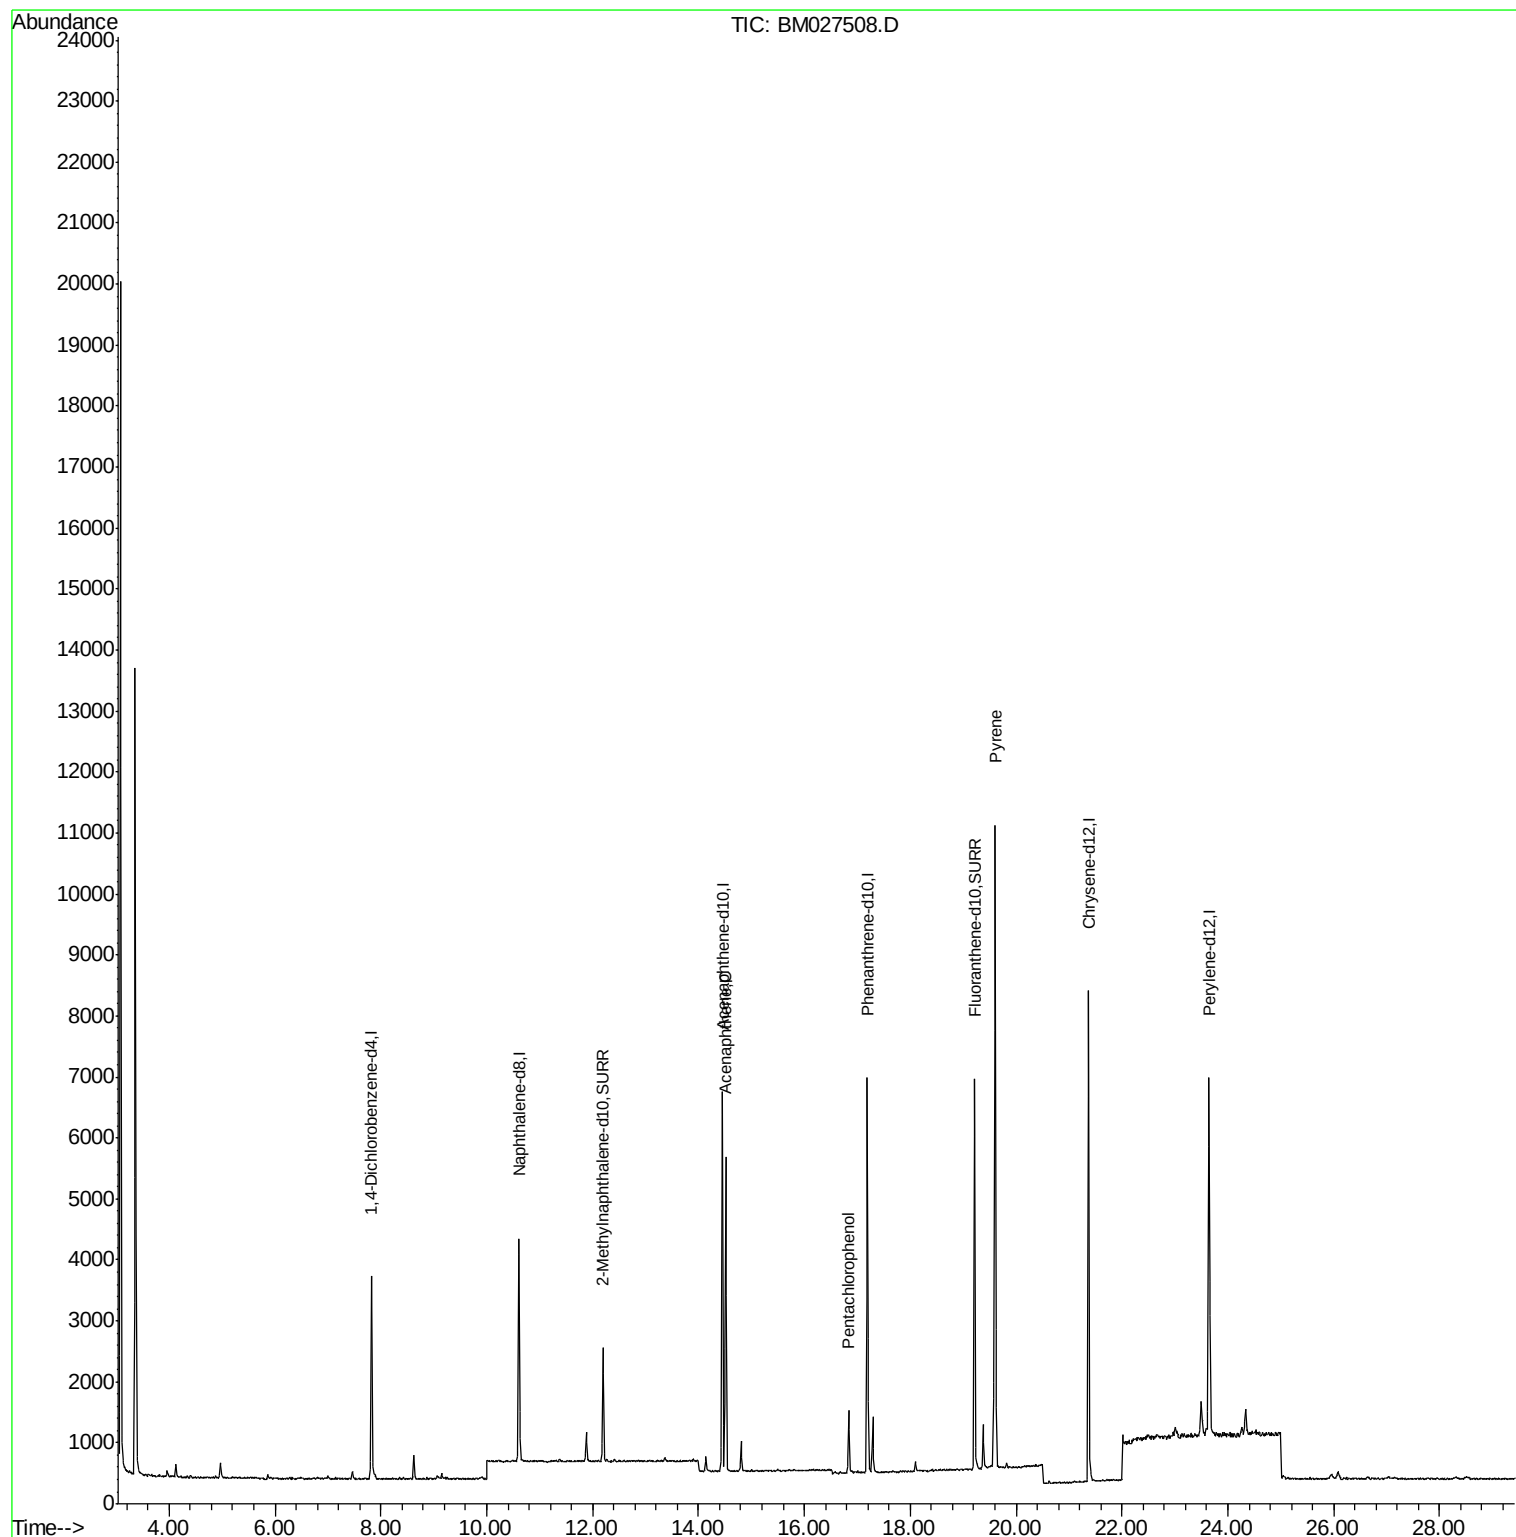

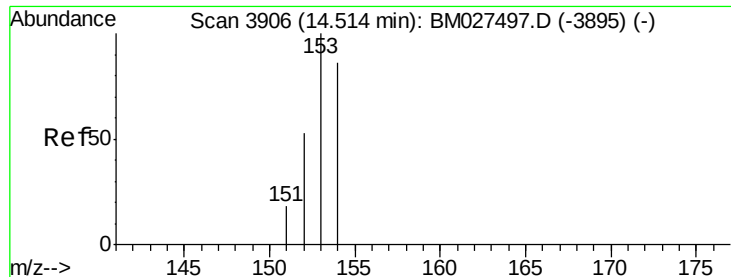

#8

Acenaphthene

Concen: 0.240 ng/ul

RT: 14.51 min Scan# 3906

Delta R.T. -0.00 min

Lab File: BM027508.D

Acq: 23 Sep 2020 18:42

Instrument :

BNA_M

ClientSampled :

ETYP2MSD


Tot Ion:153 Resp: 2826

Ion Ratio Lower Upper

153 100

152 52.6 42.8 64.2




154 86.7 69.0 103.6

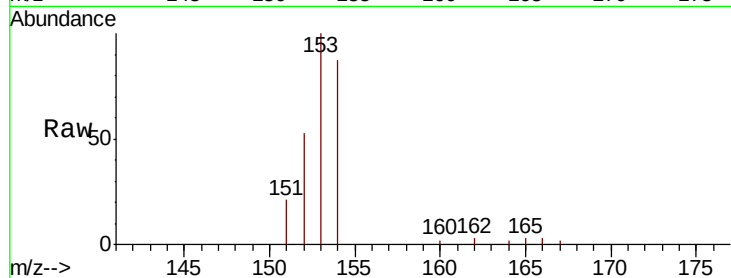

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

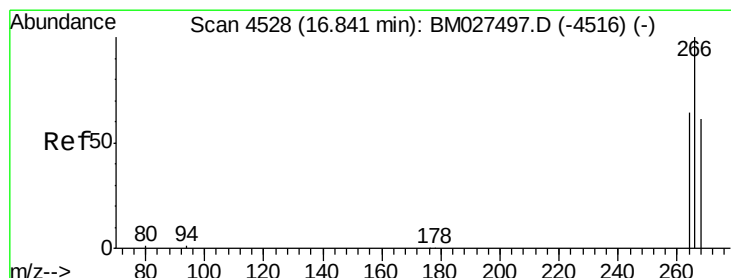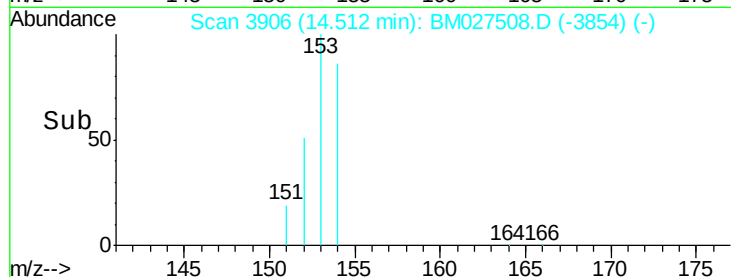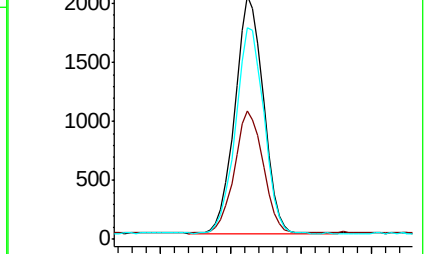

#11

Pentachlorophenol

Concen: 0.316 ng/ul

RT: 16.84 min Scan# 4527

Delta R.T. -0.01 min

Lab File: BM027508.D

Acq: 23 Sep 2020 18:42


Tgt Ion:266 Resp: 672

Ion Ratio Lower Upper

266 100

264 63.7 50.2 75.4



268 64.1 50.2 75.4

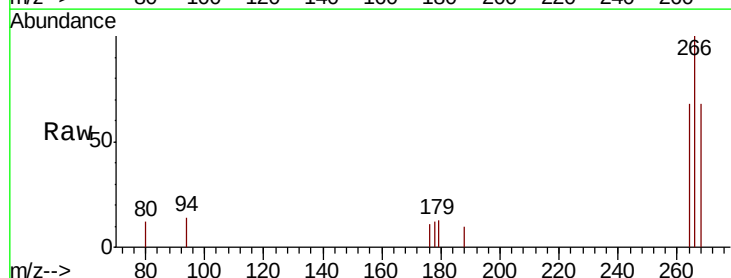


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

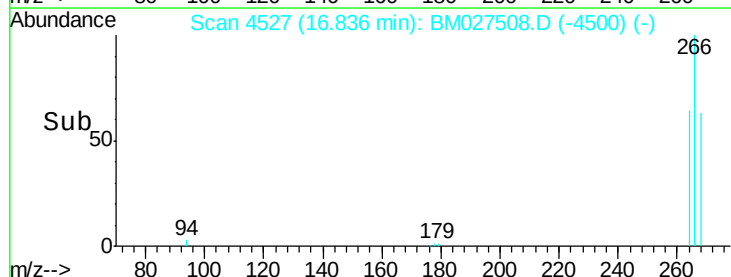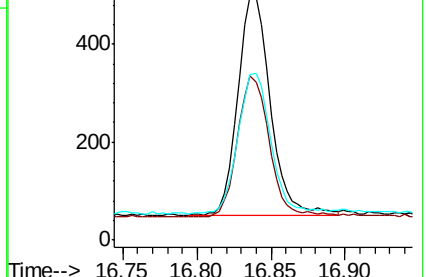

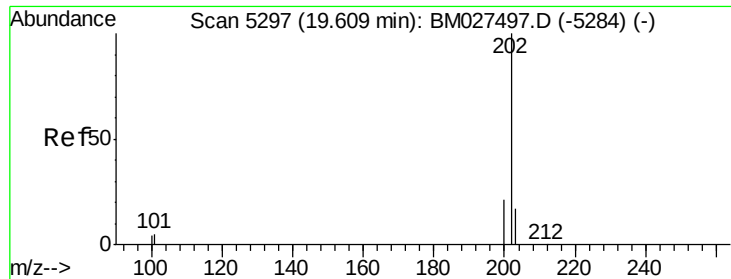

#17

Pvrene

Concen: 0.275 ng/ul

RT: 19.61 min Scan# 5297

Delta R.T. -0.00 min

Lab File: BM027508.D

Acq: 23 Sep 2020 18:42

Instrument :

BNA_M

ClientSampleId :

ETYP2MSD

Tot Ion: 202 Resp: 9143

Ion Ratio Lower Upper

202 100

101 5.4 4.7 7.1

100 5.1 3.9 5.9

