

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036673.D
 Acq On : 23 Sep 2022 12:38
 Operator : CG/JU
 Sample : N4595-04DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8G9DL

Quant Time: Sep 23 23:35:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	501599	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2249367	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.639	164	1368686	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.374	188	2661265	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1946470	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	1644828	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	4967	0.371	ng/uL	0.00
4) Pyridine-d5	3.834	84	41960	1.075	ng/u1	0.02
7) Phenol-d5	7.169	99	52262	1.166	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	150885	5.543	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	149071	4.619	ng/u1	-0.01
15) 4-Methylphenol-d8	8.722	113	100670	3.039	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	92898	6.102	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	79358	5.819	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	161990	5.126	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	129661	2.468	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	580593	6.290	ng/u1	0.00
49) Acenaphthylene-d8	14.333	160	650380	5.940	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	13951	0.779	ng/u1	0.00
60) Fluorene-d10	15.627	176	512631	6.197	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	42980	4.082	ng/u1	0.00
73) Anthracene-d10	17.474	188	737495	6.061	ng/u1	0.00
81) Pyrene-d10	19.756	212	784117	8.188	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	501740	6.244	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	340735	23.640	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036673.D
Acq On : 23 Sep 2022 12:38
Operator : CG/JU
Sample : N4595-04DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G9DL

Quant Time: Sep 23 23:35:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

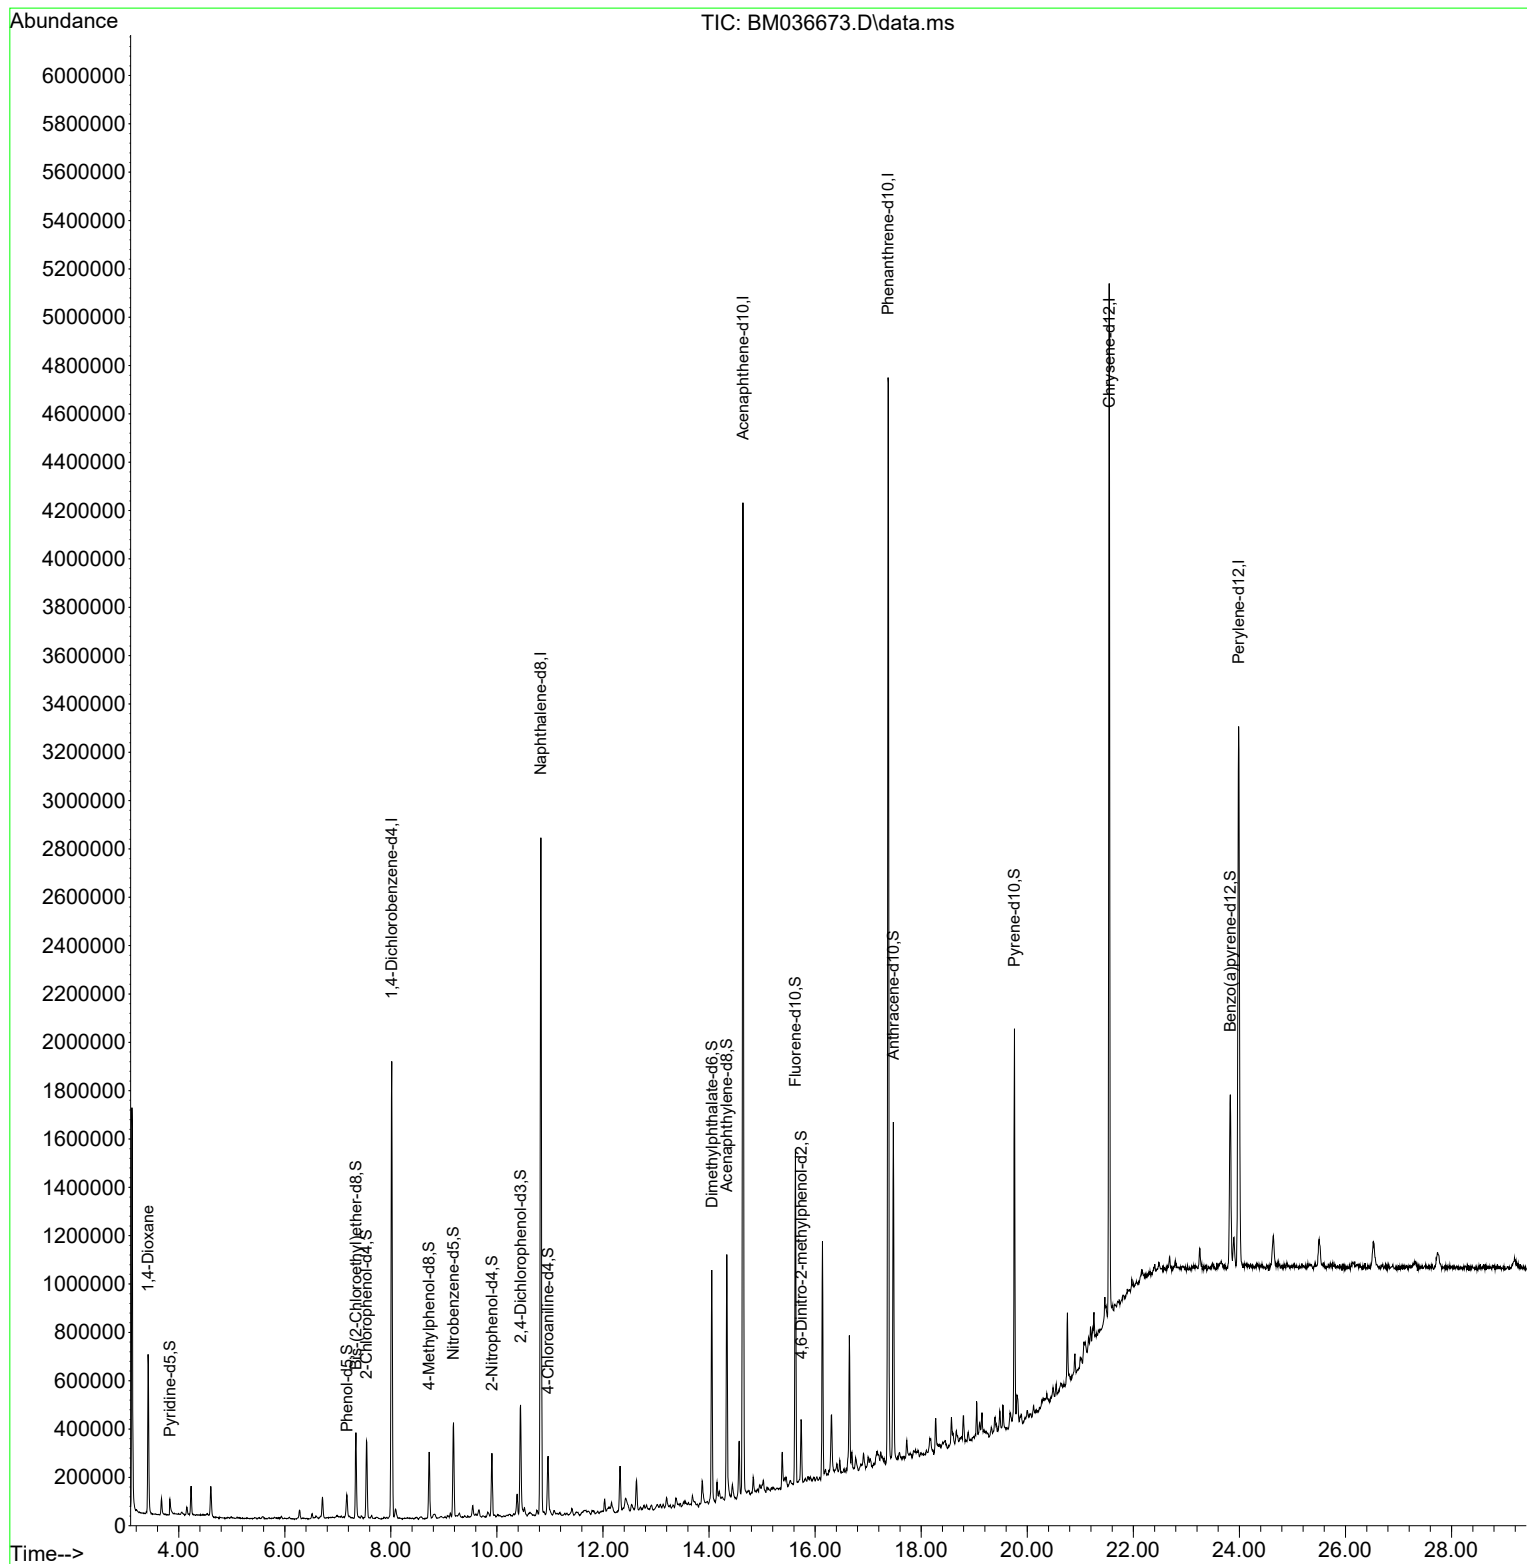

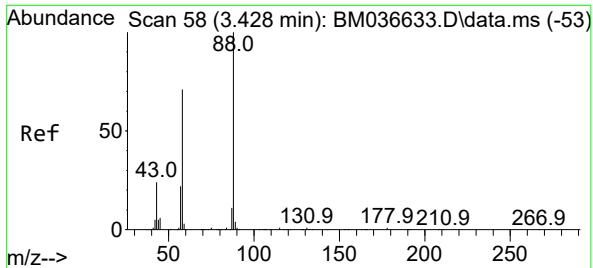

#2
 1,4-Dioxane
 Concen: 23.640 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. -0.006 min
 Lab File: BM036673.D
 Acq: 23 Sep 2022 12:38

Instrument :
 BNA_M
 ClientSampleId :
 CB8G9DL

Tgt Ion: 88	Resp: 340735
Ion Ratio	Lower Upper
88 100	
43 25.8	23.1 34.7
58 68.9	56.6 85.0

