

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036674.D
 Acq On : 23 Sep 2022 13:15
 Operator : CG/JU
 Sample : N4595-06DL 2X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8H4DL

Quant Time: Sep 23 23:35:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	496332	20.000	ng/u1	0.00
20) Naphthalene-d8	10.827	136	2196925	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.639	164	1329066	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2612524	20.000	ng/u1	0.00
79) Chrysene-d12	21.544	240	1983644	20.000	ng/u1	0.00
88) Perylene-d12	23.985	264	1763516	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	12073	0.912	ng/uL	0.00
4) Pyridine-d5	3.828	84	103311	2.676	ng/u1	0.01
7) Phenol-d5	7.169	99	141299	3.186	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.345	67	353777	13.134	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	372179	11.655	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	271349	8.279	ng/u1	0.00
21) Nitrobenzene-d5	9.180	128	239654	16.117	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	222181	16.681	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	454297	14.718	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	385401	7.510	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	1547776	17.267	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	1814601	17.066	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	42481	2.443	ng/u1	0.00
60) Fluorene-d10	15.627	176	1368352	17.034	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	150822	14.592	ng/u1	0.00
73) Anthracene-d10	17.474	188	2008597	16.815	ng/u1	0.00
81) Pyrene-d10	19.762	212	2135315	21.881	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	1525745	17.709	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	285504	20.018	ng/uL	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036674.D
Acq On : 23 Sep 2022 13:15
Operator : CG/JU
Sample : N4595-06DL 2X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8H4DL

Quant Time: Sep 23 23:35:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

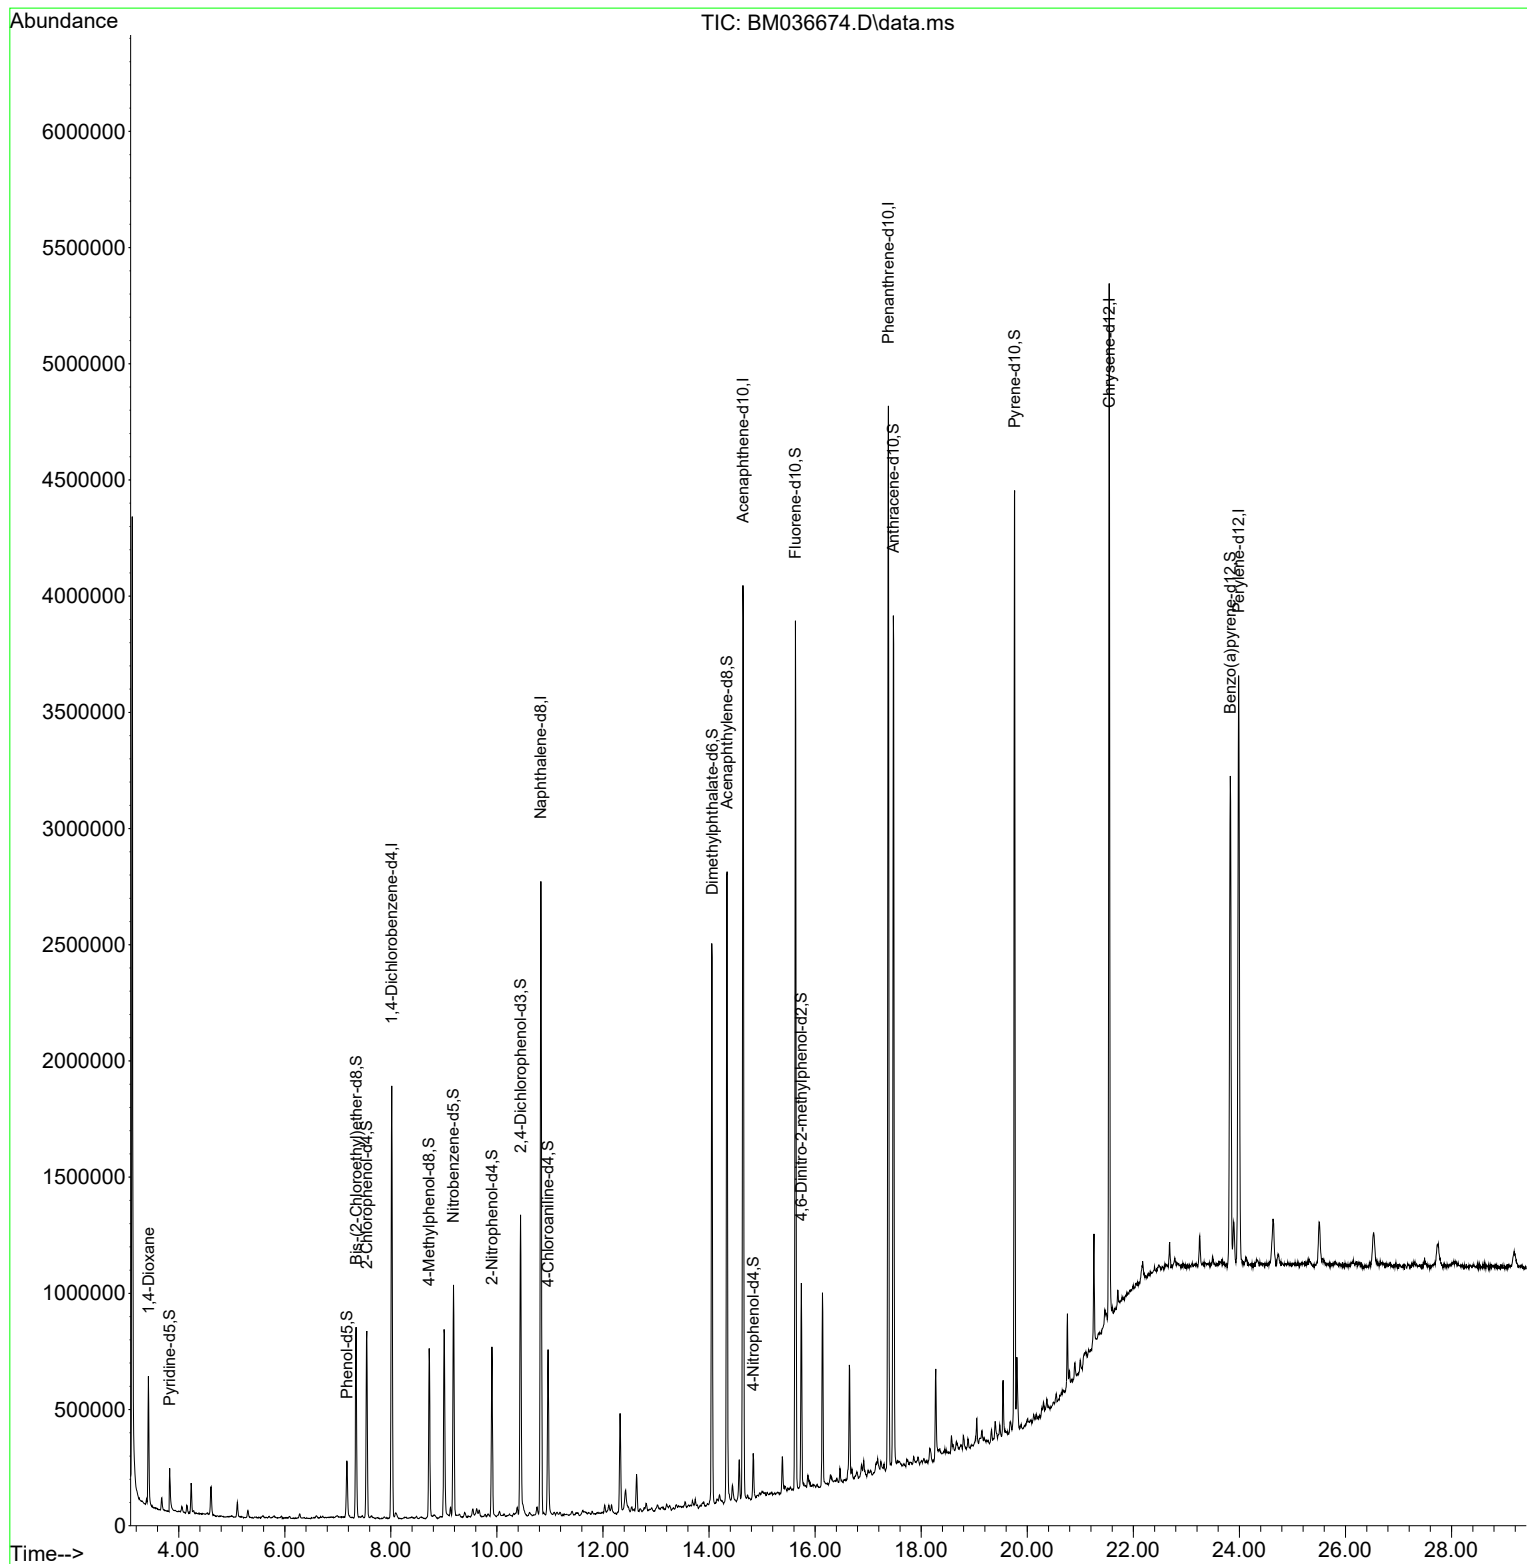

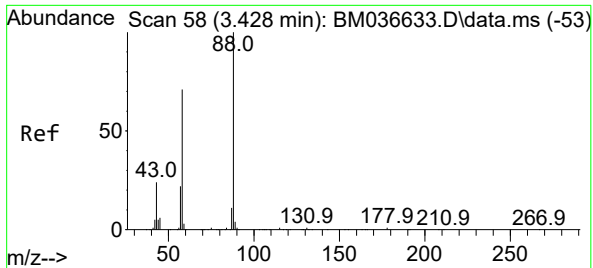

#2
 1,4-Dioxane
 Concen: 20.018 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM036674.D
 Acq: 23 Sep 2022 13:15

Instrument :
 BNA_M
 ClientSampleId :
 CB8H4DL

Tgt Ion:	88	Resp:	285504
Ion	Ratio	Lower	Upper
88	100		
43	25.7	23.1	34.7
58	69.1	56.6	85.0

