

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036676.D
 Acq On : 23 Sep 2022 14:29
 Operator : CG/JU
 Sample : N4706-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8J9

Quant Time: Sep 23 23:35:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	448333	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	1994019	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.639	164	1226767	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2355441	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1707352	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	1457048	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	46942	3.925	ng/uL	0.00
4) Pyridine-d5	3.822	84	489325	14.029	ng/u1	0.00
7) Phenol-d5	7.175	99	217818	5.437	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	592259	24.341	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	506246	17.551	ng/u1	0.00
15) 4-Methylphenol-d8	8.722	113	384705	12.995	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	390277	28.917	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	291345	24.100	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	567848	20.268	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	981790	21.077	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2496071	30.168	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	2780047	28.327	ng/u1	0.00
54) 4-Nitrophenol-d4	14.839	143	65296	4.069	ng/u1	0.01
60) Fluorene-d10	15.627	176	2124696	28.655	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	130753	14.031	ng/u1	0.00
73) Anthracene-d10	17.474	188	3216928	29.870	ng/u1	0.00
81) Pyrene-d10	19.756	212	3381987	40.264	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	2275471	31.966	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	376095	29.193	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036676.D
Acq On : 23 Sep 2022 14:29
Operator : CG/JU
Sample : N4706-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8J9

Quant Time: Sep 23 23:35:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

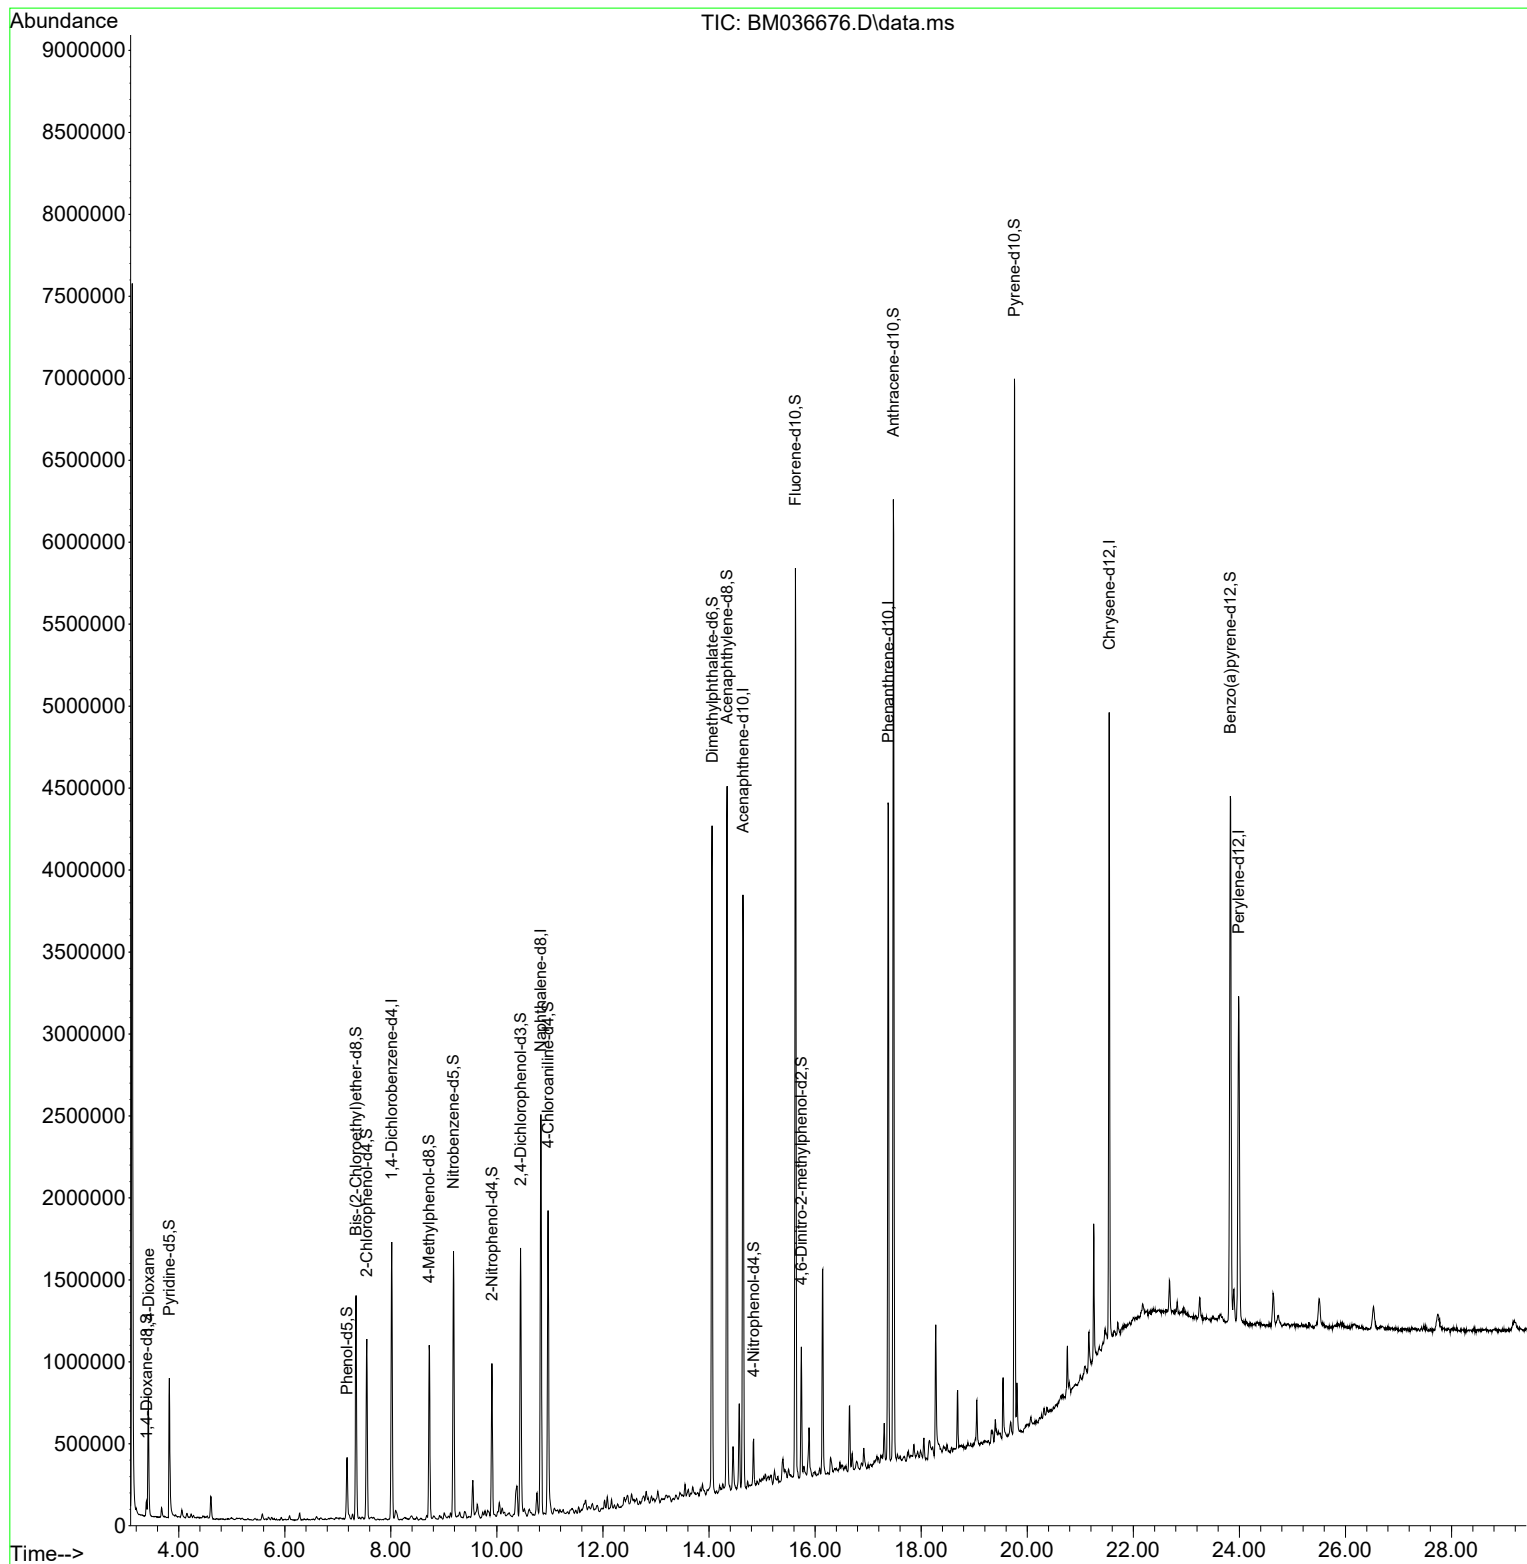

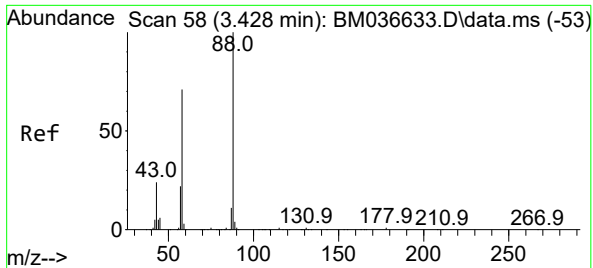

#2
 1,4-Dioxane
 Concen: 29.193 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM036676.D
 Acq: 23 Sep 2022 14:29

Instrument :
 BNA_M
 ClientSampleId :
 CB8J9

Tgt Ion: 88 Resp: 376095

Ion	Ratio	Lower	Upper
88	100		
43	25.4	23.1	34.7
58	68.1	56.6	85.0

