

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036678.D
 Acq On : 23 Sep 2022 15:42
 Operator : CG/JU
 Sample : N4706-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8K8

Quant Time: Sep 23 23:36:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	449032	20.000	ng/u1	0.00
20) Naphthalene-d8	10.828	136	2019275	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.639	164	1268417	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2447695	20.000	ng/u1	0.00
79) Chrysene-d12	21.545	240	1708952	20.000	ng/u1	0.00
88) Perylene-d12	23.986	264	1452236	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	46624	3.892	ng/uL	0.00
4) Pyridine-d5	3.822	84	201518	5.769	ng/u1	0.00
7) Phenol-d5	7.175	99	342296	8.530	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	634553	26.039	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	716402	24.798	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	562208	18.961	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	428284	31.336	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	411702	33.630	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	781363	27.541	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	502155	10.645	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	2633489	30.784	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	3023950	29.800	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	115723	6.974	ng/u1	0.00
60) Fluorene-d10	15.627	176	2239259	29.209	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	279549	28.867	ng/u1	0.00
73) Anthracene-d10	17.474	188	3270867	29.226	ng/u1	0.00
81) Pyrene-d10	19.756	212	3331562	39.627	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.827	264	2219252	31.279	ng/u1	0.00
Target Compounds					Qvalue	
2) 1,4-Dioxane	3.428	88	42927	3.327	ng/uL	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036678.D
Acq On : 23 Sep 2022 15:42
Operator : CG/JU
Sample : N4706-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K8

Quant Time: Sep 23 23:36:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

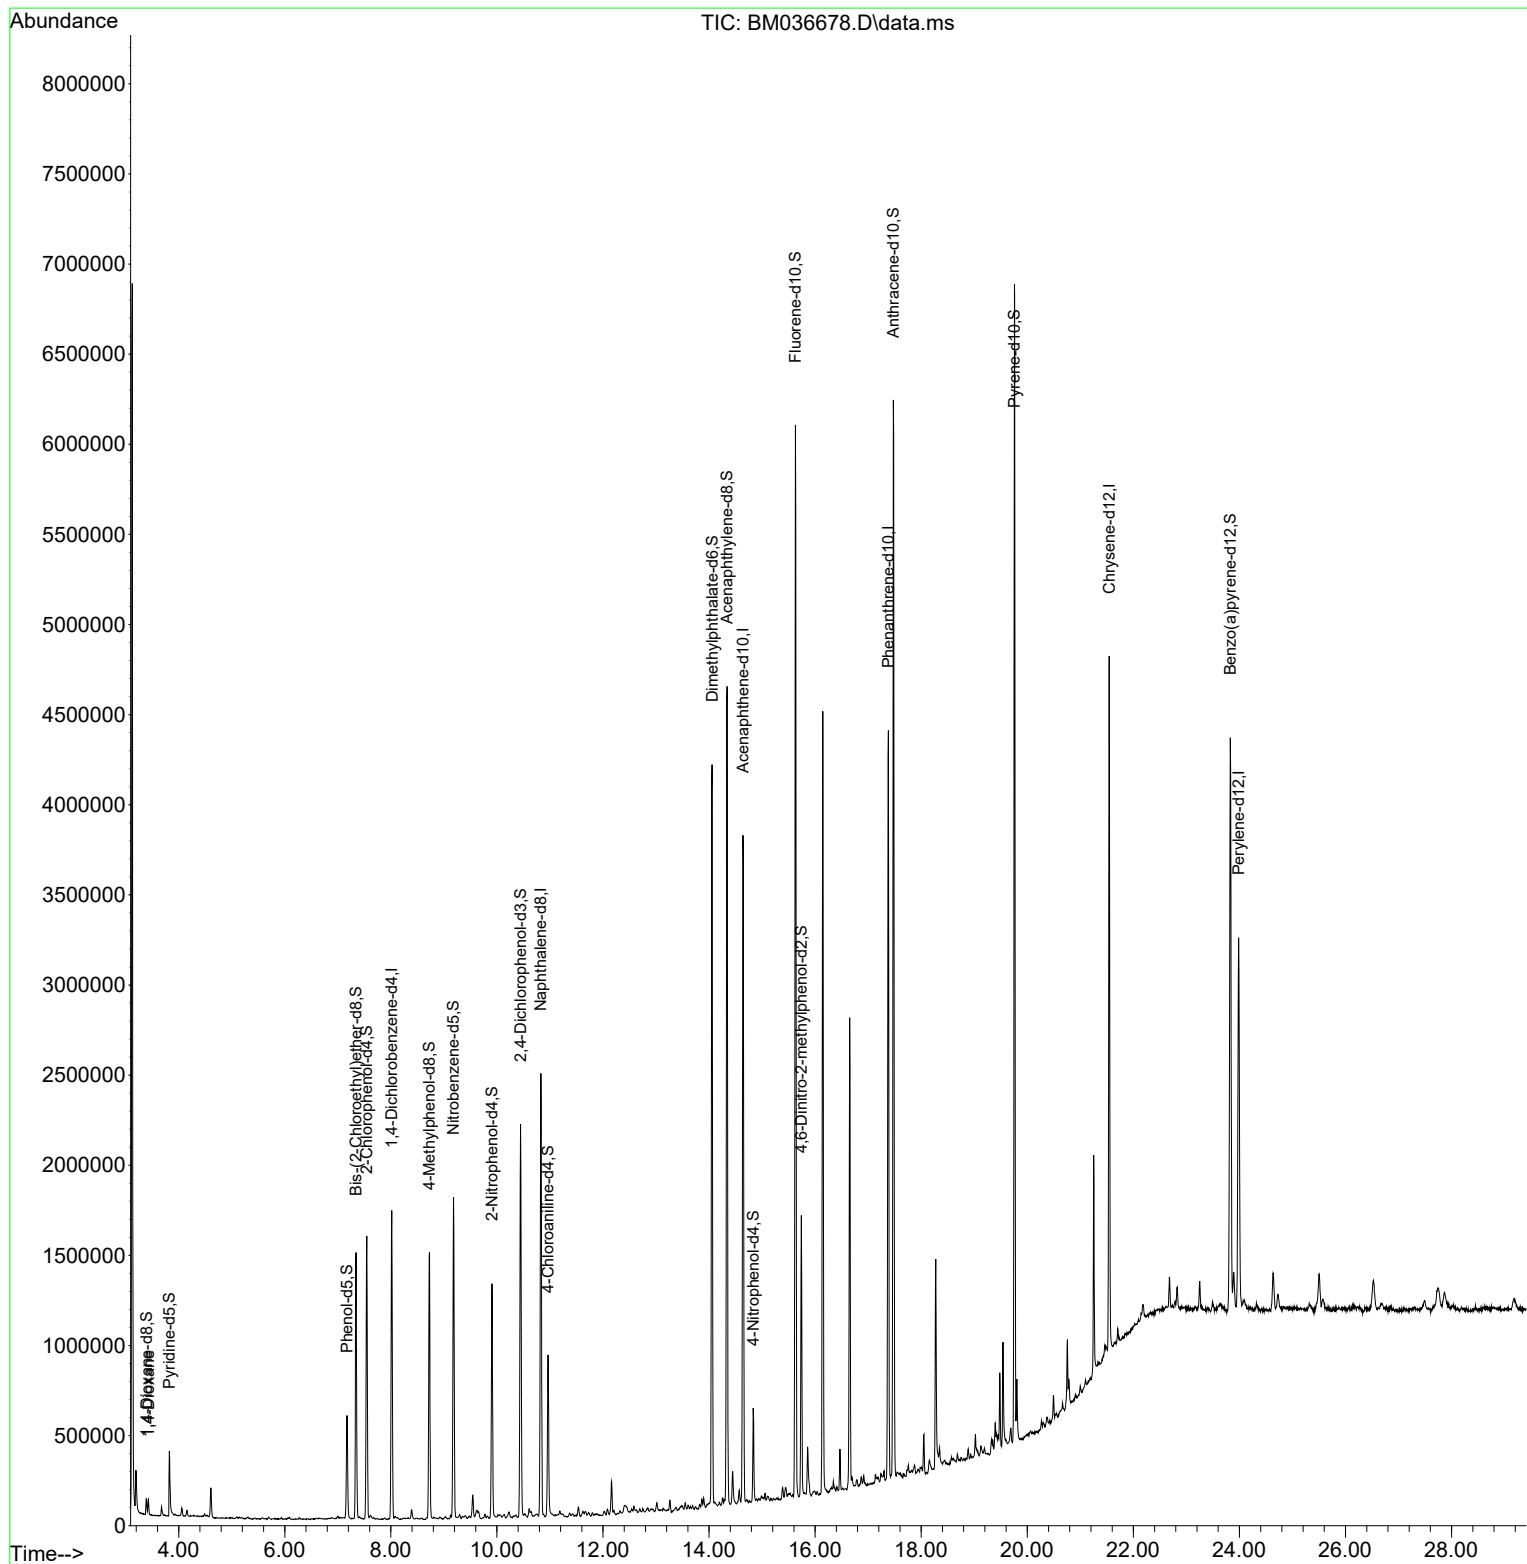

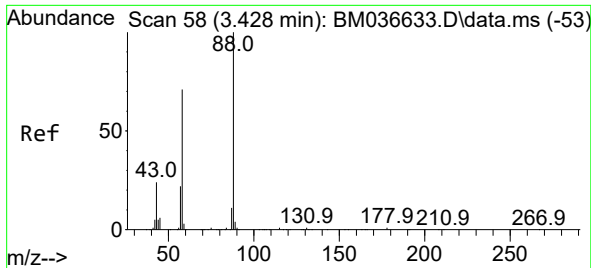

#2
 1,4-Dioxane
 Concen: 3.327 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM036678.D
 Acq: 23 Sep 2022 15:42

Instrument :
 BNA_M
 ClientSampleId :
 CB8K8

Tgt Ion: 88 Resp: 42927
 Ion Ratio Lower Upper
 88 100
 43 26.6 23.1 34.7
 58 63.6 56.6 85.0

