

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036684.D
 Acq On : 23 Sep 2022 19:23
 Operator : CG/JU
 Sample : N4706-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8M1

Quant Time: Sep 23 23:36:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	417877	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	1892065	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.639	164	1233487	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.374	188	2448065	20.000	ng/ul	0.00
79) Chrysene-d12	21.545	240	1875536	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	1614779	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	48676	4.367	ng/uL	0.00
4) Pyridine-d5	3.822	84	293097	9.016	ng/ul	0.00
7) Phenol-d5	7.175	99	236216	6.325	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	686146	30.255	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	685925	25.513	ng/ul	0.00
15) 4-Methylphenol-d8	8.722	113	445804	16.156	ng/ul	0.00
21) Nitrobenzene-d5	9.181	128	460577	35.964	ng/ul	0.00
24) 2-Nitrophenol-d4	9.904	143	449318	39.170	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	757093	28.479	ng/ul	0.00
31) 4-Chloroaniline-d4	10.963	131	1144521	25.895	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	2746670	33.016	ng/ul	0.00
49) Acenaphthylene-d8	14.333	160	3301973	33.462	ng/ul	0.00
54) 4-Nitrophenol-d4	14.833	143	74907	4.642	ng/ul	0.00
60) Fluorene-d10	15.627	176	2466021	33.078	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	249318	25.741	ng/ul	0.00
73) Anthracene-d10	17.474	188	3836407	34.274	ng/ul	0.00
81) Pyrene-d10	19.757	212	4047181	43.863	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	2866104	36.330	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	7.152	77	38967	2.155	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036684.D
Acq On : 23 Sep 2022 19:23
Operator : CG/JU
Sample : N4706-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8M1

Quant Time: Sep 23 23:36:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

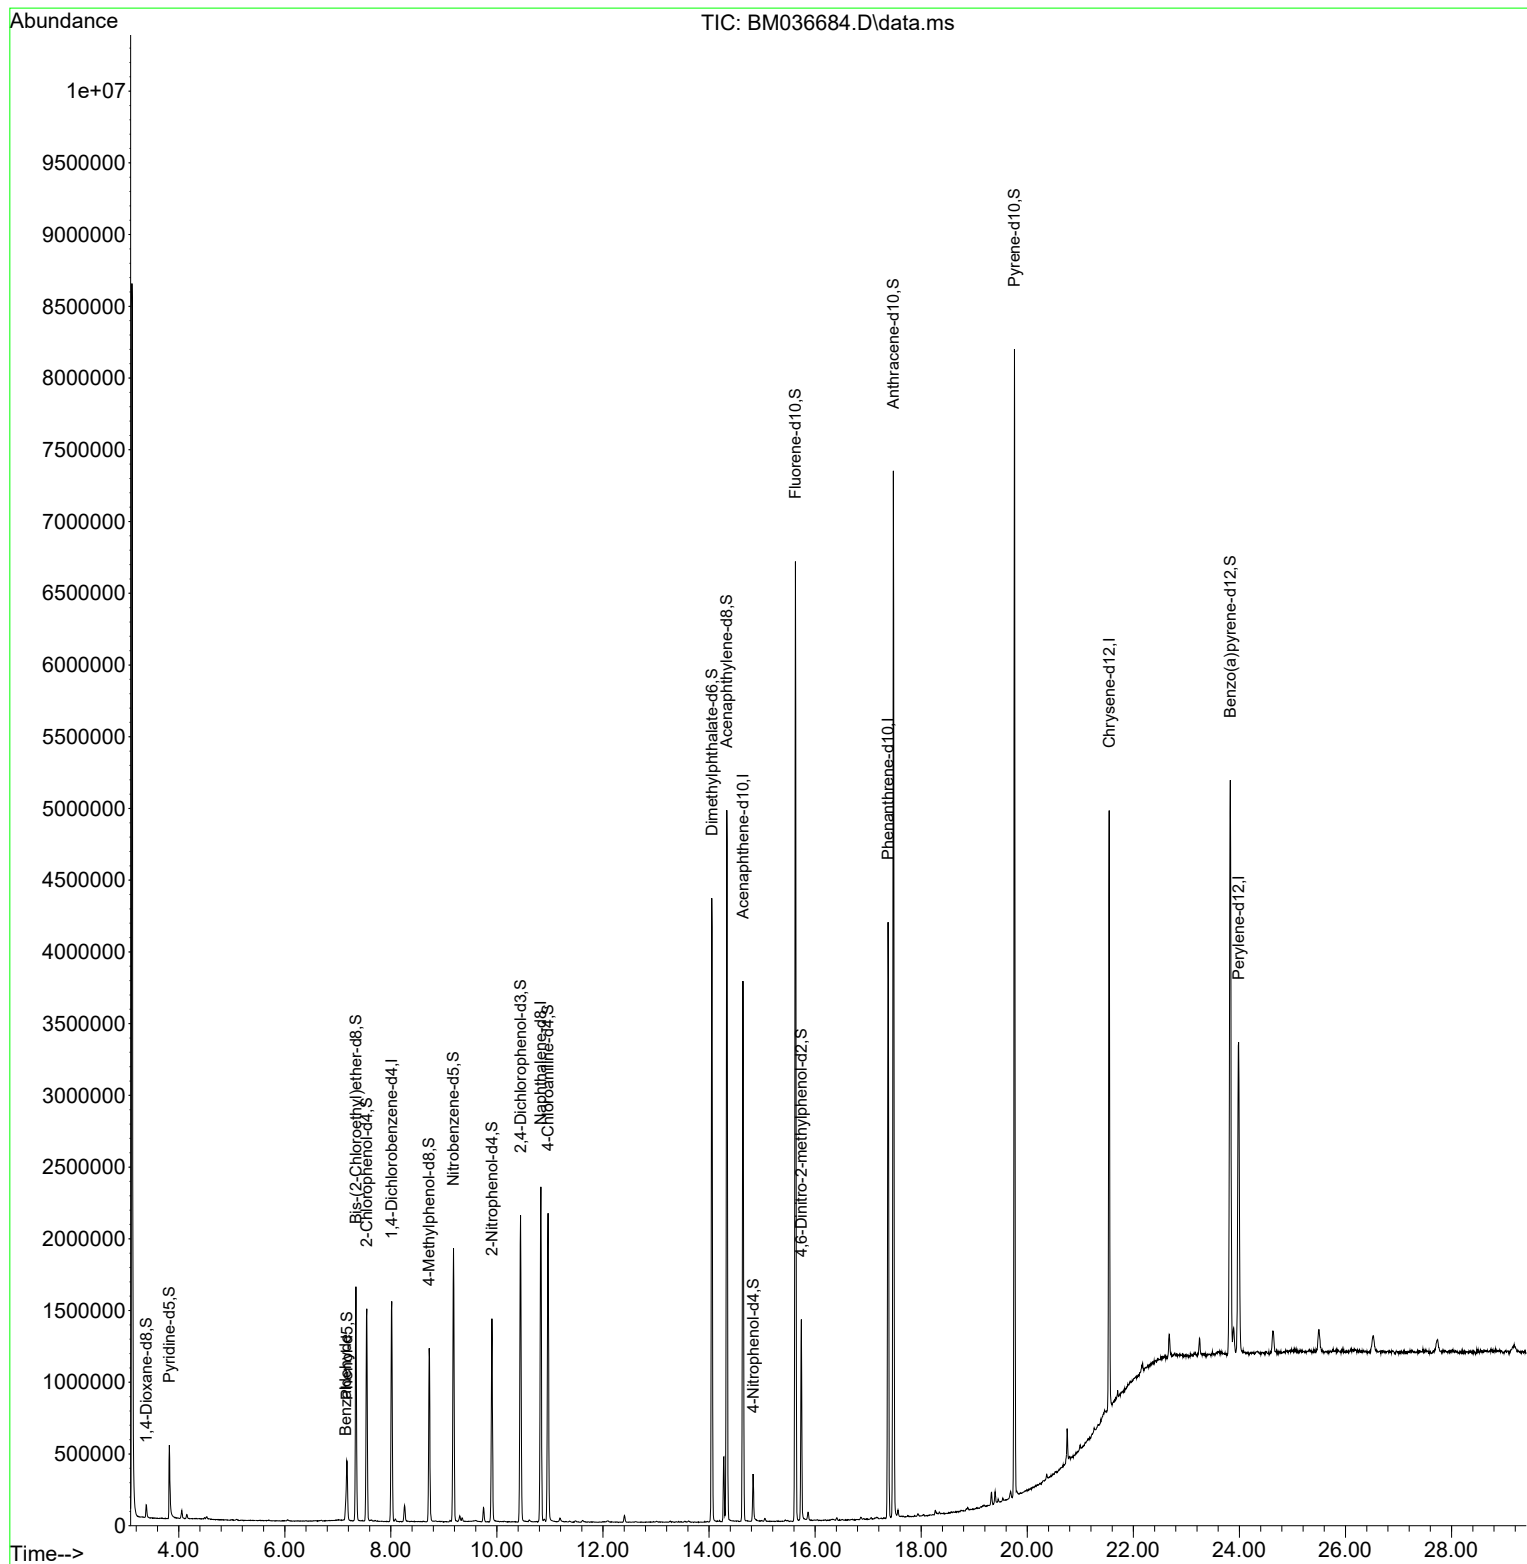

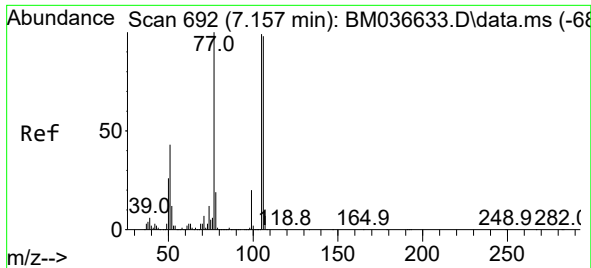

#6
Benzaldehyde
Concen: 2.155 ng/ul
RT: 7.152 min Scan# 691
Delta R.T. -0.006 min
Lab File: BM036684.D
Acq: 23 Sep 2022 19:23

Instrument :
BNA_M
ClientSampleId :
CB8M1

Tgt Ion:	77	Resp:	38967
Ion	Ratio	Lower	Upper
77	100		
105	94.6	75.1	112.7
106	92.0	73.0	109.6

