

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036716.D
 Acq On : 24 Sep 2022 15:46
 Operator : CG/JU
 Sample : N4662-10
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ45

Quant Time: Sep 26 01:12:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	378848	20.000	ng/u1	0.00
20) Naphthalene-d8	10.816	136	1645131	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.633	164	1006773	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.369	188	1925210	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1322444	20.000	ng/u1	-0.01
88) Perylene-d12	23.968	264	1146875	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	46199	4.571	ng/uL	0.00
4) Pyridine-d5	3.816	84	216167	7.334	ng/u1	0.00
7) Phenol-d5	7.163	99	222674	6.577	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	593528	28.868	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	595462	24.430	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	412426	16.486	ng/u1	-0.01
21) Nitrobenzene-d5	9.175	128	378414	33.984	ng/u1	0.00
24) 2-Nitrophenol-d4	9.898	143	349735	35.065	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	658625	28.494	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.951	131	490001	12.750	ng/u1	-0.01
46) Dimethylphthalate-d6	14.045	166	2267265	33.391	ng/u1	0.00
49) Acenaphthylene-d8	14.328	160	2622053	32.555	ng/u1	0.00
54) 4-Nitrophenol-d4	14.822	143	66417	5.043	ng/u1	-0.01
60) Fluorene-d10	15.622	176	2016575	33.140	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	215973	28.354	ng/u1	0.00
73) Anthracene-d10	17.469	188	3192546	36.268	ng/u1	0.00
81) Pyrene-d10	19.751	212	3351992	51.522	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.815	264	2228628	39.775	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.422	88	66015	6.064	ng/uL 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036716.D
Acq On : 24 Sep 2022 15:46
Operator : CG/JU
Sample : N4662-10
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ45

Quant Time: Sep 26 01:12:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 24 00:41:16 2022
Response via : Initial Calibration

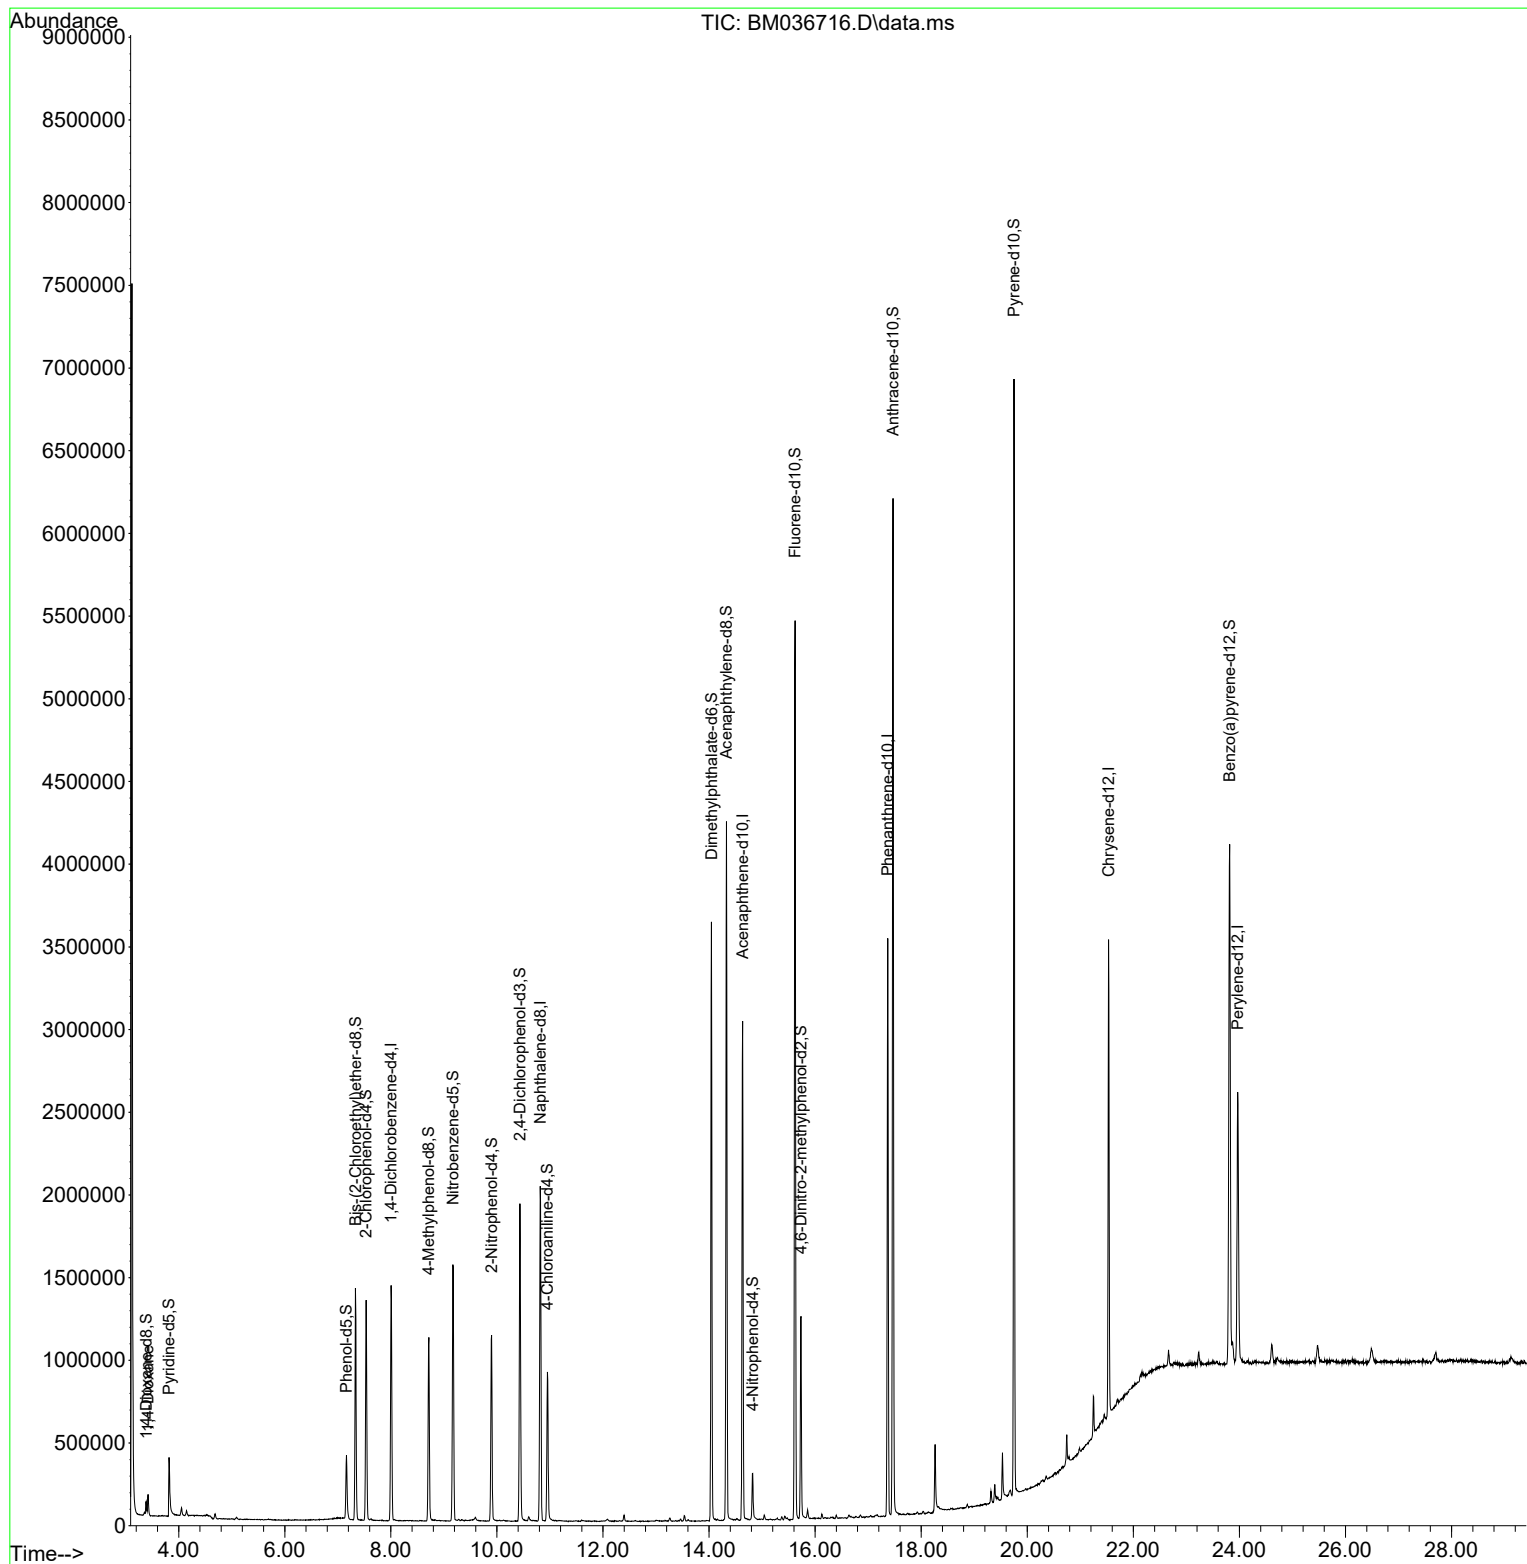

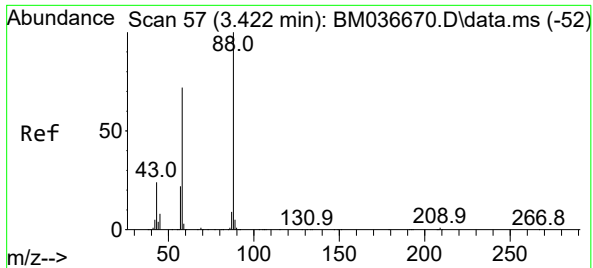

#2
 1,4-Dioxane
 Concen: 6.064 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BM036716.D
 Acq: 24 Sep 2022 15:46

Instrument :
 BNA_M
 ClientSampleId :
 EXZ45

Tgt Ion:	88	Resp:	66015
Ion	Ratio	Lower	Upper
88	100		
43	25.8	23.1	34.7
58	69.1	56.6	85.0

