

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036719.D
 Acq On : 24 Sep 2022 17:35
 Operator : CG/JU
 Sample : N4662-02
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ25

Quant Time: Sep 26 01:12:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	407433	20.000	ng/uL	0.00
20) Naphthalene-d8	10.816	136	1768044	20.000	ng/uL	-0.01
38) Acenaphthene-d10	14.633	164	1064540	20.000	ng/uL	0.00
64) Phenanthrene-d10	17.368	188	2025497	20.000	ng/uL	0.00
79) Chrysene-d12	21.539	240	1411671	20.000	ng/uL	0.00
88) Perylene-d12	23.968	264	1264834	20.000	ng/uL	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	50569	4.653	ng/uL	0.00
4) Pyridine-d5	3.822	84	109832	3.465	ng/uL	0.00
7) Phenol-d5	7.163	99	207798	5.707	ng/uL	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	570072	25.782	ng/uL	0.00
11) 2-Chlorophenol-d4	7.534	132	573840	21.891	ng/uL	0.00
15) 4-Methylphenol-d8	8.716	113	396530	14.739	ng/uL	-0.01
21) Nitrobenzene-d5	9.175	128	371103	31.010	ng/uL	0.00
24) 2-Nitrophenol-d4	9.898	143	344148	32.106	ng/uL	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	656212	26.416	ng/uL	-0.01
31) 4-Chloroaniline-d4	10.951	131	488222	11.821	ng/uL	-0.01
46) Dimethylphthalate-d6	14.045	166	2361817	32.896	ng/uL	0.00
49) Acenaphthylene-d8	14.327	160	2609135	30.637	ng/uL	0.00
54) 4-Nitrophenol-d4	14.821	143	66685	4.789	ng/uL	-0.01
60) Fluorene-d10	15.621	176	2061000	32.032	ng/uL	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	248535	31.014	ng/uL	0.00
73) Anthracene-d10	17.468	188	3440841	37.154	ng/uL	0.00
81) Pyrene-d10	19.751	212	3550547	51.125	ng/uL	0.00
92) Benzo(a)pyrene-d12	23.815	264	2447385	39.605	ng/uL	0.00
Target Compounds						
2) 1,4-Dioxane	3.422	88	60415	5.160	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036719.D
 Acq On : 24 Sep 2022 17:35
 Operator : CG/JU
 Sample : N4662-02
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ25

Quant Time: Sep 26 01:12:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration

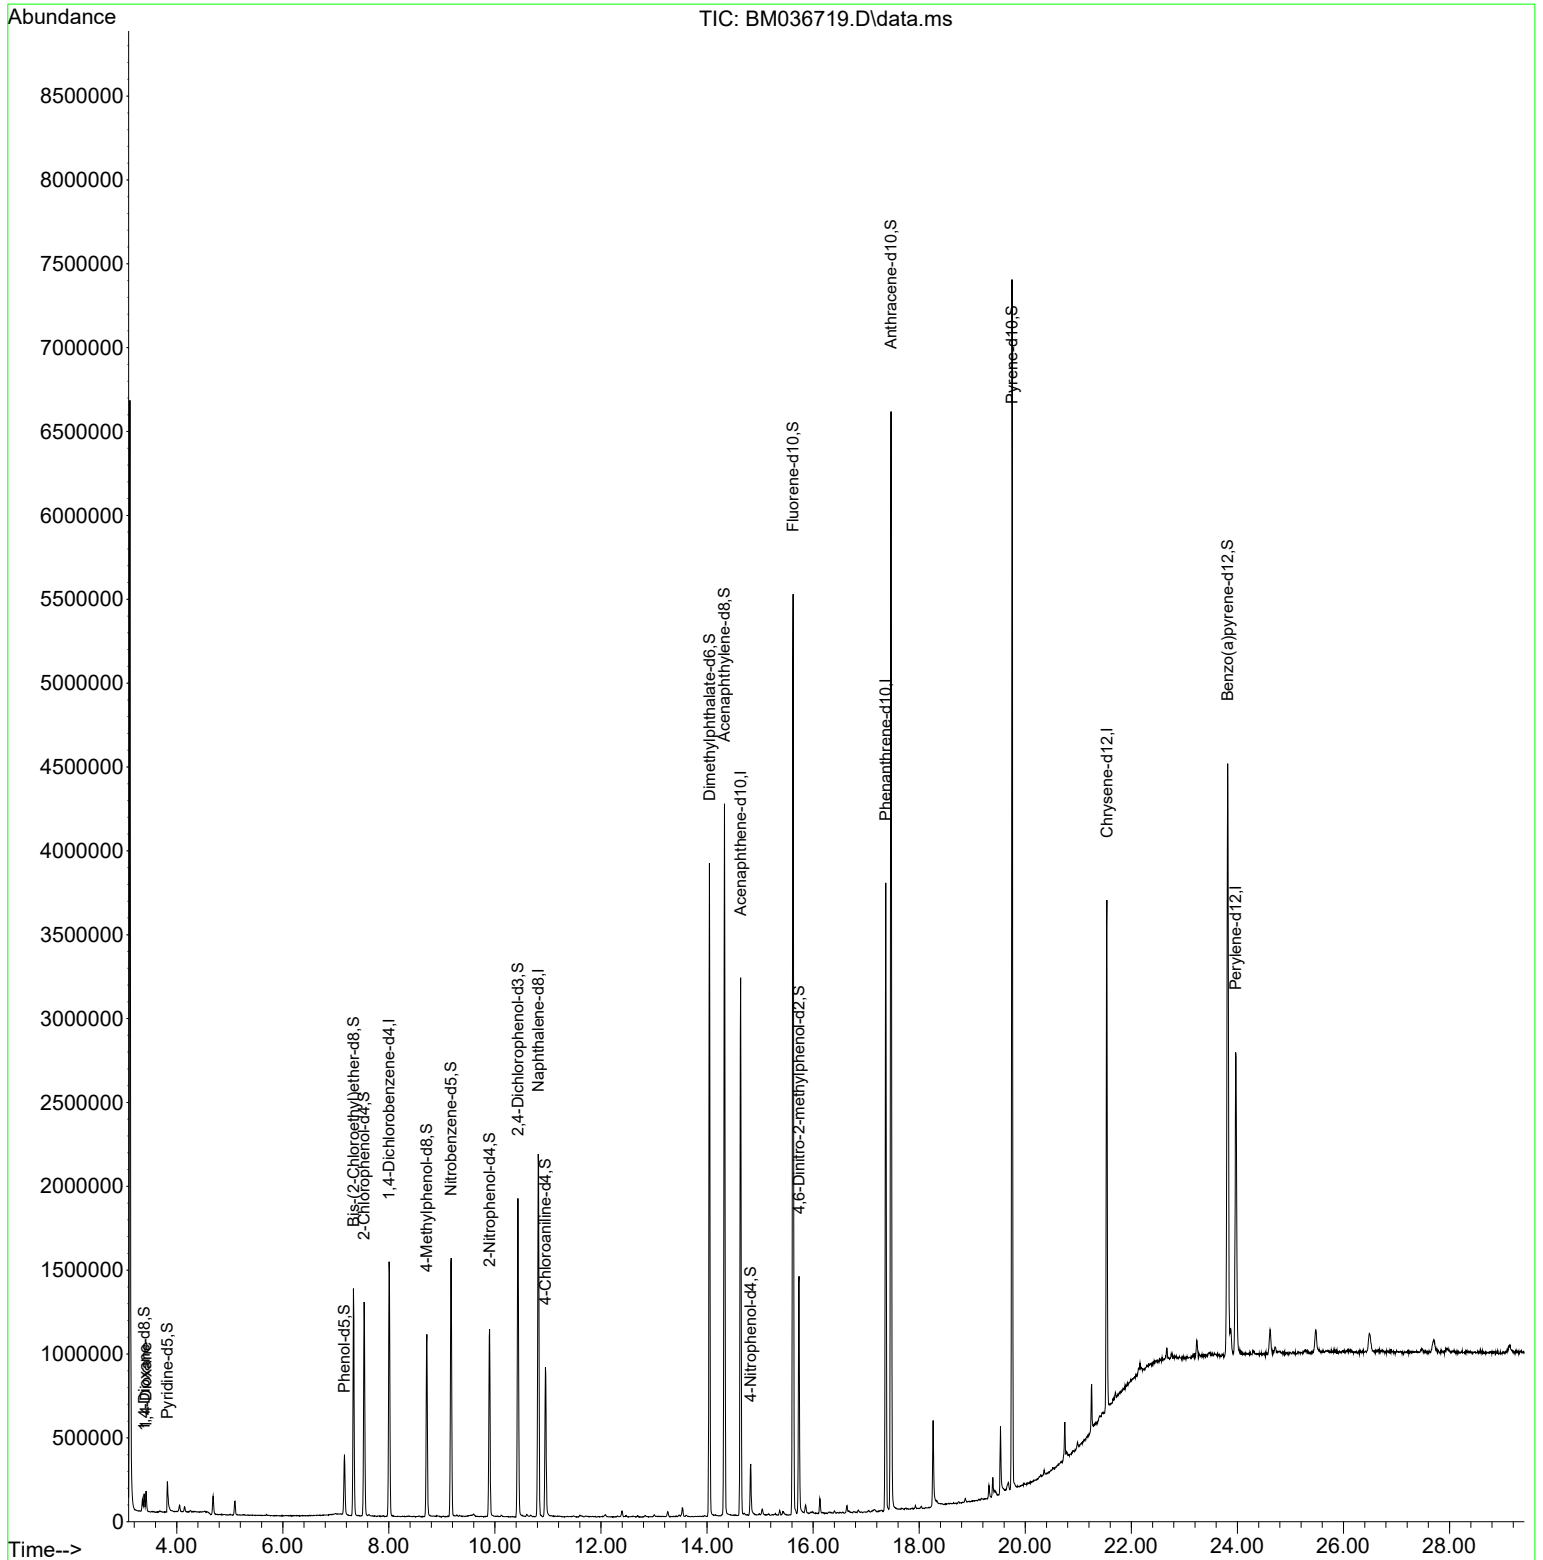

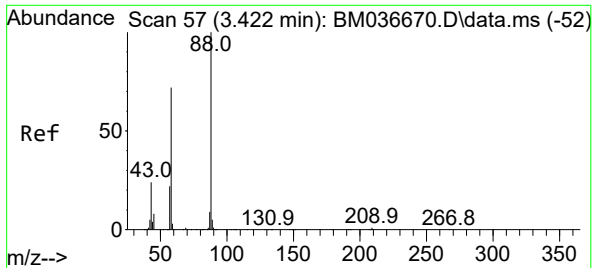

#2
 1,4-Dioxane
 Concen: 5.160 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BM036719.D
 Acq: 24 Sep 2022 17:35

Instrument :
 BNA_M
 ClientSampleId :
 EXZ25

Tgt Ion: 88 Resp: 60415

Ion	Ratio	Lower	Upper
88	100		
43	26.9	23.1	34.7
58	69.6	56.6	85.0

