

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036680.D
 Acq On : 23 Sep 2022 16:56
 Operator : CG/JU
 Sample : N4706-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8L2

Quant Time: Sep 23 23:36:18 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Sep 21 22:42:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	452107	20.000	ng/u1	0.00
20) Naphthalene-d8	10.827	136	2041375	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.639	164	1281375	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.380	188	2496872	20.000	ng/u1	0.00
79) Chrysene-d12	21.544	240	1785936	20.000	ng/u1	0.00
88) Perylene-d12	23.985	264	1478631	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	53976	4.476	ng/uL	0.00
4) Pyridine-d5	3.822	84	359249	10.214	ng/u1	0.00
7) Phenol-d5	7.175	99	353379	8.746	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.345	67	803303	32.740	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	884610	30.412	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	623606	20.889	ng/u1	0.00
21) Nitrobenzene-d5	9.180	128	530395	38.387	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	541817	43.779	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.445	165	961510	33.523	ng/u1	0.00
31) 4-Chloroaniline-d4	10.963	131	1010397	21.188	ng/u1	0.00
46) Dimethylphthalate-d6	14.057	166	3099202	35.861	ng/u1	0.00
49) Acenaphthylene-d8	14.339	160	3707144	36.163	ng/u1	0.00
54) 4-Nitrophenol-d4	14.833	143	114175	6.811	ng/u1	0.00
60) Fluorene-d10	15.627	176	2690471	34.739	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	329309	33.335	ng/u1	0.00
73) Anthracene-d10	17.474	188	3946291	34.567	ng/u1	0.00
81) Pyrene-d10	19.762	212	4075109	46.381	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.832	264	2681319	37.117	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.428	88	113710	8.753	ng/uL	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036680.D
Acq On : 23 Sep 2022 16:56
Operator : CG/JU
Sample : N4706-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8L2

Quant Time: Sep 23 23:36:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Sep 21 22:42:41 2022
Response via : Initial Calibration

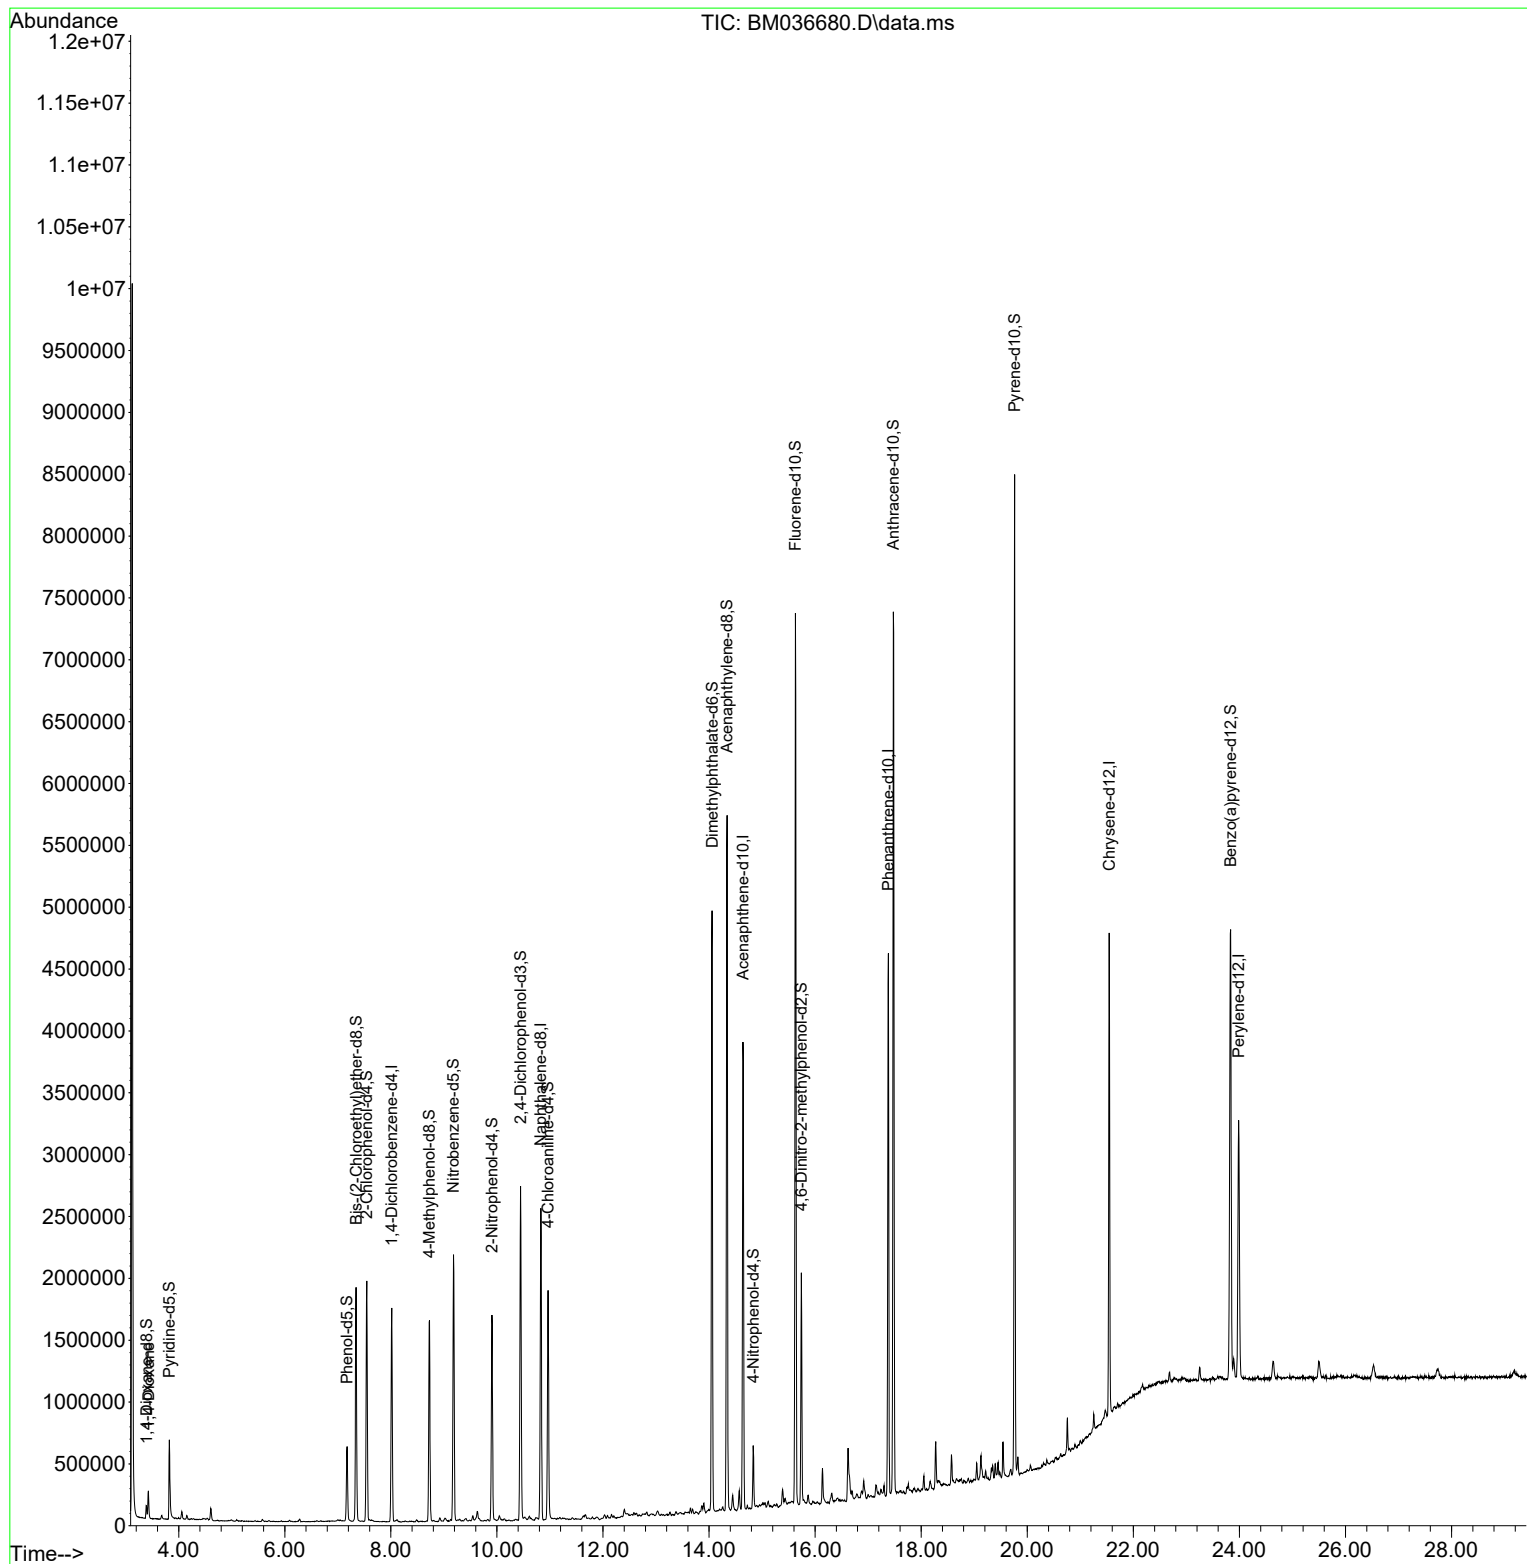

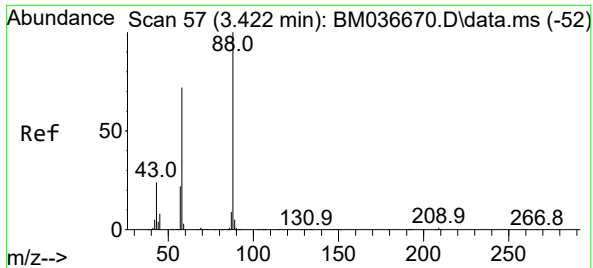

#2
 1,4-Dioxane
 Concen: 8.753 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM036680.D
 Acq: 23 Sep 2022 16:56

Instrument :
 BNA_M
 ClientSampleId :
 CB8L2

Tgt Ion:	88	Resp:	113710
Ion	Ratio	Lower	Upper
88	100		
43	23.9	23.1	34.7
58	67.9	56.6	85.0

