

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036695.D
 Acq On : 24 Sep 2022 02:34
 Operator : CG/JU
 Sample : N4649-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ40

Quant Time: Sep 24 03:04:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	431442	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1903519	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.633	164	1126264	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.374	188	2008178	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1557741	20.000	ng/u1	0.00
88) Perylene-d12	23.974	264	1485762	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	46903	4.075	ng/uL	0.00
4) Pyridine-d5	3.822	84	233313	6.951	ng/u1	0.00
7) Phenol-d5	7.169	99	248936	6.457	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	688794	29.417	ng/u1	0.00
11) 2-Chlorophenol-d4	7.540	132	705548	25.418	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	458500	16.094	ng/u1	-0.01
21) Nitrobenzene-d5	9.175	128	437846	33.984	ng/u1	0.00
24) 2-Nitrophenol-d4	9.898	143	415054	35.965	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.439	165	762389	28.506	ng/u1	0.00
31) 4-Chloroaniline-d4	10.957	131	879761	19.785	ng/u1	0.00
46) Dimethylphthalate-d6	14.051	166	2501957	32.938	ng/u1	0.00
49) Acenaphthylene-d8	14.333	160	2823892	31.341	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	60495	4.106	ng/u1	0.00
60) Fluorene-d10	15.621	176	2164897	31.803	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	100950	12.706	ng/u1	0.00
73) Anthracene-d10	17.468	188	3262073	35.527	ng/u1	0.00
81) Pyrene-d10	19.756	212	3363052	43.884	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.815	264	2794593	38.499	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.428	88	13742	1.108	ng/uL#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036695.D
Acq On : 24 Sep 2022 02:34
Operator : CG/JU
Sample : N4649-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ40

Quant Time: Sep 24 03:04:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 24 00:41:16 2022
Response via : Initial Calibration

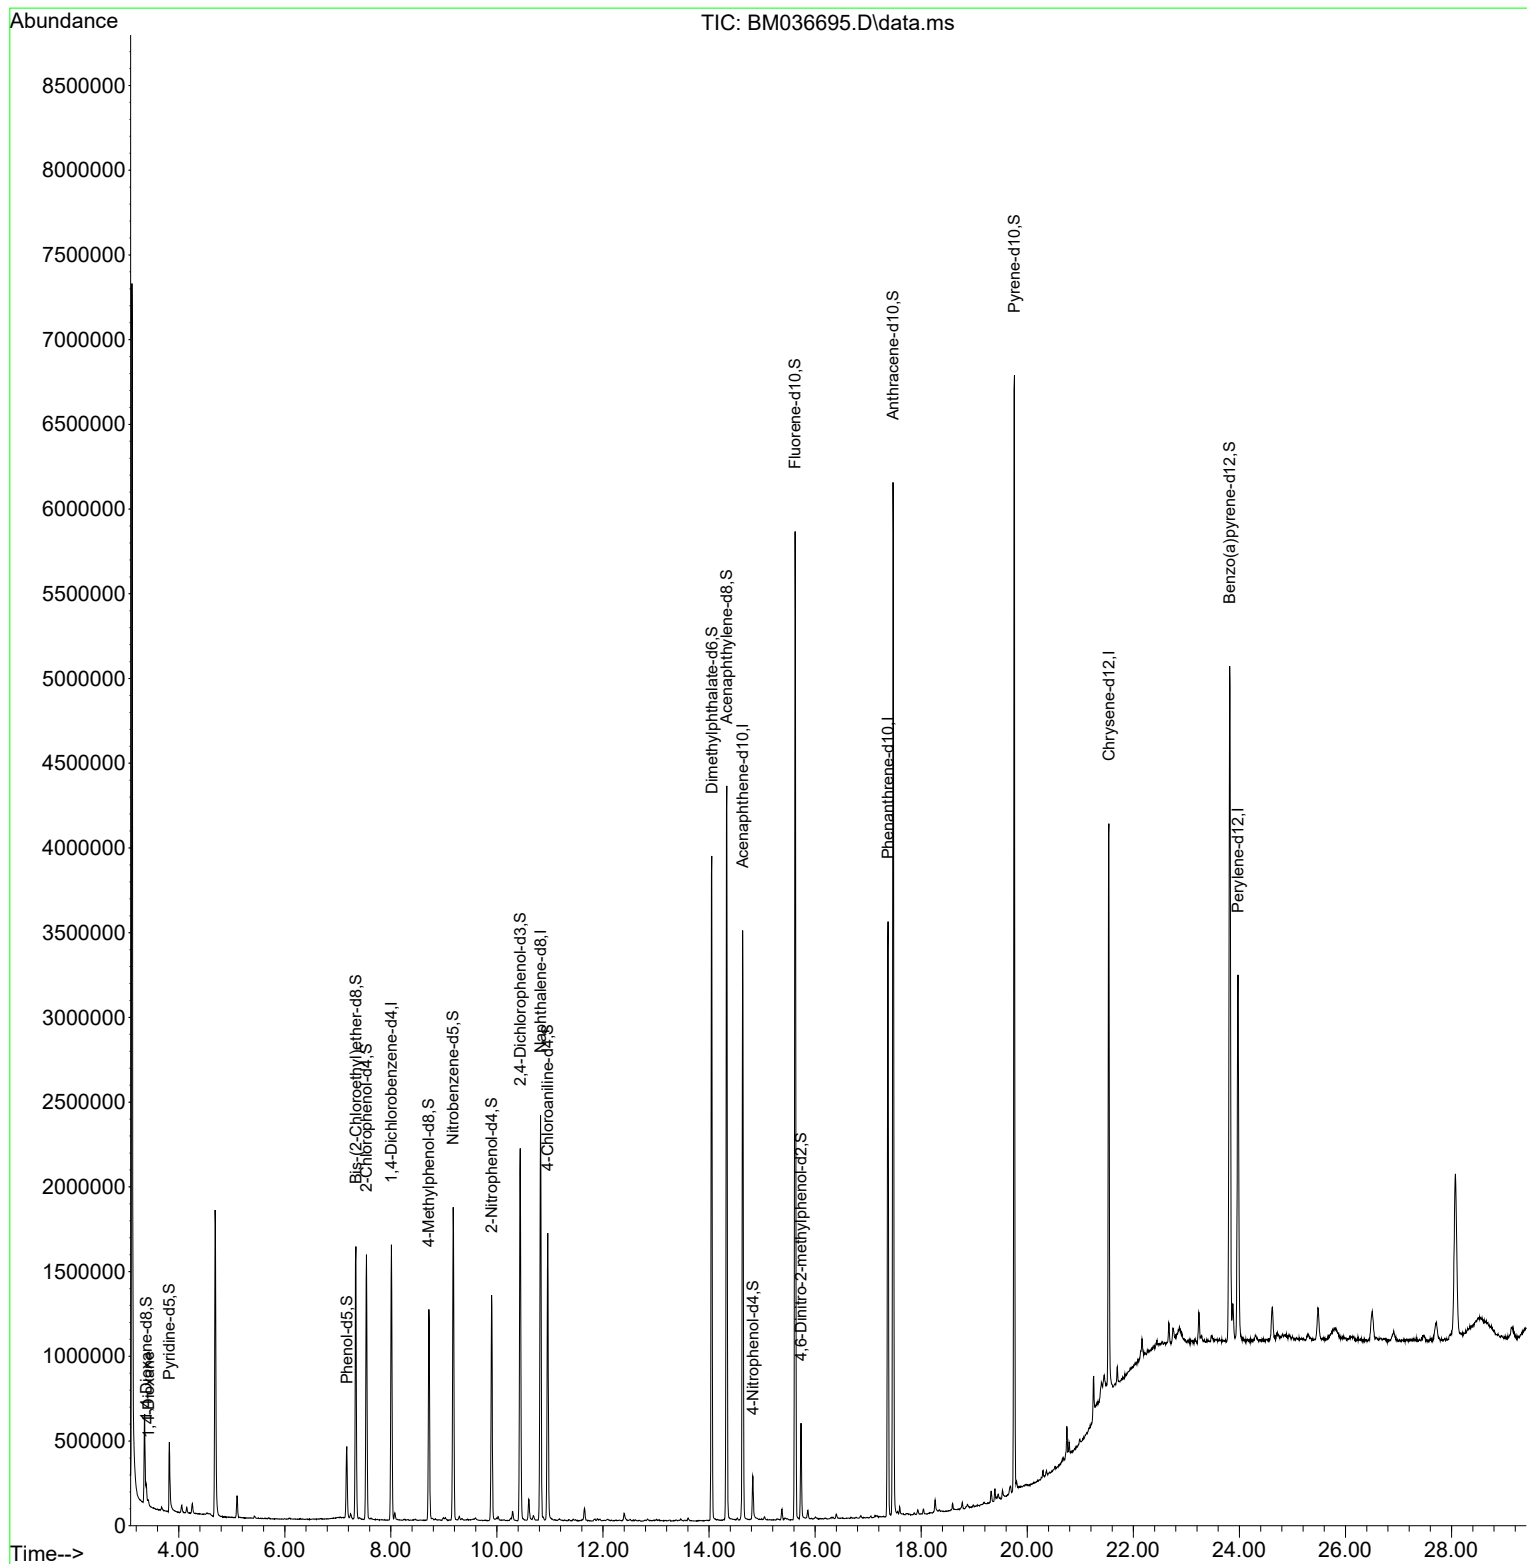

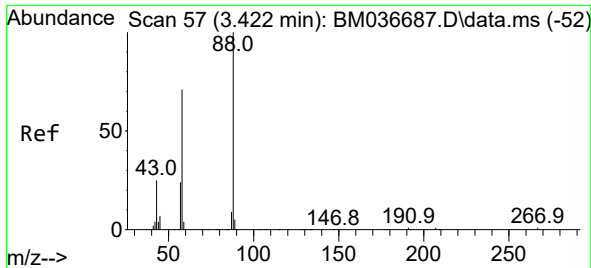

#2
 1,4-Dioxane
 Concen: 1.108 ng/uL
 RT: 3.428 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: BM036695.D
 Acq: 24 Sep 2022 02:34

Instrument :
 BNA_M
 ClientSampleId :
 EXZ40

Tgt Ion: 88 Resp: 13742
 Ion Ratio Lower Upper
 88 100
 43 27.0 23.1 34.7
 58 53.9 56.6 85.0#

