

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036704.D
 Acq On : 24 Sep 2022 07:53
 Operator : CG/JU
 Sample : N4649-22
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ43

Quant Time: Sep 26 01:08:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	400178	20.000	ng/u1	0.00
20) Naphthalene-d8	10.816	136	1876571	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.633	164	1203169	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.368	188	2341333	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1624709	20.000	ng/u1	-0.01
88) Perylene-d12	23.968	264	1448829	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	44690	4.186	ng/uL	0.00
4) Pyridine-d5	3.816	84	219651	7.055	ng/u1	0.00
7) Phenol-d5	7.163	99	201423	5.632	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	607892	27.990	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	597607	23.211	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	387618	14.669	ng/u1	-0.01
21) Nitrobenzene-d5	9.175	128	400891	31.562	ng/u1	0.00
24) 2-Nitrophenol-d4	9.898	143	377847	33.211	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.433	165	671846	25.481	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.957	131	968253	22.087	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	2528910	31.165	ng/u1	0.00
49) Acenaphthylene-d8	14.327	160	2928840	30.428	ng/u1	0.00
54) 4-Nitrophenol-d4	14.821	143	63490	4.034	ng/u1	-0.01
60) Fluorene-d10	15.621	176	2297817	31.598	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	229098	24.732	ng/u1	0.00
73) Anthracene-d10	17.468	188	3543011	33.096	ng/u1	0.00
81) Pyrene-d10	19.750	212	3653495	45.709	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.809	264	2511552	35.482	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.422	88	124498	10.827	ng/uL	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036704.D
Acq On : 24 Sep 2022 07:53
Operator : CG/JU
Sample : N4649-22
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ43

Quant Time: Sep 26 01:08:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 24 00:41:16 2022
Response via : Initial Calibration

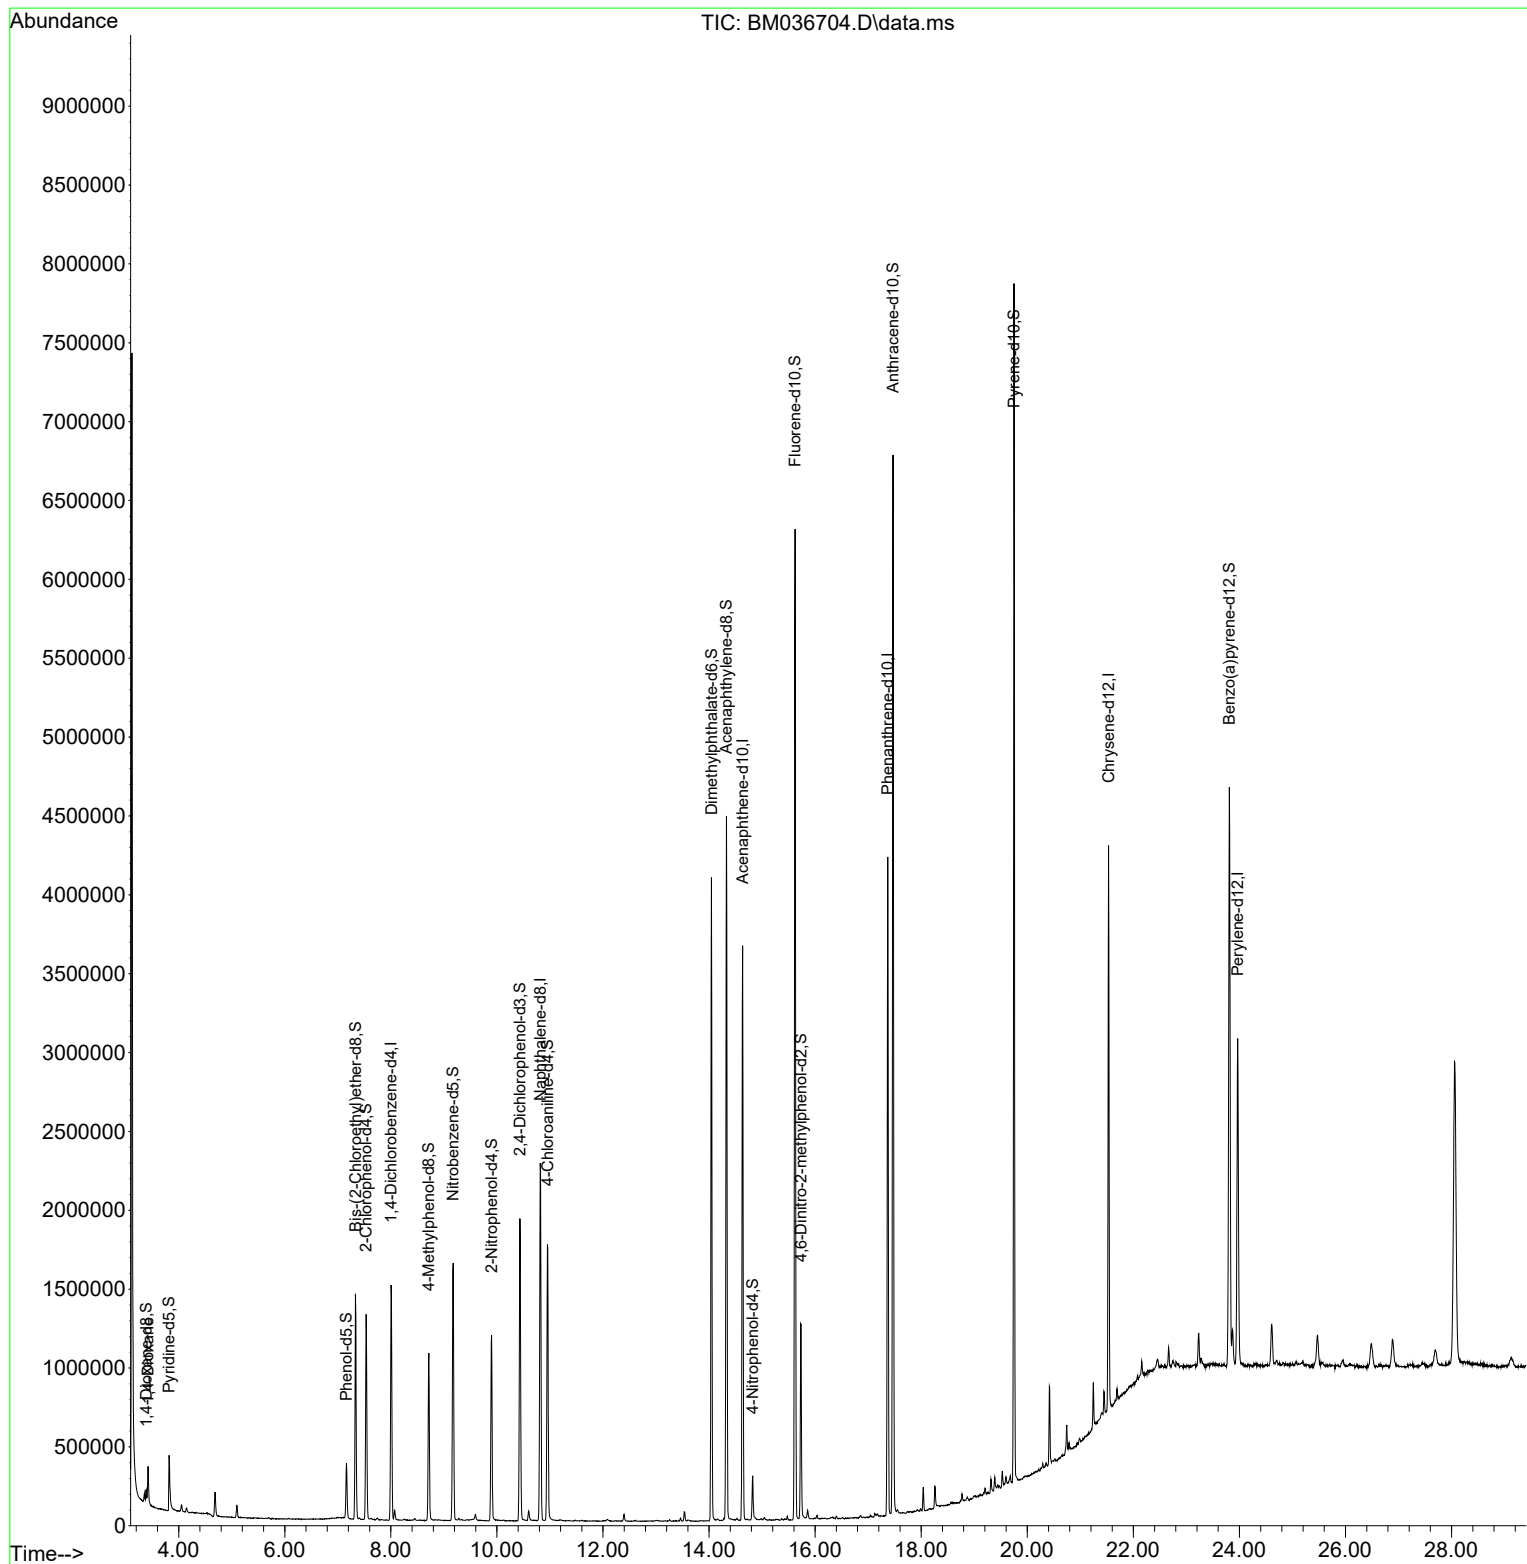

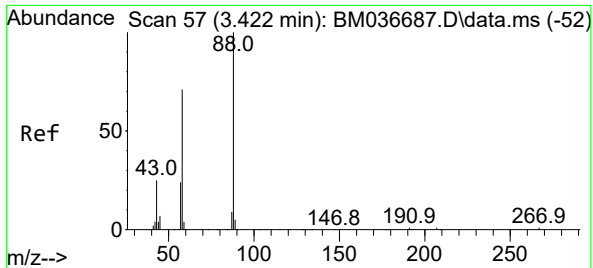

#2
 1,4-Dioxane
 Concen: 10.827 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BM036704.D
 Acq: 24 Sep 2022 07:53

Instrument :
 BNA_M
 ClientSampleId :
 EXZ43

Tgt Ion:	88	Resp:	124498
Ion	Ratio	Lower	Upper
88	100		
43	24.6	23.1	34.7
58	67.1	56.6	85.0

