

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036717.D
 Acq On : 24 Sep 2022 16:22
 Operator : CG/JU
 Sample : N4662-11
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ46

Quant Time: Sep 26 01:12:16 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	400644	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	1739671	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.633	164	1076825	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.368	188	2028840	20.000	ng/u1	0.00
79) Chrysene-d12	21.539	240	1389852	20.000	ng/u1	0.00
88) Perylene-d12	23.968	264	1203975	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	46709	4.370	ng/uL	0.00
4) Pyridine-d5	3.822	84	123582	3.965	ng/u1	0.00
7) Phenol-d5	7.163	99	243222	6.793	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	617855	28.416	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	638016	24.752	ng/u1	0.00
15) 4-Methylphenol-d8	8.716	113	456878	17.270	ng/u1	-0.01
21) Nitrobenzene-d5	9.175	128	411836	34.975	ng/u1	0.00
24) 2-Nitrophenol-d4	9.898	143	393014	37.263	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.433	165	724022	29.621	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.957	131	281808	6.934	ng/u1	0.00
46) Dimethylphthalate-d6	14.045	166	2697406	37.141	ng/u1	0.00
49) Acenaphthylene-d8	14.327	160	2919823	33.894	ng/u1	0.00
54) 4-Nitrophenol-d4	14.821	143	90332	6.413	ng/u1	-0.01
60) Fluorene-d10	15.621	176	2323181	35.695	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.733	200	288839	35.984	ng/u1	0.00
73) Anthracene-d10	17.468	188	3611692	38.934	ng/u1	0.00
81) Pyrene-d10	19.750	212	3639915	53.234	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.815	264	2423542	41.202	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.422	88	154631	13.431	ng/uL	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036717.D
Acq On : 24 Sep 2022 16:22
Operator : CG/JU
Sample : N4662-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ46

Quant Time: Sep 26 01:12:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 24 00:41:16 2022
Response via : Initial Calibration

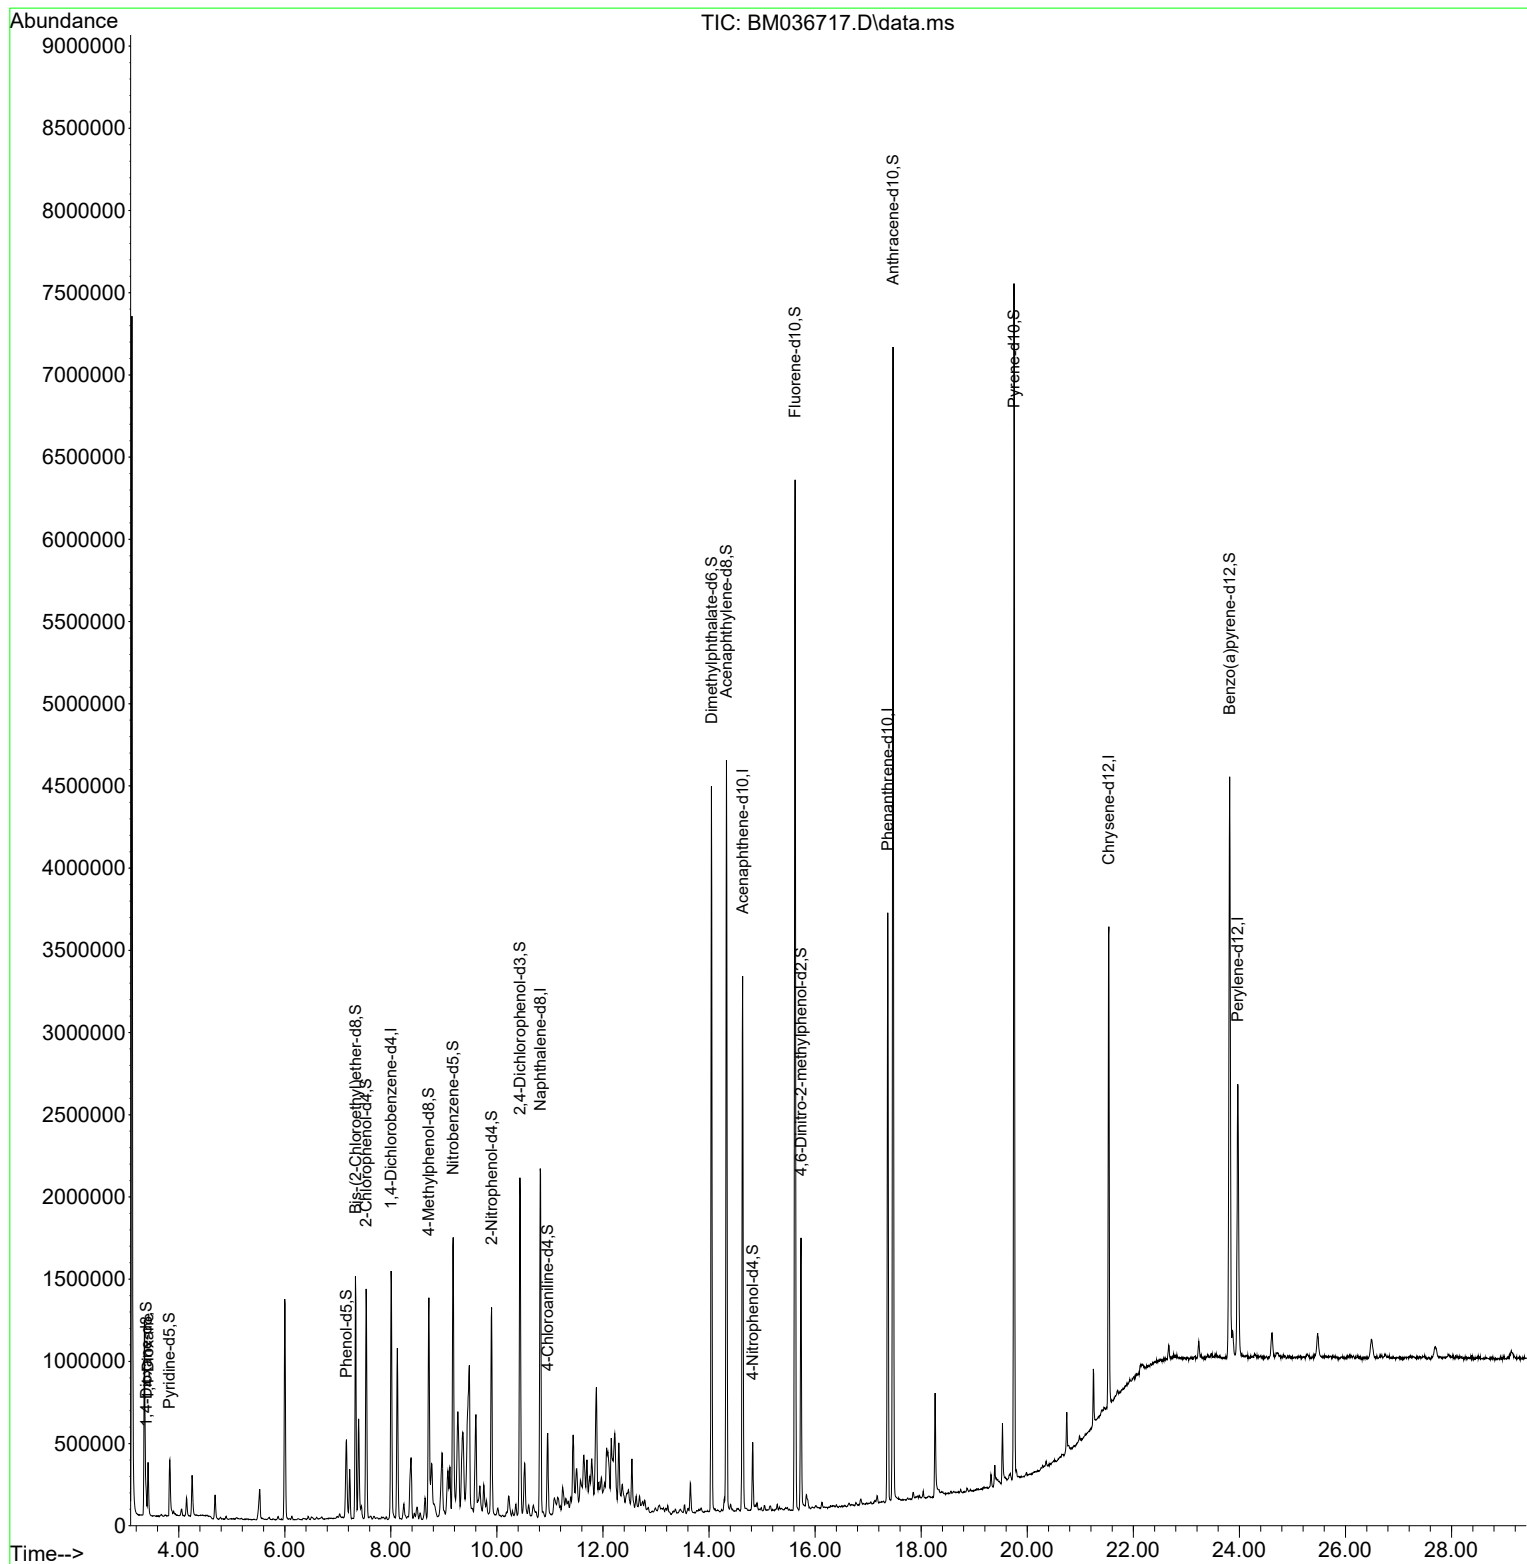

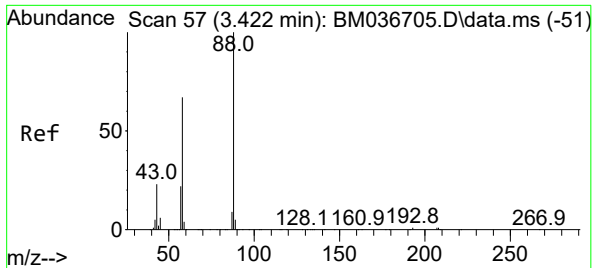

#2
 1,4-Dioxane
 Concen: 13.431 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BM036717.D
 Acq: 24 Sep 2022 16:22

Instrument :
 BNA_M
 ClientSampleId :
 EXZ46

Tgt Ion:	88	Resp:	154631
Ion	Ratio	Lower	Upper
88	100		
43	26.9	23.1	34.7
58	66.9	56.6	85.0

