

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036728.D
 Acq On : 25 Sep 2022 00:12
 Operator : CG/JU
 Sample : N4662-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ27

Quant Time: Sep 26 01:15:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Sep 24 00:41:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.004	152	342760	20.000	ng/u1	0.00
20) Naphthalene-d8	10.816	136	1533438	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.627	164	959815	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.368	188	1902425	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1392461	20.000	ng/u1	-0.01
88) Perylene-d12	23.962	264	1200307	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	37346	4.085	ng/uL	0.00
4) Pyridine-d5	3.822	84	104366	3.914	ng/u1	0.00
7) Phenol-d5	7.163	99	192321	6.279	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	563758	30.307	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	546949	24.802	ng/u1	0.00
15) 4-Methylphenol-d8	8.710	113	379339	16.760	ng/u1	-0.02
21) Nitrobenzene-d5	9.169	128	366024	35.265	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.892	143	331632	35.672	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.433	165	615246	28.556	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.951	131	488131	13.627	ng/u1	-0.01
46) Dimethylphthalate-d6	14.045	166	2157072	33.322	ng/u1	0.00
49) Acenaphthylene-d8	14.321	160	2510353	32.693	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.815	143	52797	4.205	ng/u1	-0.02
60) Fluorene-d10	15.615	176	1994664	34.384	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.727	200	208601	27.714	ng/u1	-0.01
73) Anthracene-d10	17.462	188	3288029	37.800	ng/u1	-0.01
81) Pyrene-d10	19.745	212	3433046	50.115	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.809	264	2294628	39.130	ng/u1	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	16354	1.660	ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036728.D
Acq On : 25 Sep 2022 00:12
Operator : CG/JU
Sample : N4662-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ27

Quant Time: Sep 26 01:15:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Sep 24 00:41:16 2022
Response via : Initial Calibration

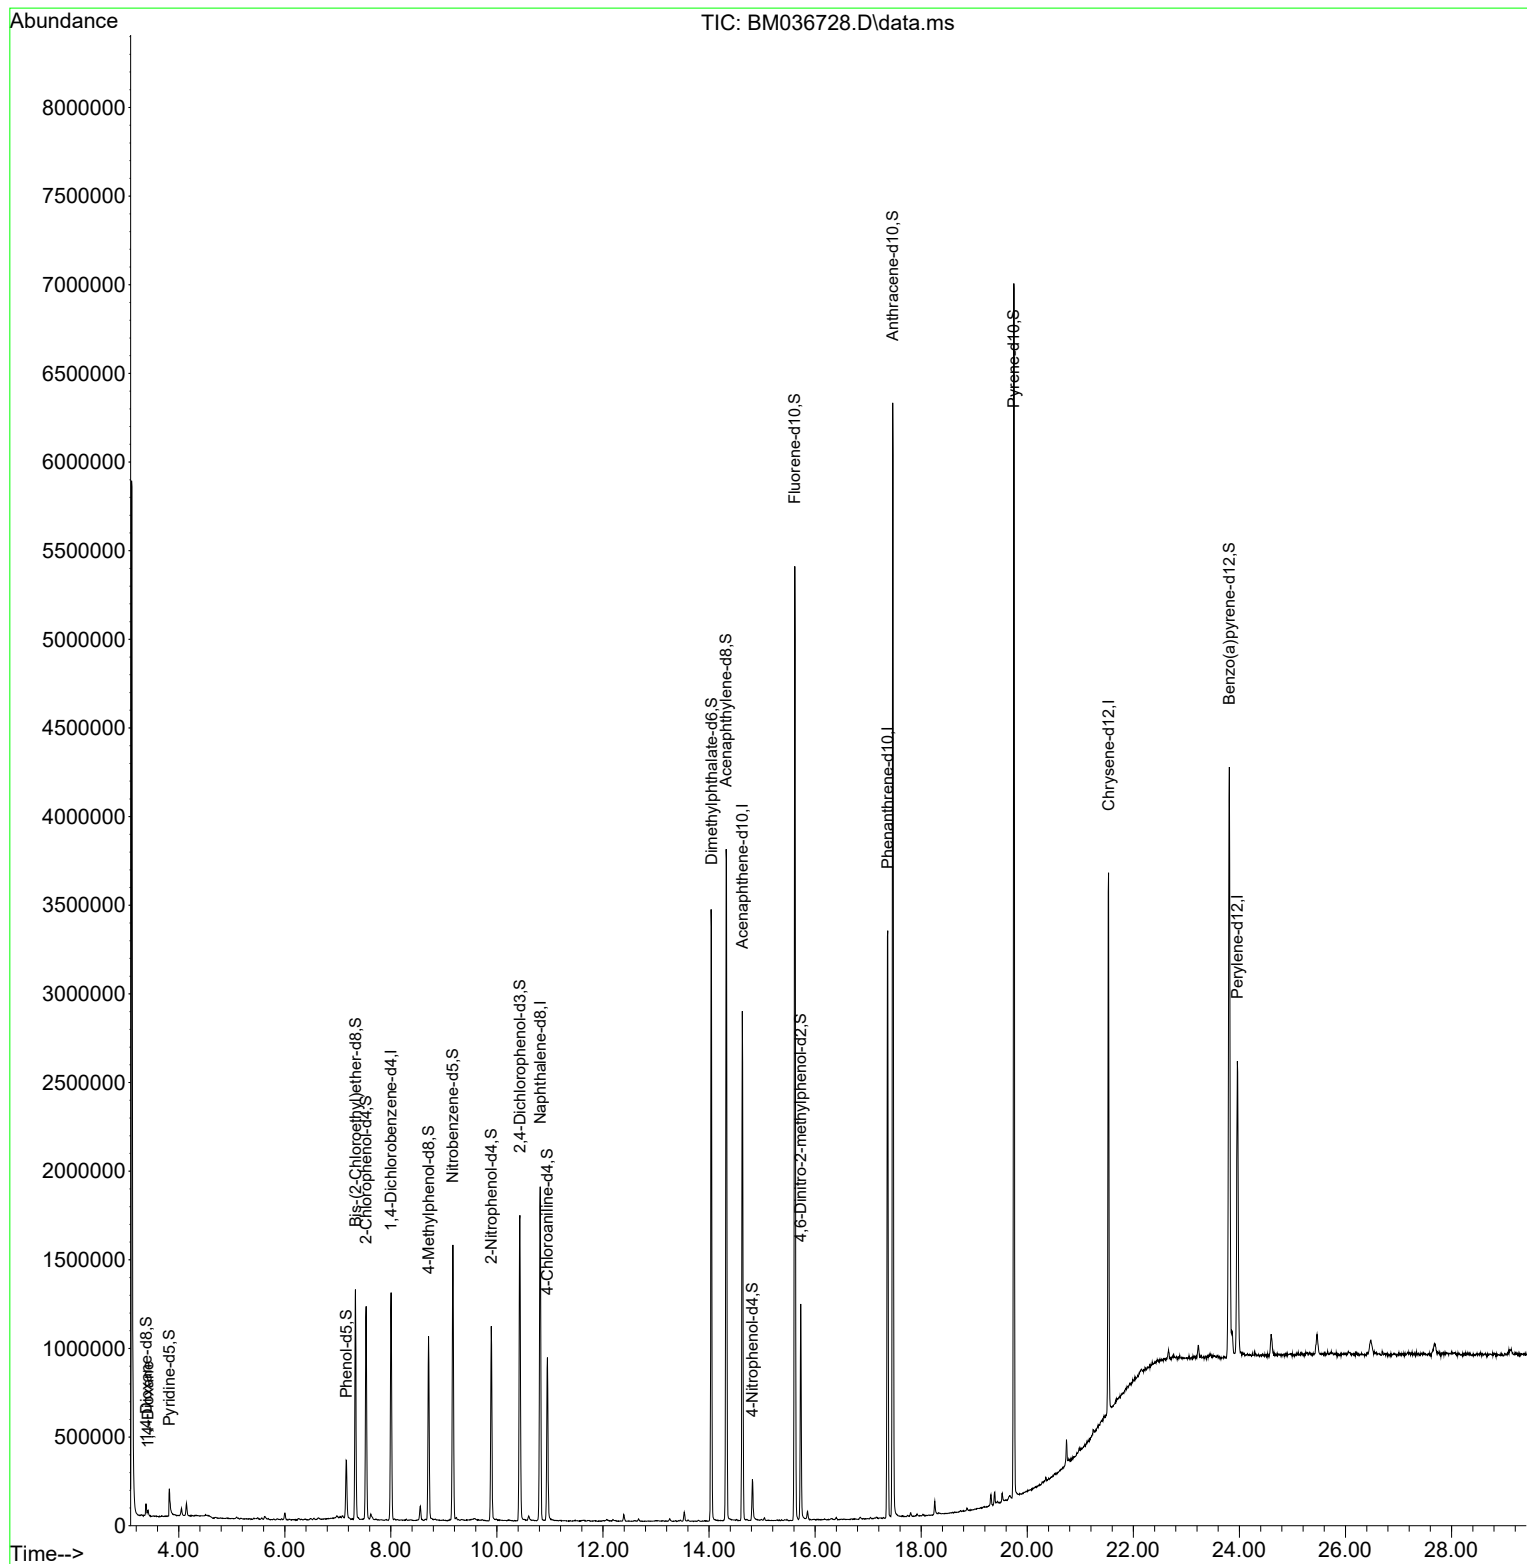

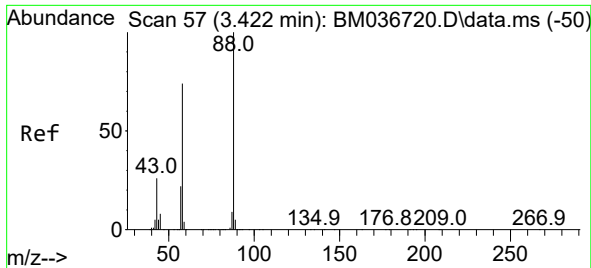

#2
 1,4-Dioxane
 Concen: 1.660 ng/uL
 RT: 3.422 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BM036728.D
 Acq: 25 Sep 2022 00:12

Instrument :
 BNA_M
 ClientSampleId :
 EXZ27

Tgt Ion:	88	Resp:	16354
Ion	Ratio	Lower	Upper
88	100		
43	26.4	23.1	34.7
58	65.9	56.6	85.0

