

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036685.D
 Acq On : 23 Sep 2022 20:00
 Operator : CG/JU
 Sample : N4708-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8K7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	26	rVB	6413406	8472508	82.03%	7.915%
2	3.393	47	52	60	rVB	88000	127910	1.24%	0.119%
3	3.681	98	101	109	rVB5	8443	16380	0.16%	0.015%
4	3.828	122	126	136	rBV	211354	341111	3.30%	0.319%
5	4.057	160	165	169	rVB	37384	54687	0.53%	0.051%
6	4.151	177	181	188	rVB	47829	72464	0.70%	0.068%
7	5.098	337	342	347	rVB5	12437	25295	0.24%	0.024%
8	5.698	438	444	451	rVB8	6429	16173	0.16%	0.015%
9	6.010	493	497	500	rBV6	12140	16252	0.16%	0.015%
10	6.987	658	663	664	rBV4	10814	13553	0.13%	0.013%
11	7.098	678	682	687	rVB	18637	25670	0.25%	0.024%
12	7.169	687	694	707	rVB2	363854	707460	6.85%	0.661%
13	7.340	716	723	737	rBV	1319236	2040595	19.76%	1.906%
14	7.540	748	757	765	rBV	1242123	1987754	19.25%	1.857%
15	7.634	769	773	774	rBV4	12088	12813	0.12%	0.012%
16	8.016	829	838	845	rBV	1683288	2642148	25.58%	2.468%
17	8.081	845	849	854	rVB2	16395	24945	0.24%	0.023%
18	8.722	951	958	968	rBV	1114446	1737822	16.83%	1.624%
19	9.181	1029	1036	1044	rBV	1492818	2447606	23.70%	2.287%
20	9.292	1051	1055	1059	rVB2	13848	19146	0.19%	0.018%
21	9.345	1061	1064	1070	rVB4	20530	29473	0.29%	0.028%
22	9.604	1103	1108	1117	rVB2	47189	87778	0.85%	0.082%
23	9.904	1151	1159	1174	rBV	1169856	1863700	18.04%	1.741%
24	10.139	1194	1199	1204	rVB7	9501	16482	0.16%	0.015%
25	10.351	1228	1235	1237	rBV6	5129	10441	0.10%	0.010%
26	10.445	1242	1251	1260	rBV	1859059	3095346	29.97%	2.892%
27	10.604	1272	1278	1286	rBV	120840	196377	1.90%	0.183%
28	10.828	1306	1316	1324	rBV	2486467	4109842	39.79%	3.840%
29	10.963	1329	1339	1350	rVV	743422	1275902	12.35%	1.192%
30	11.116	1361	1365	1371	rVB6	18858	28619	0.28%	0.027%
31	11.486	1422	1428	1433	rBV6	7694	15443	0.15%	0.014%
32	11.616	1446	1450	1457	rVB9	12281	25417	0.25%	0.024%
33	11.845	1486	1489	1496	rVB9	6910	12430	0.12%	0.012%
34	11.986	1508	1513	1516	rBV6	5475	10541	0.10%	0.010%
35	12.092	1526	1531	1538	rVB3	16013	30256	0.29%	0.028%
36	12.245	1551	1557	1561	rVB5	13410	27094	0.26%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036685.D
 Acq On : 23 Sep 2022 20:00
 Operator : CG/JU
 Sample : N4708-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8K7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	12.404	1576	1584	1590	rBV2	36615	65530	0.63%	0.061%
38	13.016	1683	1688	1692	rBV7	10984	20315	0.20%	0.019%
39	13.186	1714	1717	1721	rVV6	6741	10564	0.10%	0.010%
40	13.263	1725	1730	1735	rVB6	11652	20261	0.20%	0.019%
41	13.469	1760	1765	1774	rBV2	45166	68996	0.67%	0.064%
42	13.545	1774	1778	1783	rVV3	25140	41372	0.40%	0.039%
43	13.616	1783	1790	1796	rVB3	10919	23604	0.23%	0.022%
44	14.051	1857	1864	1874	rBV	4105806	5515209	53.40%	5.152%
45	14.168	1880	1884	1890	rVB8	10194	18547	0.18%	0.017%
46	14.286	1900	1904	1906	rBV4	19951	30399	0.29%	0.028%
47	14.333	1906	1912	1920	rVB	4244378	6080562	58.87%	5.681%
48	14.427	1925	1928	1932	rVB5	9604	15393	0.15%	0.014%
49	14.539	1942	1947	1953	rVB4	24493	35316	0.34%	0.033%
50	14.639	1957	1964	1973	rBV	3915801	5550850	53.74%	5.186%
51	14.827	1987	1996	2003	rBV	346567	569923	5.52%	0.532%
52	14.986	2021	2023	2029	rVB7	8232	11633	0.11%	0.011%
53	15.051	2029	2034	2040	rVB10	17491	33628	0.33%	0.031%
54	15.145	2048	2050	2057	rVB8	8208	14308	0.14%	0.013%
55	15.221	2059	2063	2066	rBV4	7146	11583	0.11%	0.011%
56	15.380	2084	2090	2095	rVB2	14930	24930	0.24%	0.023%
57	15.433	2095	2099	2104	rBV3	20000	41849	0.41%	0.039%
58	15.480	2104	2107	2110	rVV	22185	28410	0.28%	0.027%
59	15.527	2110	2115	2120	rVV	120745	165521	1.60%	0.155%
60	15.627	2125	2132	2144	rBV	5932503	8339928	80.75%	7.791%
61	15.739	2144	2151	2163	rBV	1466586	2002856	19.39%	1.871%
62	15.862	2168	2172	2180	rVB	50078	88894	0.86%	0.083%
63	15.992	2189	2194	2196	rBV6	6741	10609	0.10%	0.010%
64	16.262	2236	2240	2243	rBV6	12077	14697	0.14%	0.014%
65	16.304	2243	2247	2249	rBV5	13970	18182	0.18%	0.017%
66	16.345	2251	2254	2256	rVB4	14046	16432	0.16%	0.015%
67	16.410	2262	2265	2268	rVB3	24990	32810	0.32%	0.031%
68	16.774	2324	2327	2334	rVB6	16990	25937	0.25%	0.024%
69	16.868	2338	2343	2346	rVV2	17934	29263	0.28%	0.027%
70	17.051	2372	2374	2379	rVB6	9611	11122	0.11%	0.010%
71	17.133	2384	2388	2392	rBV2	65973	95399	0.92%	0.089%
72	17.245	2404	2407	2411	rBV5	17313	21592	0.21%	0.020%
73	17.298	2412	2416	2420	rVB4	20102	26547	0.26%	0.025%
74	17.374	2423	2429	2436	rBV	4427512	6317038	61.16%	5.902%
75	17.474	2440	2446	2456	rBV2	6558968	9090514	88.02%	8.493%
76	18.045	2540	2543	2548	rVB	29728	32983	0.32%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036685.D
 Acq On : 23 Sep 2022 20:00
 Operator : CG/JU
 Sample : N4708-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8K7

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

77	18.268	2576	2581	2590	rBV	259088	420144	4.07%	0.393%
78	19.321	2757	2760	2768	rBV2	77312	98574	0.95%	0.092%
79	19.392	2769	2772	2776	rBV2	77893	109095	1.06%	0.102%
80	19.539	2793	2797	2802	rBV2	126508	187458	1.81%	0.175%
81	19.756	2828	2834	2841	rBV	7776659	10328318	100.00%	9.649%
82	20.750	3000	3003	3007	rBV	223882	243357	2.36%	0.227%
83	21.250	3084	3088	3094	rBV	777733	970816	9.40%	0.907%
84	21.544	3133	3138	3145	rBV	4530715	5808579	56.24%	5.427%
85	23.827	3519	3526	3533	rBV2	3837766	7608022	73.66%	7.108%
86	23.980	3546	3552	3565	rVB2	2457829	5054526	48.94%	4.722%




Sum of corrected areas: 107039828

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036685.D
Acq On : 23 Sep 2022 20:00
Operator : CG/JU
Sample : N4708-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

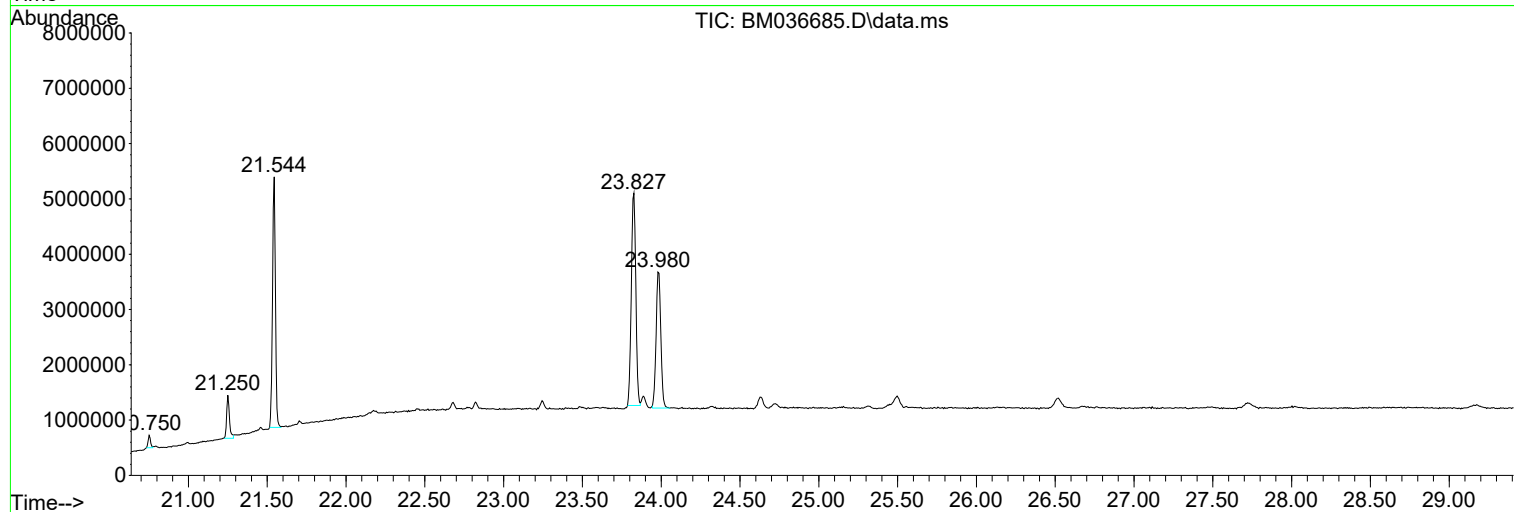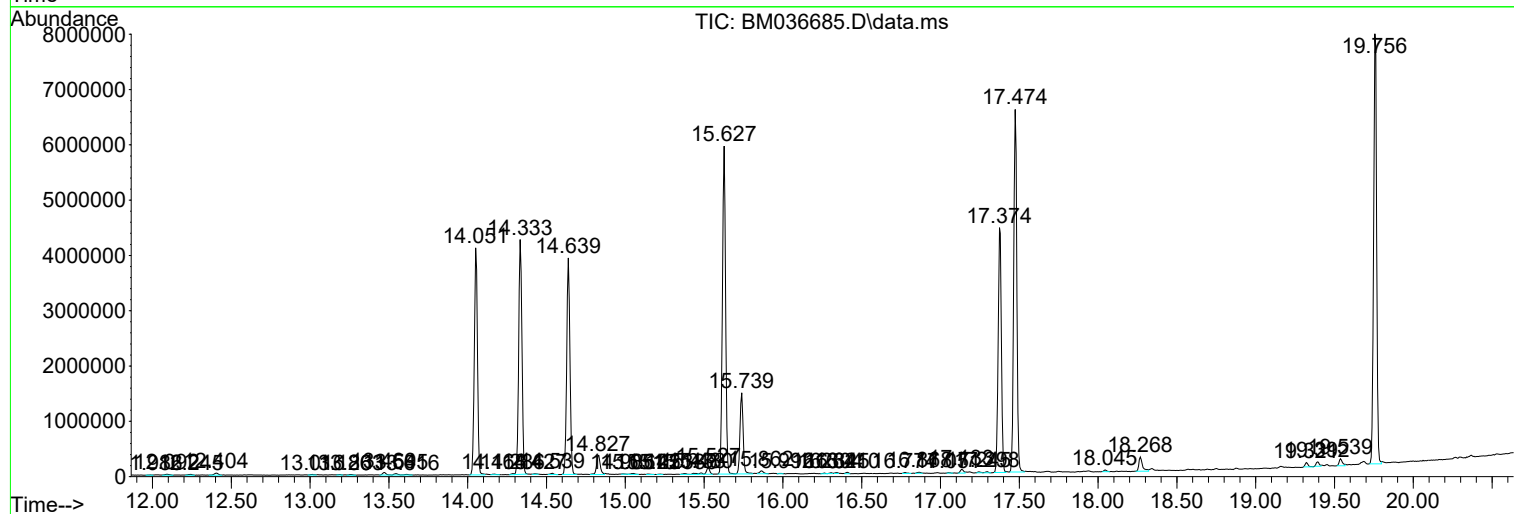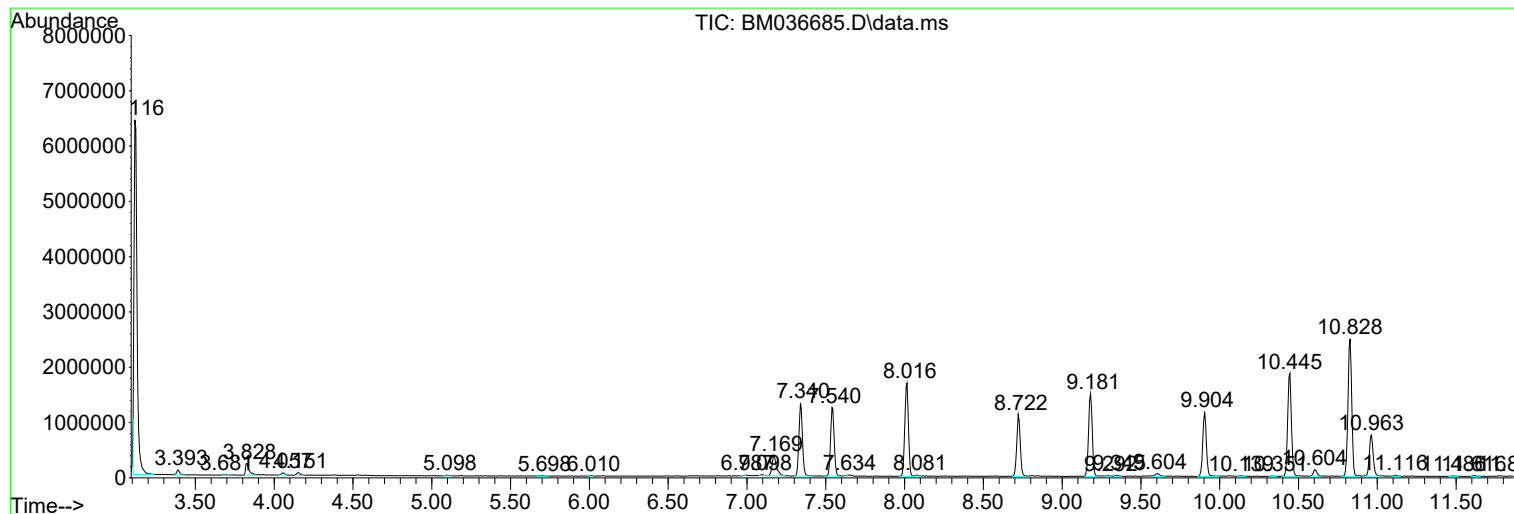

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036685.D
Acq On : 23 Sep 2022 20:00
Operator : CG/JU
Sample : N4708-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036685.D
Acq On : 23 Sep 2022 20:00
Operator : CG/JU
Sample : N4708-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8K7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc