

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036689.D
 Acq On : 23 Sep 2022 23:00
 Operator : CG/JU
 Sample : PB147828BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK828

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	3	5	20	rVB	207935	278986	3.23%	0.289%
2	3.387	47	51	61	rVB	111891	148068	1.71%	0.153%
3	3.817	120	124	141	rBV	1212642	1854906	21.46%	1.921%
4	4.152	177	181	187	rVB	27397	41530	0.48%	0.043%
5	7.169	687	694	707	rVB	1695944	2598855	30.07%	2.692%
6	7.340	716	723	734	rVB	1461297	2190869	25.35%	2.269%
7	7.540	749	757	767	rBV	1739852	2675304	30.95%	2.771%
8	8.010	830	837	849	rBV	1494424	2317217	26.81%	2.400%
9	8.722	950	958	971	rBV	2128519	3382744	39.13%	3.504%
10	9.175	1026	1035	1046	rBV	1591716	2602382	30.11%	2.696%
11	9.904	1151	1159	1170	rBV	1207551	2026659	23.45%	2.099%
12	10.440	1243	1250	1262	rBV	2076499	3366002	38.94%	3.487%
13	10.822	1307	1315	1324	rBV	2191494	3653890	42.27%	3.785%
14	10.957	1331	1338	1356	rBV	2063172	3381610	39.12%	3.503%
15	12.404	1577	1584	1592	rBV	40512	69086	0.80%	0.072%
16	12.616	1613	1620	1624	rBV9	5136	10356	0.12%	0.011%
17	13.616	1785	1790	1795	rBV4	7104	12849	0.15%	0.013%
18	14.051	1856	1864	1872	rBV	3749120	5060376	58.54%	5.242%
19	14.333	1904	1912	1923	rBV	4376241	6069708	70.22%	6.287%
20	14.404	1923	1924	1933	rVB8	6673	12995	0.15%	0.013%
21	14.633	1956	1963	1974	rBV	3399892	5031179	58.21%	5.212%
22	14.828	1989	1996	2011	rBV	1597895	2372737	27.45%	2.458%
23	14.992	2022	2024	2029	rVB6	6762	10423	0.12%	0.011%
24	15.039	2029	2032	2037	rVB6	6383	9733	0.11%	0.010%
25	15.622	2125	2131	2144	rBV	5370540	7703192	89.12%	7.979%
26	15.733	2144	2150	2162	rBV	1088889	1489447	17.23%	1.543%
27	15.863	2167	2172	2181	rVB	47746	77280	0.89%	0.080%
28	16.404	2260	2264	2269	rBV4	16082	22809	0.26%	0.024%
29	16.863	2339	2342	2345	rVB2	12379	13663	0.16%	0.014%
30	17.051	2372	2374	2378	rVB4	8085	9929	0.11%	0.010%
31	17.169	2390	2394	2398	rVB5	6884	11568	0.13%	0.012%
32	17.374	2422	2429	2438	rBV	4062681	5690143	65.83%	5.894%
33	17.474	2439	2446	2461	rVV	5775986	8067389	93.33%	8.357%
34	17.939	2521	2525	2529	rVB2	11942	16040	0.19%	0.017%
35	19.321	2756	2760	2765	rVB	63489	77841	0.90%	0.081%
36	19.392	2768	2772	2777	rVB	62418	84556	0.98%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036689.D
Acq On : 23 Sep 2022 23:00
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	19.757	2828	2834	2845	rBV	6630563	8643888	100.00%	8.954%
38	20.751	3000	3003	3007	rBV	146500	160935	1.86%	0.167%
39	21.539	3132	3137	3146	rBV	3885796	5020003	58.08%	5.200%
40	23.821	3519	3525	3532	rVB2	3115570	5986878	69.26%	6.201%
41	23.980	3546	3552	3564	rVB2	2167914	4285667	49.58%	4.439%




Sum of corrected areas: 96539692

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036689.D
Acq On : 23 Sep 2022 23:00
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

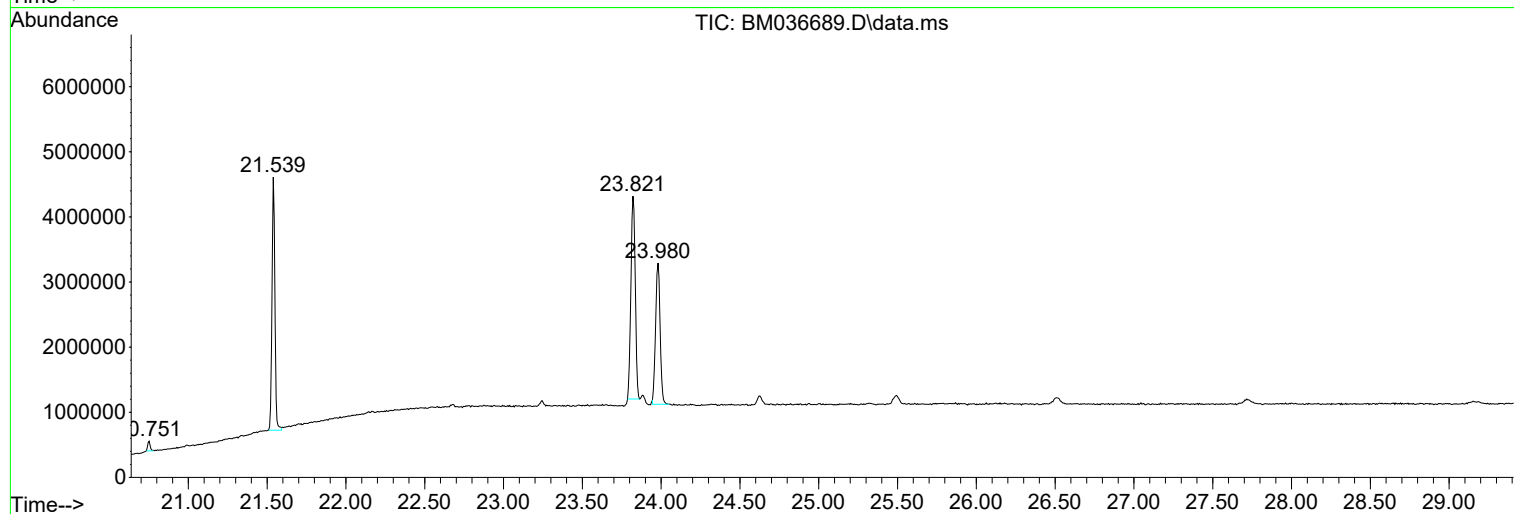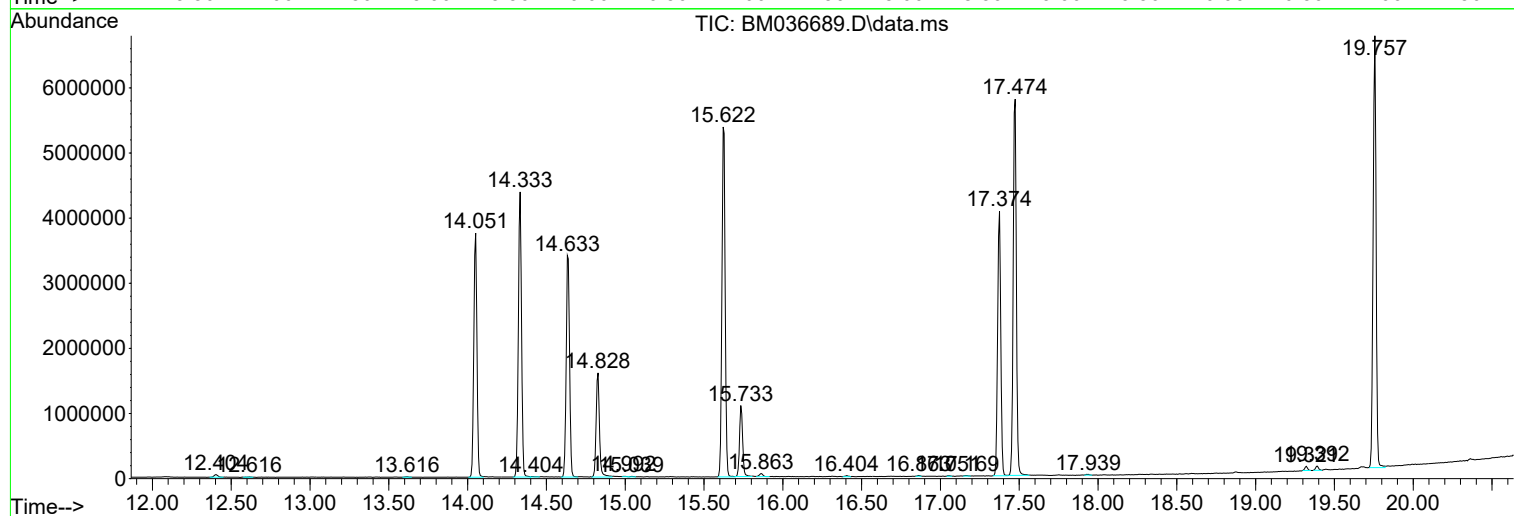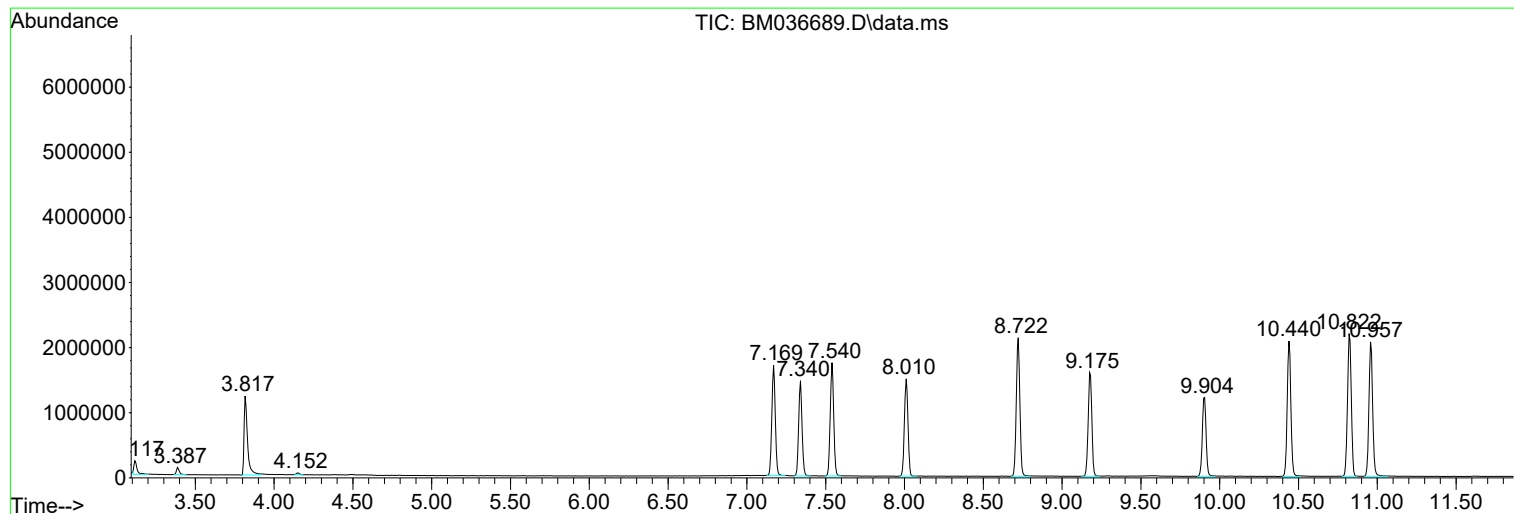

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036689.D
Acq On : 23 Sep 2022 23:00
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.117	2.41 ng/ul	278986	1,4-Dichlorobenzene-d4	8.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	25
5			1,3-Dioxolane, 2-propyl-	116	C6H12O2	003390-13-4	23

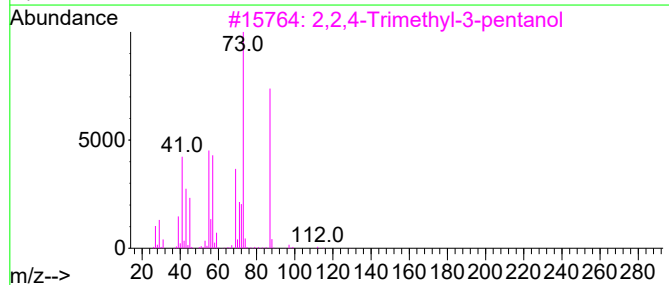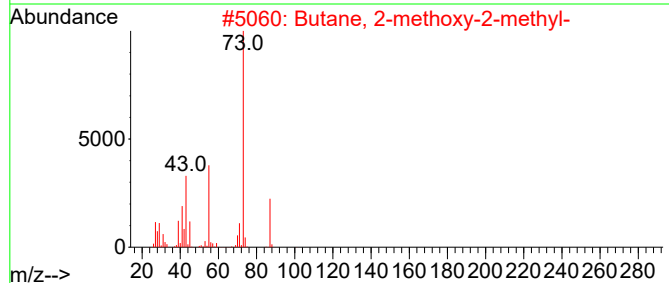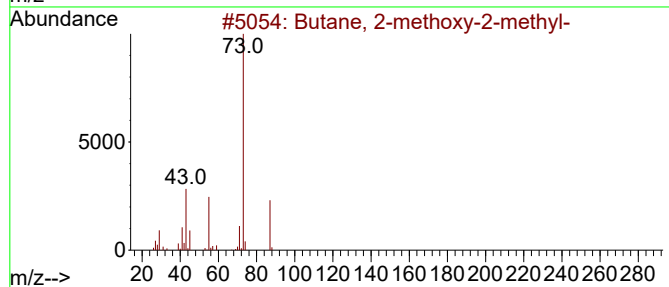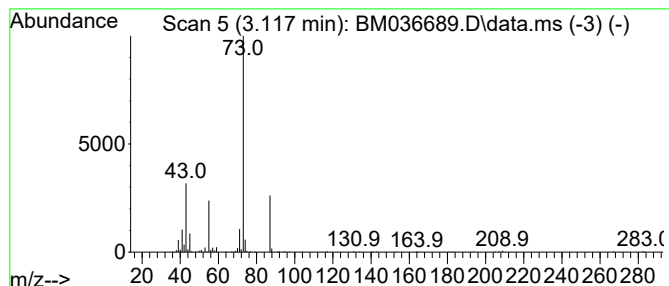

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036689.D
Acq On : 23 Sep 2022 23:00
Operator : CG/JU
Sample : PB147828BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK828

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.117	2.4	ng/ul	278986	1	8.010	2317220	20.0