

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036694.D
 Acq On : 24 Sep 2022 01:59
 Operator : CG/JU
 Sample : N4649-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	25	rVB	7499579	8954754	98.07%	8.570%
2	3.387	47	51	60	rVB	90515	123504	1.35%	0.118%
3	3.822	122	125	137	rBV	416219	665514	7.29%	0.637%
4	4.057	160	165	171	rVB	43636	65103	0.71%	0.062%
5	4.152	177	181	189	rVB	32866	47636	0.52%	0.046%
6	5.099	338	342	348	rVB	42524	62866	0.69%	0.060%
7	7.169	687	694	704	rVB	412210	665663	7.29%	0.637%
8	7.340	716	723	732	rVB	1586404	2497935	27.36%	2.391%
9	7.540	750	757	768	rBV	1536996	2384076	26.11%	2.282%
10	7.634	768	773	777	rVB7	7026	13283	0.15%	0.013%
11	7.892	812	817	823	rBV8	6130	11416	0.13%	0.011%
12	8.010	830	837	846	rBV	1703075	2644610	28.96%	2.531%
13	8.716	950	957	972	rBV	1213428	1933594	21.18%	1.851%
14	9.175	1026	1035	1049	rBV	1859779	2986052	32.70%	2.858%
15	9.286	1049	1054	1059	rVV9	9350	16495	0.18%	0.016%
16	9.328	1059	1061	1068	rVV8	5521	10400	0.11%	0.010%
17	9.898	1149	1158	1171	rBV	1339077	2170627	23.77%	2.077%
18	10.128	1193	1197	1201	rBV7	5593	10580	0.12%	0.010%
19	10.439	1242	1250	1262	rBV	2123507	3423003	37.49%	3.276%
20	10.616	1275	1280	1285	rBV8	10308	21575	0.24%	0.021%
21	10.686	1287	1292	1298	rVB6	17731	34446	0.38%	0.033%
22	10.822	1307	1315	1323	rBV	2497181	4069227	44.56%	3.894%
23	10.957	1329	1338	1359	rBV	2118726	3526291	38.62%	3.375%
24	11.157	1368	1372	1377	rVB8	6920	9655	0.11%	0.009%
25	11.610	1442	1449	1455	rBV8	8342	15361	0.17%	0.015%
26	12.080	1527	1529	1539	rVB6	8770	18195	0.20%	0.017%
27	12.398	1577	1583	1591	rBV2	40515	72420	0.79%	0.069%
28	12.475	1591	1596	1603	rVB2	14933	25939	0.28%	0.025%
29	12.610	1610	1619	1625	rVB2	6735	17052	0.19%	0.016%
30	12.692	1628	1633	1637	rBV4	9514	15045	0.16%	0.014%
31	12.833	1650	1657	1662	rBV3	32034	55325	0.61%	0.053%
32	13.269	1725	1731	1736	rVB2	27795	45240	0.50%	0.043%
33	13.474	1760	1766	1770	rBV	18696	30968	0.34%	0.030%
34	13.516	1770	1773	1780	rVV3	19187	35472	0.39%	0.034%
35	13.610	1783	1789	1794	rVV8	7343	13909	0.15%	0.013%
36	13.969	1843	1850	1853	rVB9	7192	11735	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036694.D
 Acq On : 24 Sep 2022 01:59
 Operator : CG/JU
 Sample : N4649-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	14.045	1856	1863	1879	rVV	4011261	5600856	61.34%	5.360%
38	14.333	1904	1912	1921	rBV	4461739	6584261	72.11%	6.302%
39	14.633	1956	1963	1971	rBV	3649890	5255852	57.56%	5.030%
40	14.698	1971	1974	1982	rVB7	13787	28816	0.32%	0.028%
41	14.821	1988	1995	2009	rBV	266661	452070	4.95%	0.433%
42	15.039	2027	2032	2038	rVB2	27838	58245	0.64%	0.056%
43	15.621	2124	2131	2137	rBV	6123887	8625462	94.46%	8.255%
44	15.674	2137	2140	2144	rVV3	33333	48634	0.53%	0.047%
45	15.733	2144	2150	2160	rVV	1165726	1541092	16.88%	1.475%
46	15.857	2166	2171	2178	rVB2	50641	92163	1.01%	0.088%
47	16.404	2259	2264	2268	rVB6	16996	26380	0.29%	0.025%
48	16.562	2288	2291	2296	rBV5	12109	15974	0.17%	0.015%
49	16.680	2307	2311	2314	rVB5	7907	11296	0.12%	0.011%
50	16.862	2337	2342	2346	rBV4	14241	21279	0.23%	0.020%
51	17.051	2371	2374	2378	rVB5	10871	13295	0.15%	0.013%
52	17.227	2399	2404	2406	rBV5	5208	9359	0.10%	0.009%
53	17.374	2422	2429	2435	rBV	3757287	5494081	60.17%	5.258%
54	17.468	2439	2445	2456	rVV	6470040	9131061	100.00%	8.739%
55	17.557	2457	2460	2467	rVB7	33533	53409	0.58%	0.051%
56	17.933	2521	2524	2529	rVB3	16364	20985	0.23%	0.020%
57	18.262	2576	2580	2585	rBV2	53112	76199	0.83%	0.073%
58	19.321	2756	2760	2766	rVB3	67794	96385	1.06%	0.092%
59	19.386	2768	2771	2775	rVV2	65486	84189	0.92%	0.081%
60	19.533	2793	2796	2800	rBV4	42708	57802	0.63%	0.055%
61	19.751	2827	2833	2847	rBV	6526893	9126846	99.95%	8.735%
62	20.745	2999	3002	3007	rVB	248922	268826	2.94%	0.257%
63	21.539	3132	3137	3145	rBV	3319648	4402308	48.21%	4.213%
64	23.821	3518	3525	3531	rBV	3436171	6674549	73.10%	6.388%
65	23.974	3545	3551	3562	rVB2	1955072	3910379	42.83%	3.742%




Sum of corrected areas: 104487019

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036694.D
Acq On : 24 Sep 2022 01:59
Operator : CG/JU
Sample : N4649-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

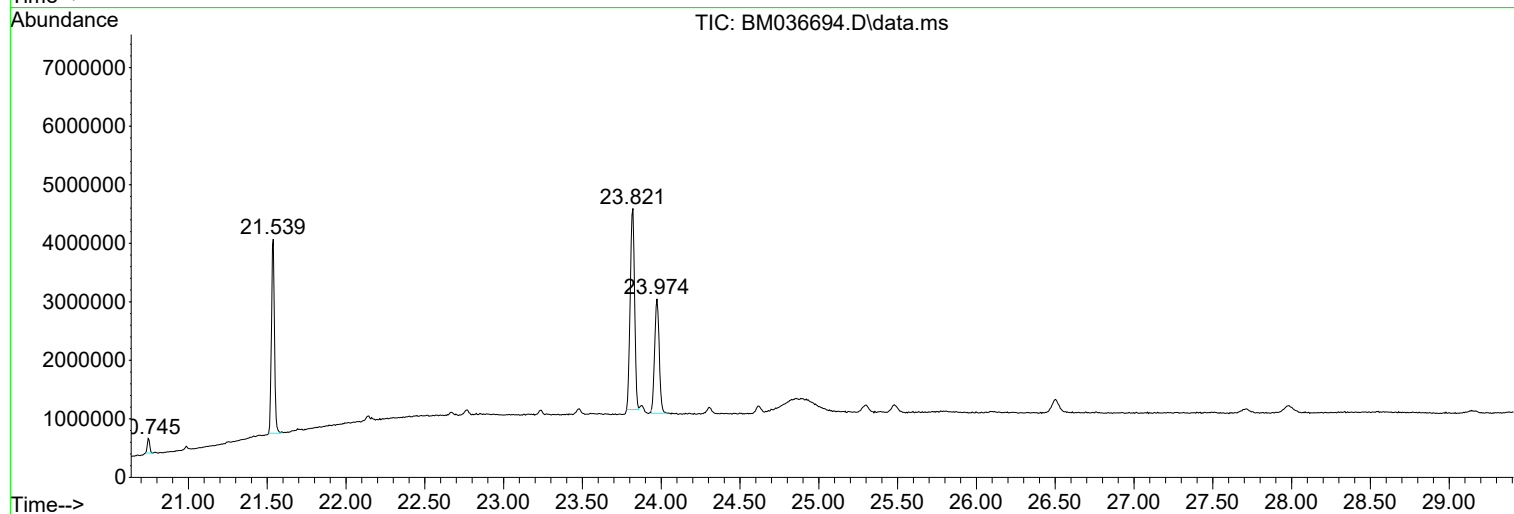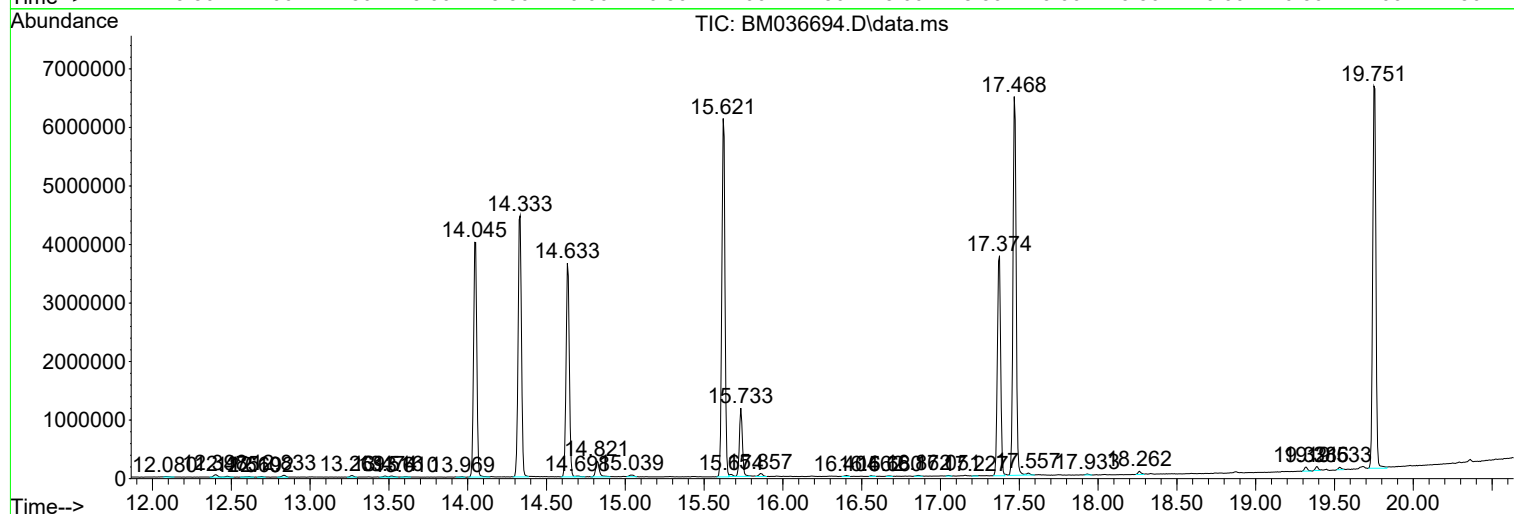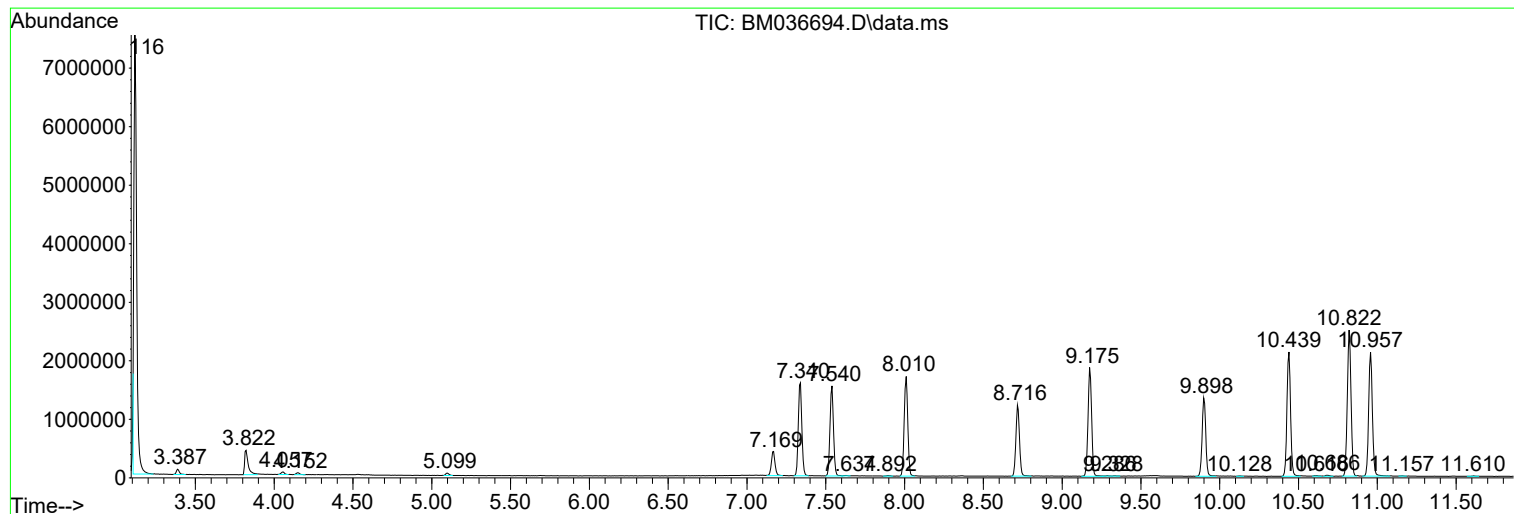

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036694.D
Acq On : 24 Sep 2022 01:59
Operator : CG/JU
Sample : N4649-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ17










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.116	67.72 ng/ul	8954750	1,4-Dichlorobenzene-d4	8.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83		
2	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78		
3	2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39		
4	Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23		
5	Silane, tetramethyl-	88	C4H12Si	000075-76-3	9		

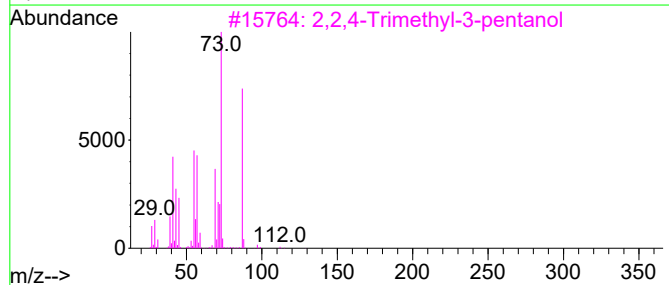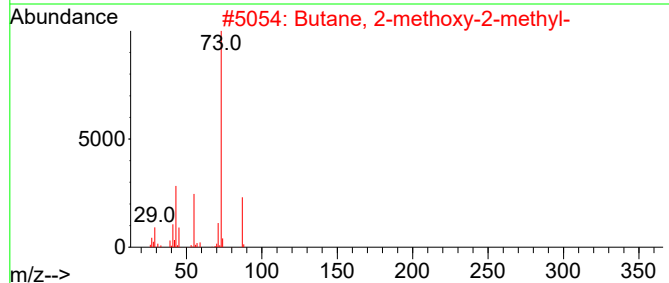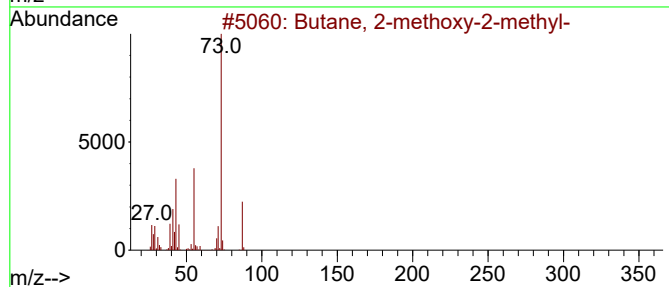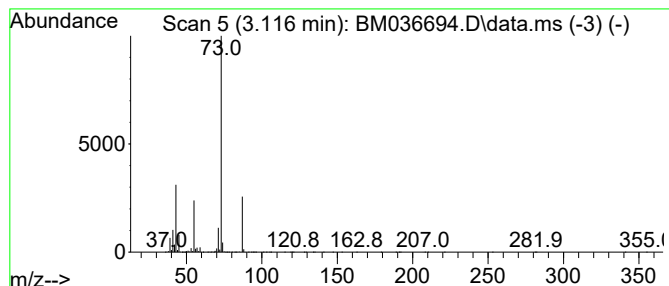

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036694.D
Acq On : 24 Sep 2022 01:59
Operator : CG/JU
Sample : N4649-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ17

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.116	67.7	ng/ul	8954750	1	8.010	2644610	20.0