

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036730.D
 Acq On : 25 Sep 2022 01:23
 Operator : CG/JU
 Sample : N4662-08
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ33

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	3	4	23	rVB	6684184	7534988	86.14%	8.344%
2	3.381	47	50	59	rVB	75911	106268	1.21%	0.118%
3	3.816	122	124	141	rBV	226882	406004	4.64%	0.450%
4	4.046	159	163	175	rVB	40915	71123	0.81%	0.079%
5	4.140	176	179	186	rVB	22077	30859	0.35%	0.034%
6	4.687	268	272	277	rVB5	10530	17712	0.20%	0.020%
7	5.081	336	339	344	rVB5	6132	9816	0.11%	0.011%
8	7.157	687	692	704	rVB	386436	617462	7.06%	0.684%
9	7.328	714	721	734	rVB	1365048	2181592	24.94%	2.416%
10	7.534	747	756	766	rBV	1289925	2085035	23.84%	2.309%
11	8.004	829	836	844	rBV	1276748	2027970	23.18%	2.246%
12	8.710	949	956	967	rBV	1127812	1790058	20.46%	1.982%
13	9.169	1025	1034	1043	rBV	1662123	2646278	30.25%	2.931%
14	9.281	1048	1053	1056	rVV7	6706	13347	0.15%	0.015%
15	9.328	1058	1061	1067	rVB6	5295	10297	0.12%	0.011%
16	9.587	1102	1105	1111	rVB8	10572	20085	0.23%	0.022%
17	9.892	1148	1157	1172	rBV	1203433	1924372	22.00%	2.131%
18	10.428	1240	1248	1261	rBV	1851732	3092673	35.36%	3.425%
19	10.598	1273	1277	1283	rBV7	9671	21838	0.25%	0.024%
20	10.816	1305	1314	1322	rBV	1888317	3125996	35.74%	3.462%
21	10.951	1329	1337	1347	rBV	1125193	1958882	22.39%	2.169%
22	12.081	1524	1529	1536	rVB3	10195	24997	0.29%	0.028%
23	12.392	1576	1582	1589	rVB2	37169	60500	0.69%	0.067%
24	13.257	1724	1729	1734	rBV3	17167	26360	0.30%	0.029%
25	13.463	1759	1764	1767	rBV8	6661	10288	0.12%	0.011%
26	13.527	1769	1775	1784	rBV	54029	95580	1.09%	0.106%
27	13.598	1784	1787	1798	rVB9	7568	17375	0.20%	0.019%
28	14.039	1855	1862	1876	rBV	3655891	4959331	56.70%	5.492%
29	14.322	1900	1910	1926	rBV	4134516	5961344	68.15%	6.602%
30	14.527	1942	1945	1951	rVB8	6695	11736	0.13%	0.013%
31	14.627	1955	1962	1970	rBV	2850915	4124863	47.16%	4.568%
32	14.816	1988	1994	2007	rBV	275580	435613	4.98%	0.482%
33	15.039	2027	2032	2038	rVB8	19404	29868	0.34%	0.033%
34	15.369	2083	2088	2092	rBV2	6300	11122	0.13%	0.012%
35	15.616	2123	2130	2138	rBV	5703889	7863731	89.90%	8.709%
36	15.727	2143	2149	2161	rVV	1179430	1593626	18.22%	1.765%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036730.D
 Acq On : 25 Sep 2022 01:23
 Operator : CG/JU
 Sample : N4662-08
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXZ33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	15.857	2164	2171	2176	rVB2	47837	79342	0.91%	0.088%
38	16.304	2242	2247	2249	rBV5	6831	11712	0.13%	0.013%
39	16.392	2258	2262	2267	rBV6	14619	18894	0.22%	0.021%
40	16.851	2336	2340	2343	rBV3	12129	14750	0.17%	0.016%
41	17.045	2369	2373	2377	rBV6	8233	11443	0.13%	0.013%
42	17.363	2421	2427	2437	rBV	3296691	4520229	51.68%	5.006%
43	17.463	2438	2444	2464	rVV	6269476	8569336	97.97%	9.490%
44	17.921	2519	2522	2526	rVB3	12956	15358	0.18%	0.017%
45	18.251	2574	2578	2587	rBV2	109643	181380	2.07%	0.201%
46	19.309	2754	2758	2762	rBV2	64168	93214	1.07%	0.103%
47	19.380	2767	2770	2774	rVV	67074	87300	1.00%	0.097%
48	19.527	2791	2795	2801	rBV4	74287	113602	1.30%	0.126%
49	19.745	2826	2832	2842	rBV	6751740	8747130	100.00%	9.687%
50	20.739	2998	3001	3005	rBV	128769	130432	1.49%	0.144%
51	21.527	3131	3135	3141	rBV	2693334	3551867	40.61%	3.933%
52	23.803	3516	3522	3530	rBV2	3078979	6054918	69.22%	6.705%
53	23.962	3543	3549	3560	rVB2	1598619	3179533	36.35%	3.521%


Sum of corrected areas: 90299429

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036730.D
Acq On : 25 Sep 2022 01:23
Operator : CG/JU
Sample : N4662-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

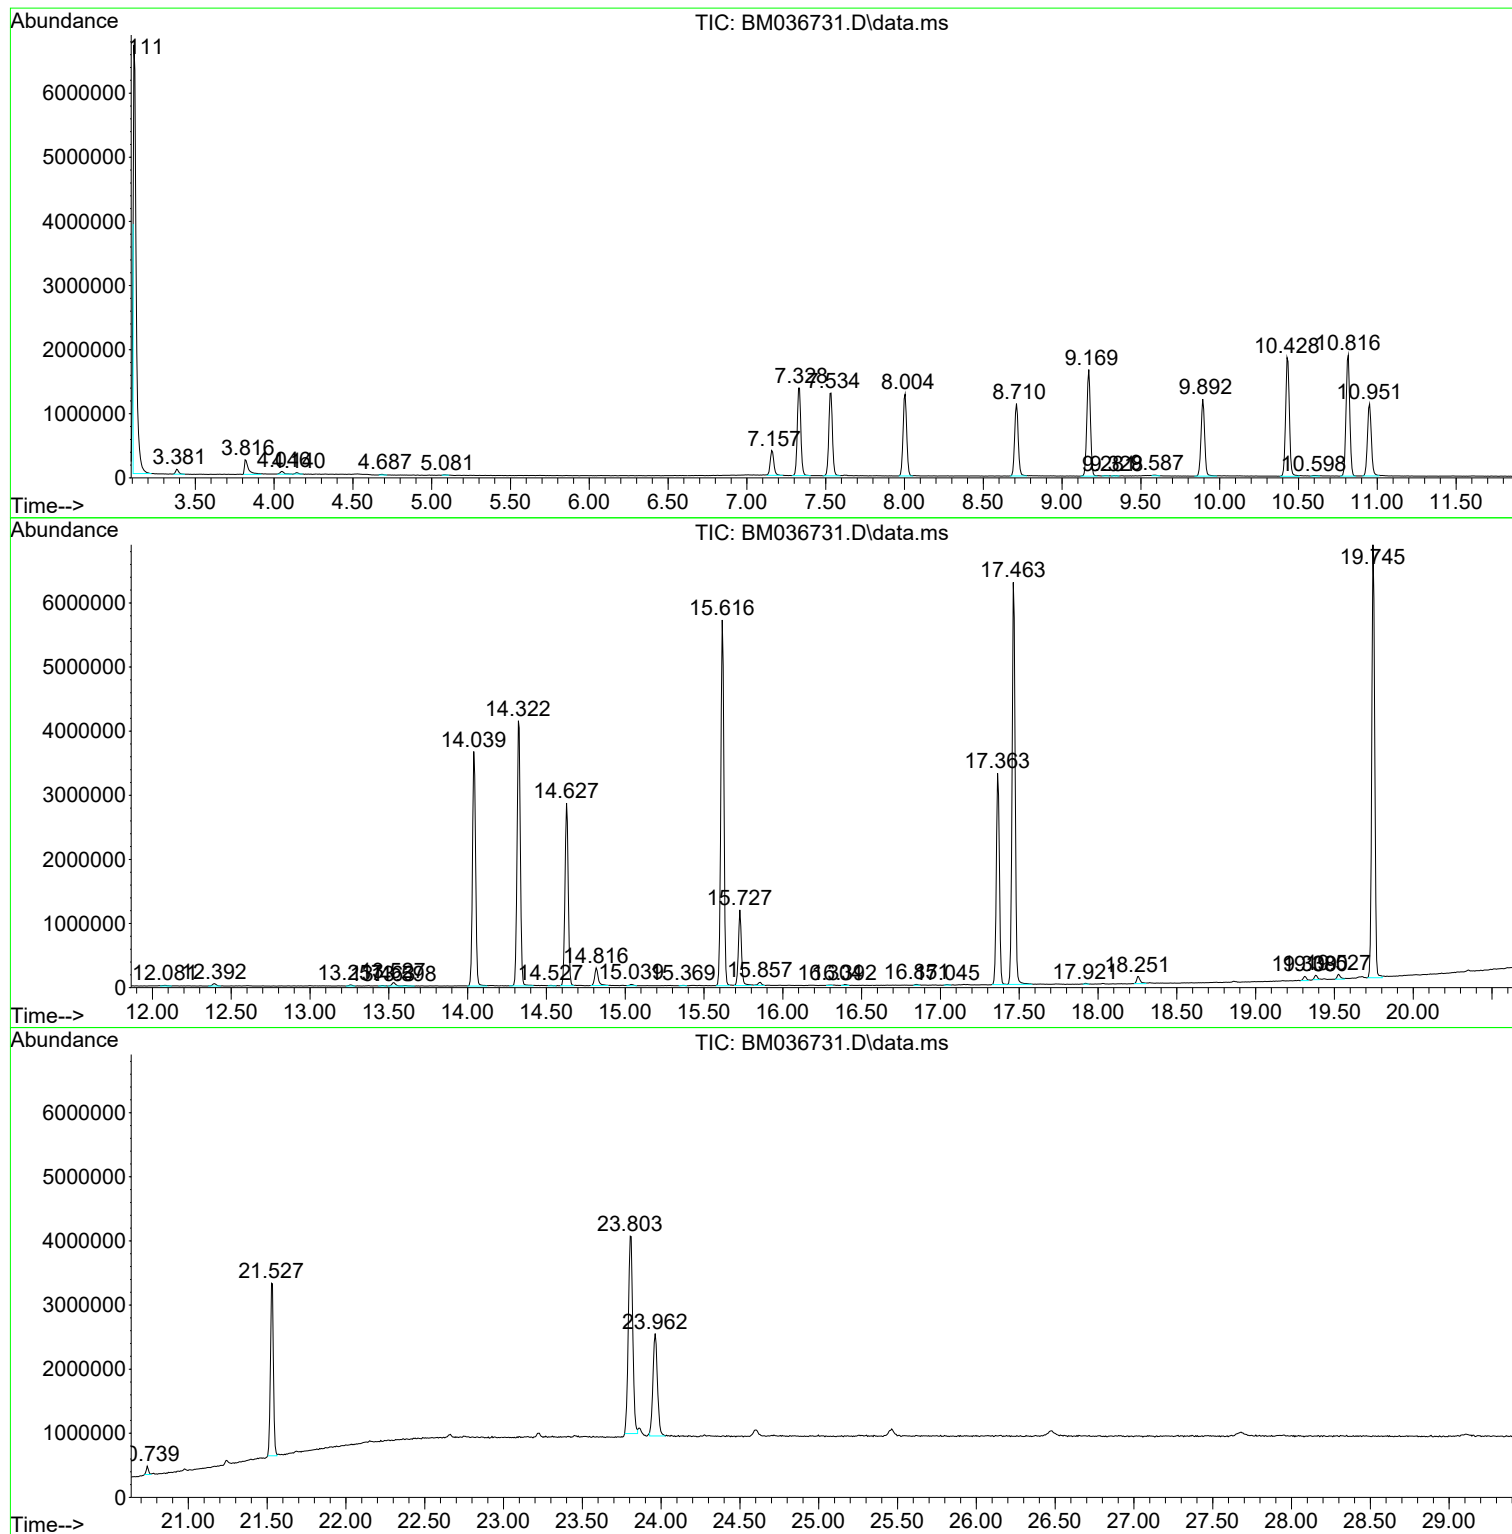

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036730.D
Acq On : 25 Sep 2022 01:23
Operator : CG/JU
Sample : N4662-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ33










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.111	74.31 ng/ul	7534990	1,4-Dichlorobenzene-d4	8.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	80
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Borane, dimethoxy-	74	C2H7BO2	004542-61-4	9

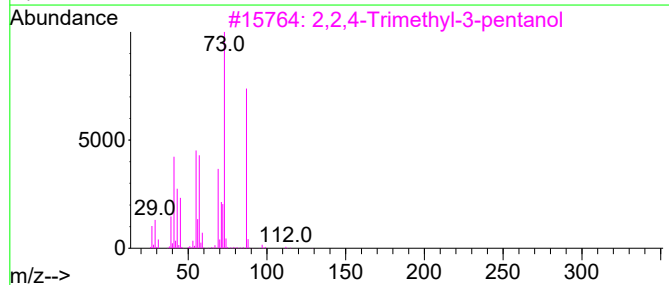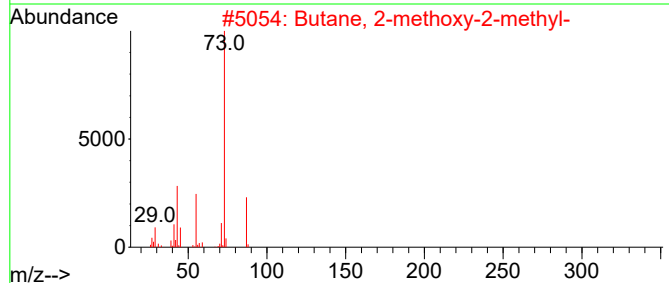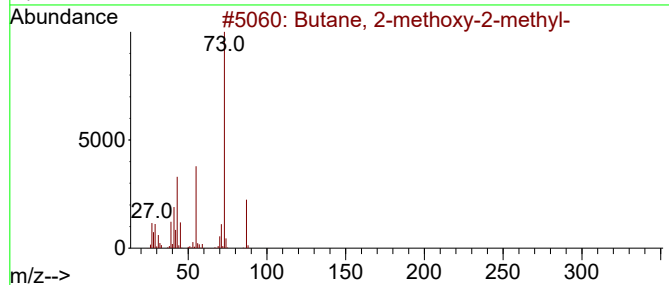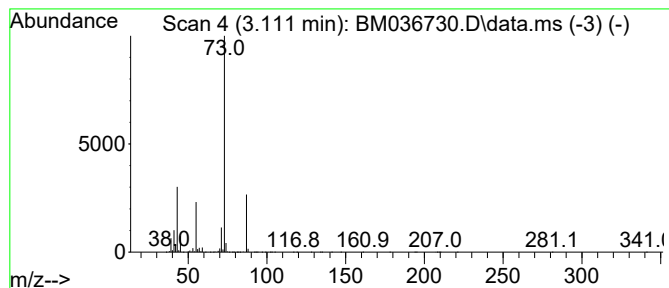

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036730.D
Acq On : 25 Sep 2022 01:23
Operator : CG/JU
Sample : N4662-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXZ33

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	3.111	74.3	ng/ul	7534990	1	8.004	2027970	20.0