

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036732.D
 Acq On : 25 Sep 2022 02:35
 Operator : CG/JU
 Sample : PB147827BL
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK827

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036733.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	51	rVB	1649303	1845818	46.94%	9.439%
2	3.651	92	96	101	rVB	41148	54364	1.38%	0.278%
3	4.134	176	178	185	rVB2	20198	25826	0.66%	0.132%
4	5.598	426	427	430	rBV3	3803	4561	0.12%	0.023%
5	6.622	598	601	603	rBV4	3278	3964	0.10%	0.020%
6	6.722	614	618	621	rBV5	3473	4503	0.11%	0.023%
7	7.392	730	732	738	rVB7	3663	7028	0.18%	0.036%
8	7.439	738	740	747	rVB8	2514	4693	0.12%	0.024%
9	7.998	828	835	845	rBV	983884	1551461	39.45%	7.934%
10	8.828	969	976	979	rBV9	2127	5091	0.13%	0.026%
11	9.498	1085	1090	1091	rBV5	2981	4617	0.12%	0.024%
12	9.563	1099	1101	1105	rVB5	3675	4109	0.10%	0.021%
13	9.904	1157	1159	1163	rVB5	2857	4339	0.11%	0.022%
14	10.475	1254	1256	1259	rVB4	3706	4704	0.12%	0.024%
15	10.510	1259	1262	1263	rBV3	3708	4157	0.11%	0.021%
16	10.810	1304	1313	1327	rBV	1283110	2181980	55.49%	11.158%
17	12.074	1522	1528	1530	rBV4	8363	14056	0.36%	0.072%
18	12.221	1549	1553	1557	rVB7	4184	7715	0.20%	0.039%
19	12.527	1602	1605	1610	rVB7	2464	4493	0.11%	0.023%
20	12.998	1678	1685	1689	rBV9	2999	6480	0.16%	0.033%
21	13.127	1705	1707	1711	rBV4	3169	4634	0.12%	0.024%
22	14.051	1859	1864	1867	rBV5	9955	16427	0.42%	0.084%
23	14.527	1943	1945	1949	rBV5	2487	3938	0.10%	0.020%
24	14.627	1955	1962	1972	rBV	2024086	2923168	74.34%	14.948%
25	14.992	2019	2024	2028	rBV8	2762	4507	0.11%	0.023%
26	15.609	2124	2129	2136	rBV6	9177	19735	0.50%	0.101%
27	15.880	2173	2175	2179	rVB4	4324	4372	0.11%	0.022%
28	16.015	2195	2198	2199	rBV3	4314	4020	0.10%	0.021%
29	16.574	2290	2293	2295	rVB4	3659	4226	0.11%	0.022%
30	16.598	2295	2297	2299	rBV3	4644	4385	0.11%	0.022%
31	16.851	2337	2340	2345	rBV3	10401	15192	0.39%	0.078%
32	17.362	2421	2427	2440	rBV	2740533	3932252	100.00%	20.109%
33	17.921	2519	2522	2526	rBV5	9567	13651	0.35%	0.070%
34	18.033	2538	2541	2547	rBV7	8588	11691	0.30%	0.060%
35	18.321	2588	2590	2591	rBV2	6334	5017	0.13%	0.026%
36	20.739	2998	3001	3006	rBV2	107856	119315	3.03%	0.610%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036732.D
Acq On : 25 Sep 2022 02:35
Operator : CG/JU
Sample : PB147827BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

37	21.527	3131	3135	3141	rBV	2757174	3561300	90.57%	18.212%
38	23.962	3543	3549	3561	rVB2	1601693	3163309	80.45%	16.176%




Sum of corrected areas: 19555098

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036732.D
Acq On : 25 Sep 2022 02:35
Operator : CG/JU
Sample : PB147827BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

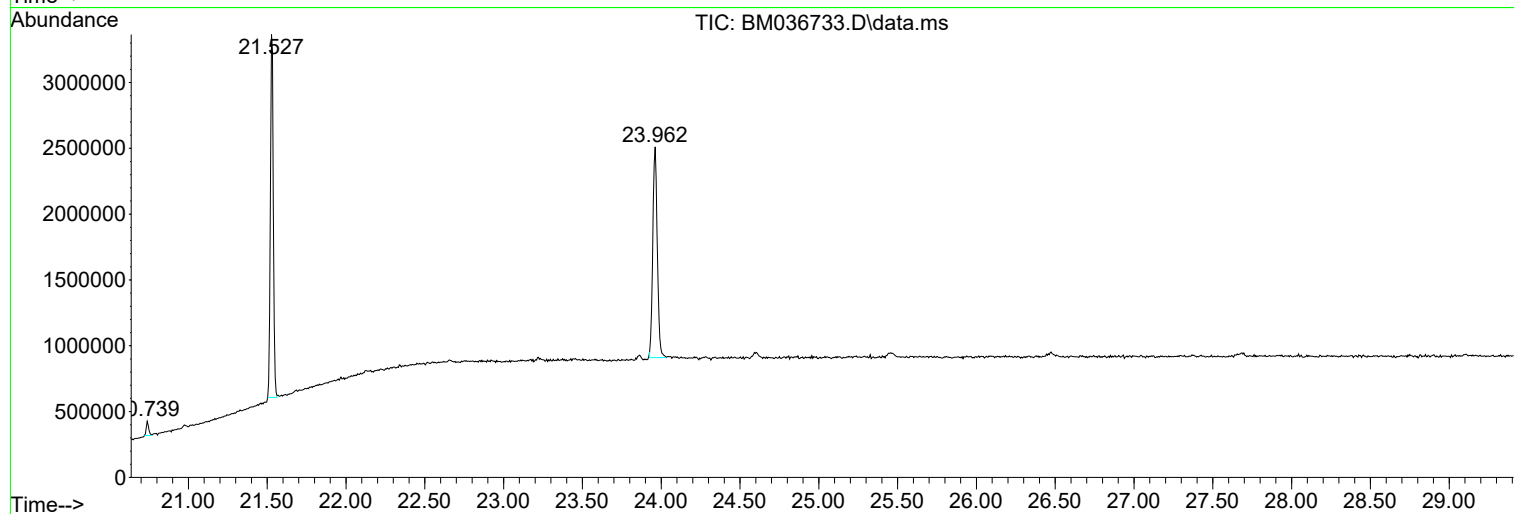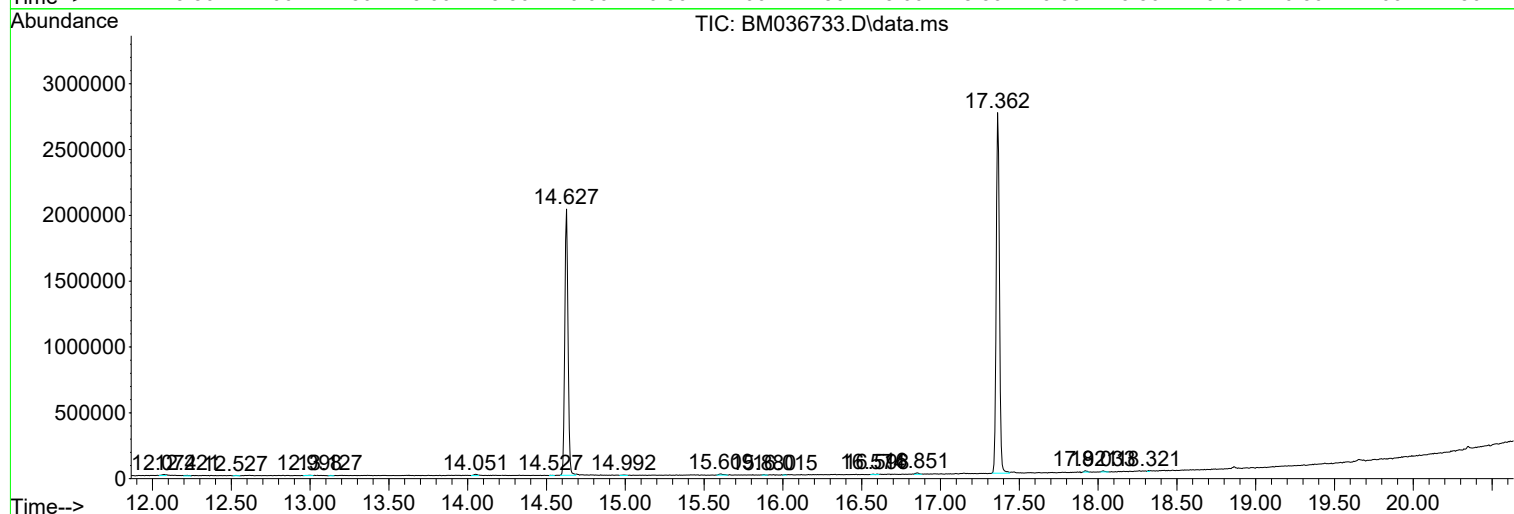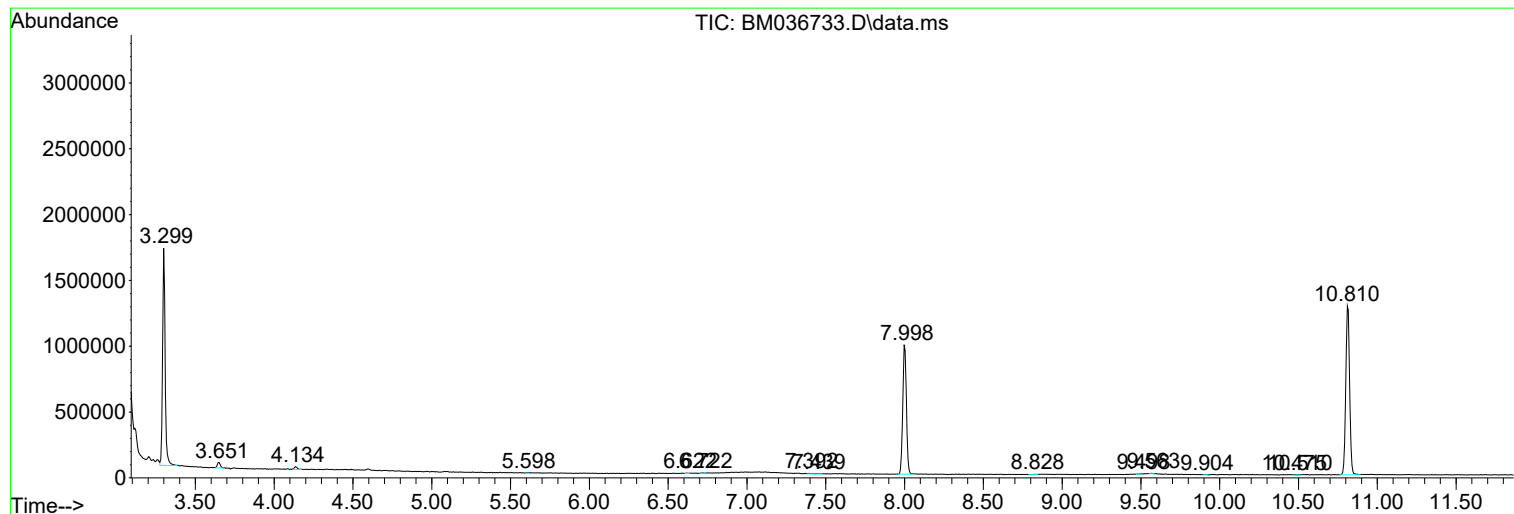

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036732.D
Acq On : 25 Sep 2022 02:35
Operator : CG/JU
Sample : PB147827BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.299	23.79 ng/ul	1845820	1,4-Dichlorobenzene-d4	7.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	94
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	90
4			Heptane	100	C7H16	000142-82-5	86
5			Hexane, 3-methyl-	100	C7H16	000589-34-4	43

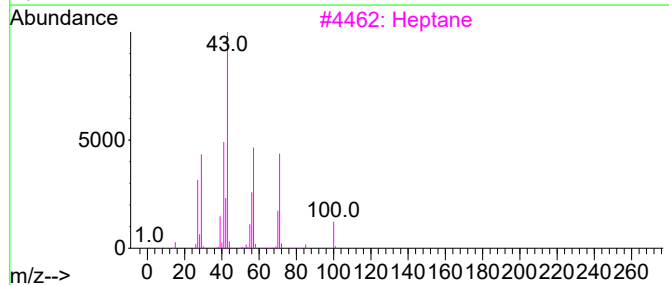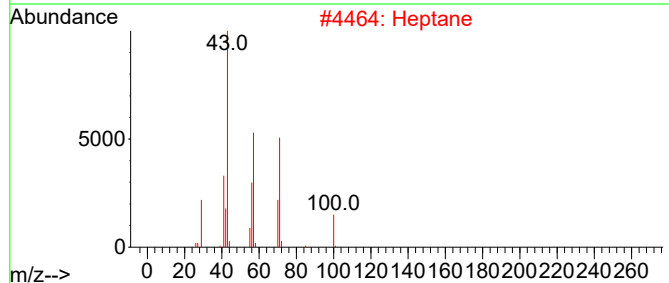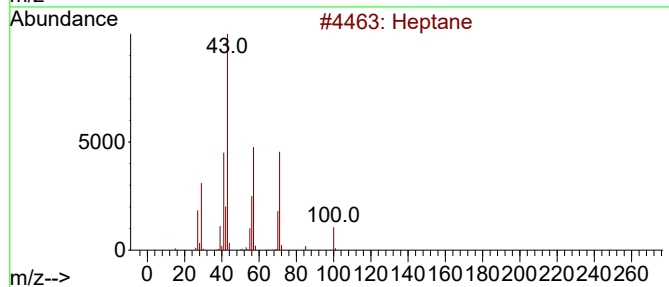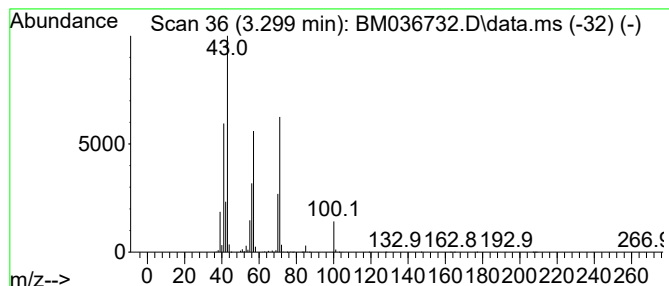

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036732.D
Acq On : 25 Sep 2022 02:35
Operator : CG/JU
Sample : PB147827BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.299	23.8	ng/ul	1845820	1	7.998	1551460	20.0