

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036734.D
 Acq On : 25 Sep 2022 03:46
 Operator : CG/JU
 Sample : N4693-08
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

Signal : TIC: BM036735.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	16	rVB2	313835	420063	8.47%	1.459%
2	3.210	17	21	24	rVV	75901	86159	1.74%	0.299%
3	3.240	24	26	28	rVV3	33105	34418	0.69%	0.120%
4	3.263	28	30	33	rVV	52680	55842	1.13%	0.194%
5	3.304	33	37	48	rVB	4804860	4956591	100.00%	17.214%
6	3.622	88	91	93	rBV4	16796	18624	0.38%	0.065%
7	3.652	93	96	103	rVB	135758	163667	3.30%	0.568%
8	3.746	110	112	117	rVB6	11835	10976	0.22%	0.038%
9	4.140	175	179	185	rVB	29713	38400	0.77%	0.133%
10	4.599	253	257	261	rVB2	18716	30709	0.62%	0.107%
11	4.904	305	309	311	rBV4	4942	7126	0.14%	0.025%
12	5.004	323	326	330	rVB5	8076	9713	0.20%	0.034%
13	5.287	371	374	376	rBV4	4941	6018	0.12%	0.021%
14	5.469	404	405	411	rBV7	3956	7586	0.15%	0.026%
15	5.998	493	495	499	rVB5	5178	6694	0.14%	0.023%
16	6.475	573	576	580	rVB6	4574	6379	0.13%	0.022%
17	7.998	829	835	848	rBV	1188125	1876296	37.85%	6.516%
18	8.139	854	859	864	rVB8	5218	10626	0.21%	0.037%
19	8.545	927	928	935	rVB7	5433	7034	0.14%	0.024%
20	9.551	1095	1099	1102	rBV6	4734	7794	0.16%	0.027%
21	9.763	1131	1135	1137	rBV5	3588	5326	0.11%	0.018%
22	10.204	1207	1210	1214	rVB6	5163	6273	0.13%	0.022%
23	10.498	1253	1260	1267	rBV6	8143	15808	0.32%	0.055%
24	10.586	1271	1275	1280	rBV7	5326	11061	0.22%	0.038%
25	10.810	1306	1313	1320	rBV	1603972	2627843	53.02%	9.126%
26	10.945	1329	1336	1340	rBV9	7668	15353	0.31%	0.053%
27	11.075	1355	1358	1364	rVB8	5787	8804	0.18%	0.031%
28	11.169	1370	1374	1377	rVB5	3713	5426	0.11%	0.019%
29	11.286	1389	1394	1400	rBV8	6048	12374	0.25%	0.043%
30	12.063	1520	1526	1527	rBV5	4314	6311	0.13%	0.022%
31	12.227	1551	1554	1557	rVB5	3416	5215	0.11%	0.018%
32	12.463	1591	1594	1601	rVB7	7428	13990	0.28%	0.049%
33	12.686	1628	1632	1636	rVB6	6549	9258	0.19%	0.032%
34	13.363	1742	1747	1749	rBV5	5462	6396	0.13%	0.022%
35	13.439	1753	1760	1761	rBV6	6050	10052	0.20%	0.035%
36	13.674	1795	1800	1801	rBV4	5165	7784	0.16%	0.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
 Data File : BM036734.D
 Acq On : 25 Sep 2022 03:46
 Operator : CG/JU
 Sample : N4693-08
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A0AZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
 Title : SVOA CALIBRATION

37	13.957	1841	1848	1851	rBV8	7202	13800	0.28%	0.048%
38	14.051	1860	1864	1868	rBV4	10684	15630	0.32%	0.054%
39	14.351	1909	1915	1920	rBV3	12159	22049	0.44%	0.077%
40	14.533	1941	1946	1949	rBV6	3232	6060	0.12%	0.021%
41	14.627	1954	1962	1969	rBV	2556293	3634417	73.32%	12.622%
42	14.939	2012	2015	2019	rBV4	10710	14205	0.29%	0.049%
43	15.021	2025	2029	2033	rVB4	13699	16177	0.33%	0.056%
44	15.104	2040	2043	2046	rVB5	5492	6484	0.13%	0.023%
45	15.245	2064	2067	2070	rVB5	5663	6979	0.14%	0.024%
46	15.410	2093	2095	2099	rVB4	7329	8963	0.18%	0.031%
47	15.474	2102	2106	2108	rVB4	5545	7251	0.15%	0.025%
48	15.604	2122	2128	2134	rBV7	10201	18021	0.36%	0.063%
49	15.663	2134	2138	2144	rBV3	17075	28010	0.57%	0.097%
50	15.833	2163	2167	2170	rBV6	4938	8536	0.17%	0.030%
51	15.874	2170	2174	2178	rVV7	8443	12564	0.25%	0.044%
52	15.962	2185	2189	2197	rVB7	10287	17365	0.35%	0.060%
53	16.104	2210	2213	2219	rVB6	6950	12959	0.26%	0.045%
54	16.174	2221	2225	2226	rBV4	5502	5598	0.11%	0.019%
55	16.327	2249	2251	2253	rBV3	9641	10887	0.22%	0.038%
56	16.480	2273	2277	2278	rBV4	4069	5768	0.12%	0.020%
57	16.668	2305	2309	2314	rBV6	13543	21386	0.43%	0.074%
58	16.815	2331	2334	2336	rBV4	5388	6824	0.14%	0.024%
59	16.845	2337	2339	2343	rVB2	9015	9277	0.19%	0.032%
60	16.898	2346	2348	2352	rVV4	8947	9629	0.19%	0.033%
61	16.945	2352	2356	2359	rVV5	5717	9130	0.18%	0.032%
62	17.098	2378	2382	2383	rBV4	6879	9338	0.19%	0.032%
63	17.180	2393	2396	2400	rVB3	10835	14999	0.30%	0.052%
64	17.362	2421	2427	2432	rBV	3119559	4337047	87.50%	15.062%
65	17.404	2432	2434	2440	rVB	289815	355850	7.18%	1.236%
66	17.880	2513	2515	2519	rVB4	10306	11179	0.23%	0.039%
67	18.033	2538	2541	2545	rVB5	18320	21398	0.43%	0.074%
68	18.239	2572	2576	2581	rBV3	52068	103845	2.10%	0.361%
69	18.286	2581	2584	2590	rVB	64550	89019	1.80%	0.309%
70	18.433	2604	2609	2613	rBV2	71045	125759	2.54%	0.437%
71	18.468	2613	2615	2622	rVB2	35762	53470	1.08%	0.186%
72	18.739	2657	2661	2666	rVB2	35151	50978	1.03%	0.177%
73	19.151	2727	2731	2735	rBV	40689	66145	1.33%	0.230%
74	19.274	2749	2752	2758	rBV7	32896	43188	0.87%	0.150%
75	19.409	2770	2775	2781	rBV	550773	775307	15.64%	2.693%
76	19.550	2797	2799	2803	rVB3	51201	62521	1.26%	0.217%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036734.D
Acq On : 25 Sep 2022 03:46
Operator : CG/JU
Sample : N4693-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AZ3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Title : SVOA CALIBRATION

77	19.745	2828	2832	2833	rBV2	69705	93496	1.89%	0.325%
78	19.774	2833	2837	2843	rVB	301193	423412	8.54%	1.470%
79	20.262	2916	2920	2926	rVB3	181381	250308	5.05%	0.869%
80	20.533	2963	2966	2970	rBV3	144920	165631	3.34%	0.575%
81	20.739	2998	3001	3005	rBV	102871	105882	2.14%	0.368%
82	21.527	3130	3135	3140	rBV	2912236	4066172	82.04%	14.121%
83	23.962	3543	3549	3561	rVB2	1501863	3113874	62.82%	10.814%




Sum of corrected areas: 28794776

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036734.D
Acq On : 25 Sep 2022 03:46
Operator : CG/JU
Sample : N4693-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

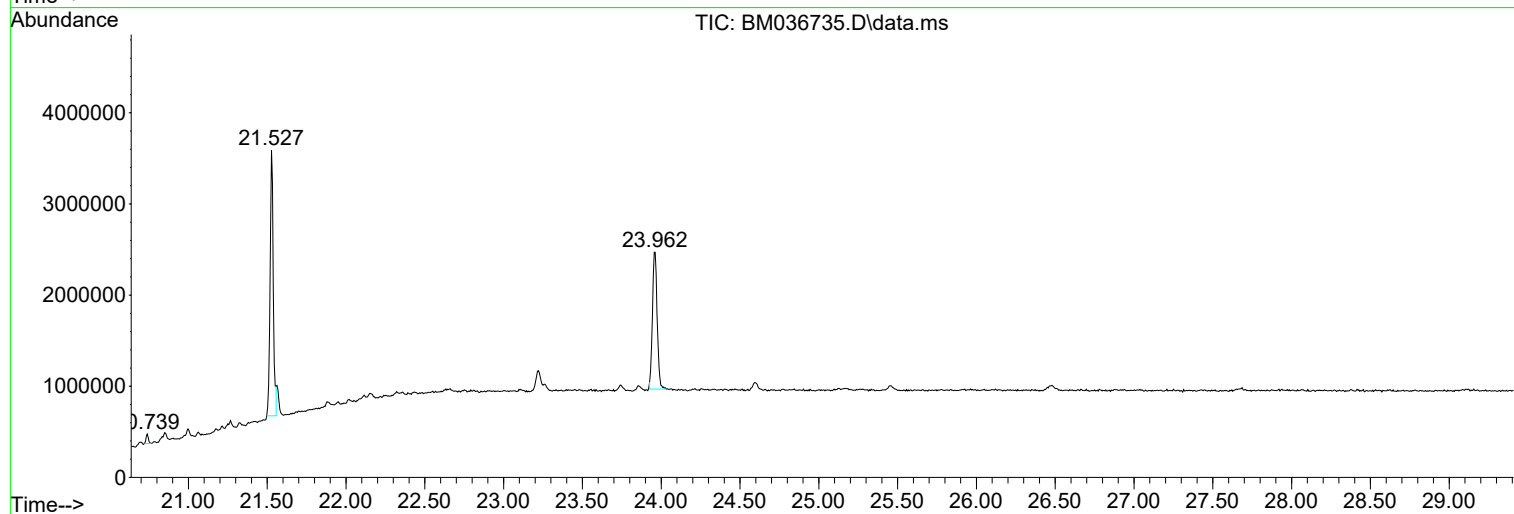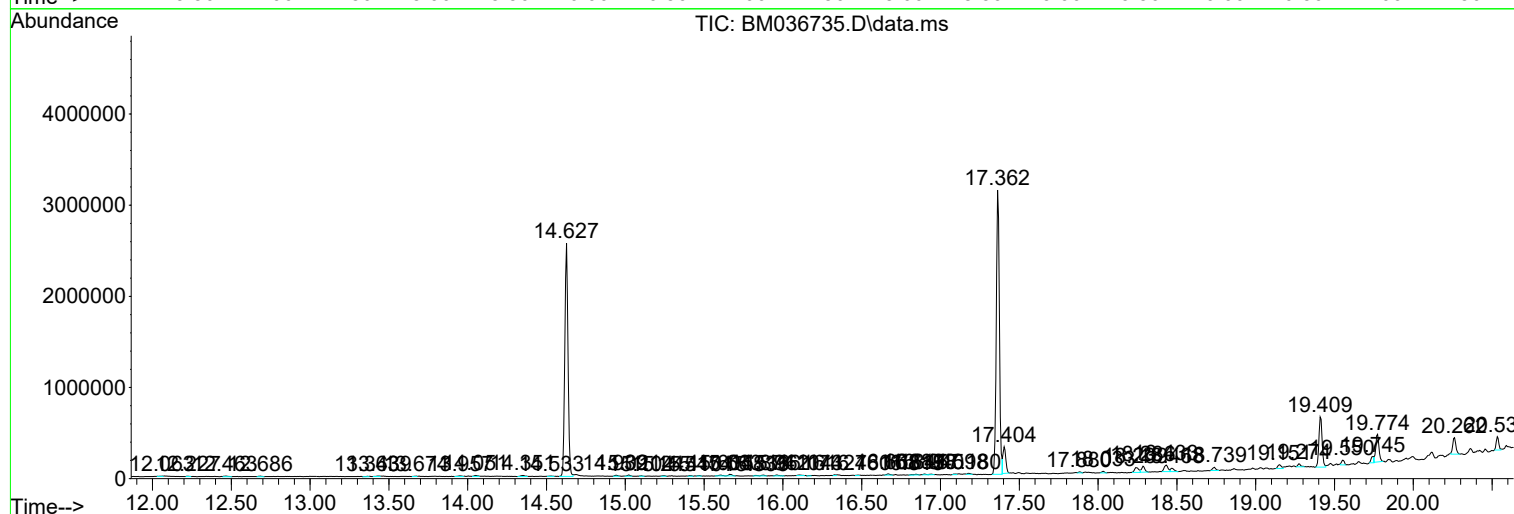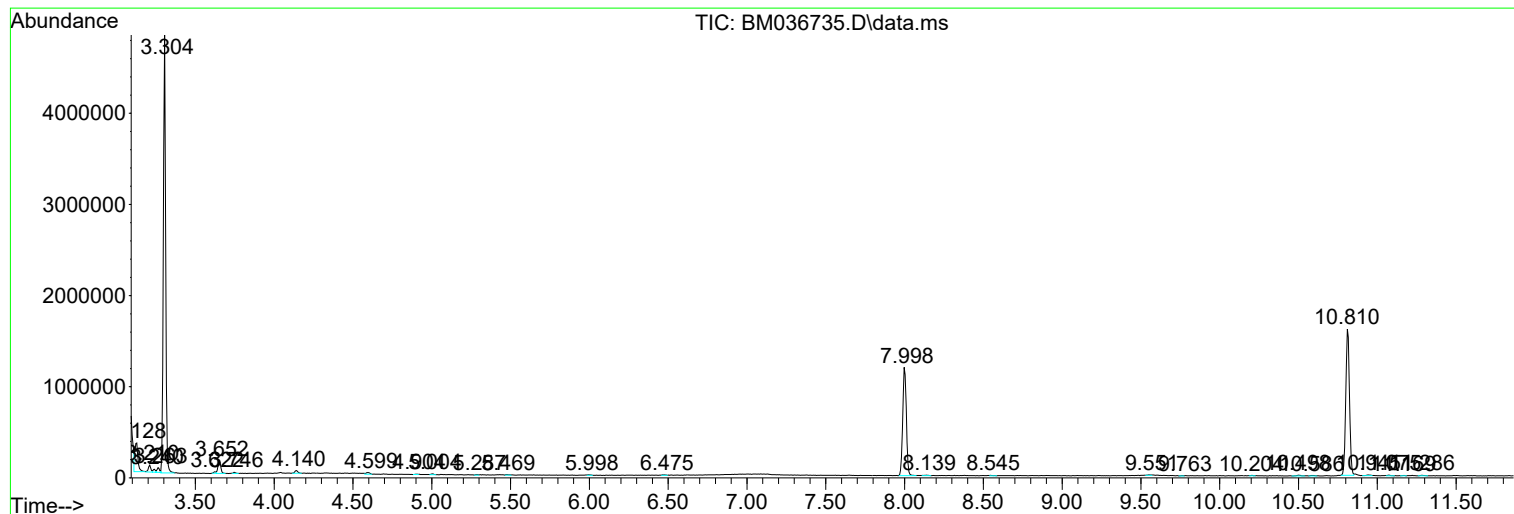

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036734.D
Acq On : 25 Sep 2022 03:46
Operator : CG/JU
Sample : N4693-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.128	4.48 ng/ul	420063	1,4-Dichlorobenzene-d4	7.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexene, 3,3,5-trimethyl-		126	C9H18		013427-43-5	40
2	4-Octene, 2,6-dimethyl-, [S-(Z)]-		140	C10H20		062960-77-4	40
3	3-Decene, 2,2-dimethyl-, (E)-		168	C12H24		055499-02-0	39
4	1-Hexene, 3-methyl-		98	C7H14		003404-61-3	38
5	1-Pentene, 3,3-dimethyl-		98	C7H14		003404-73-7	35

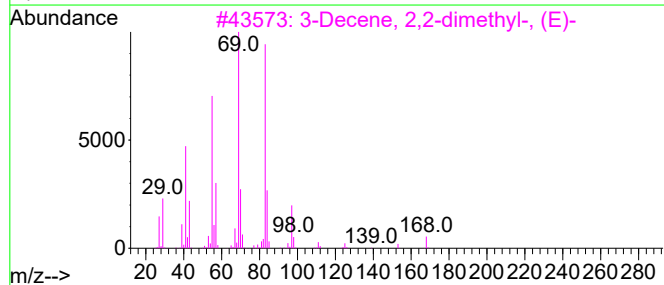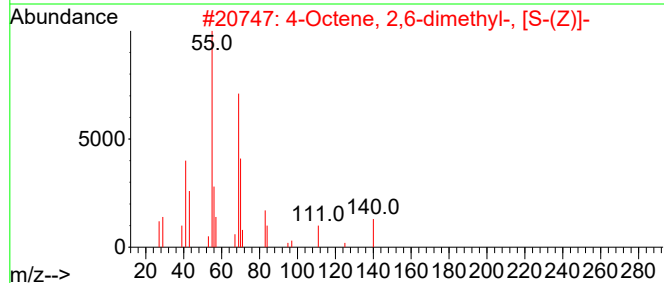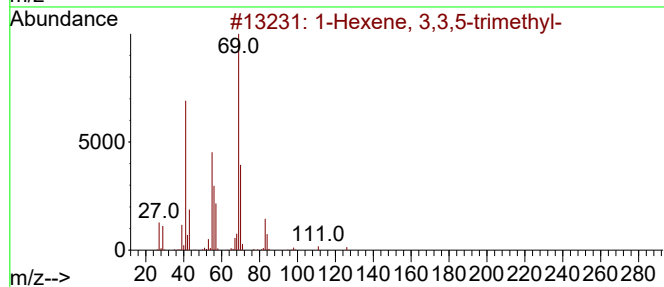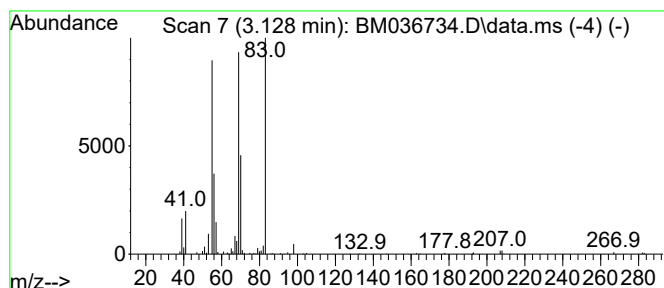

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036734.D
Acq On : 25 Sep 2022 03:46
Operator : CG/JU
Sample : N4693-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AZ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.304	52.83 ng/ul	4956590	1,4-Dichlorobenzene-d4	7.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	91
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	91
4			Heptane	100	C7H16	000142-82-5	91
5			Hexane, 3-methyl-	100	C7H16	000589-34-4	40

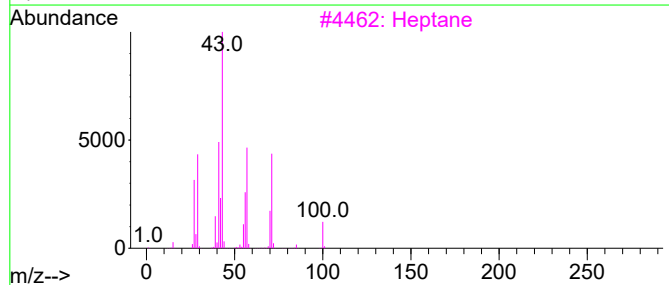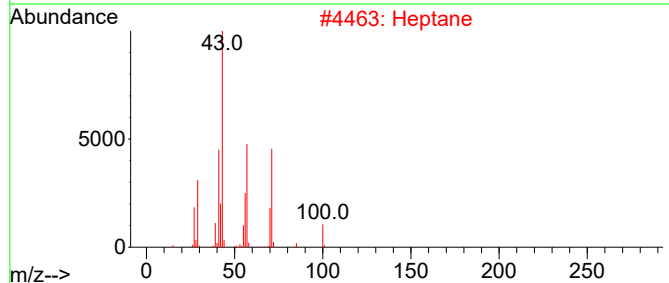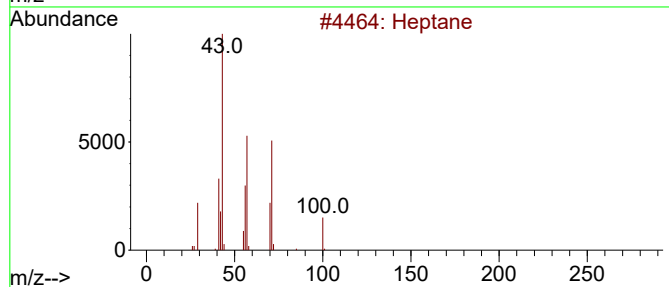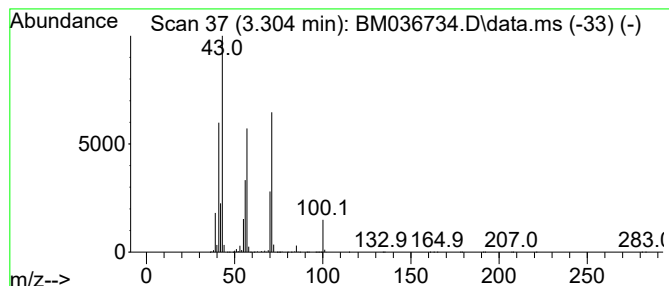

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM092322\
Data File : BM036734.D
Acq On : 25 Sep 2022 03:46
Operator : CG/JU
Sample : N4693-08
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A0AZ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM091522.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.128	4.5	ng/ul	420063	1	7.998	1876300	20.0
(DEL) Alkane: S...	3.304	52.8	ng/ul	4956590	1	7.998	1876300	20.0