


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM092415\
Data File : BM002707.D
Acq On : 24 Sep 2015 11:13
Operator : UM/IZ
Sample : DFTPP15
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP15

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM092415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 25 18:41:20 2015

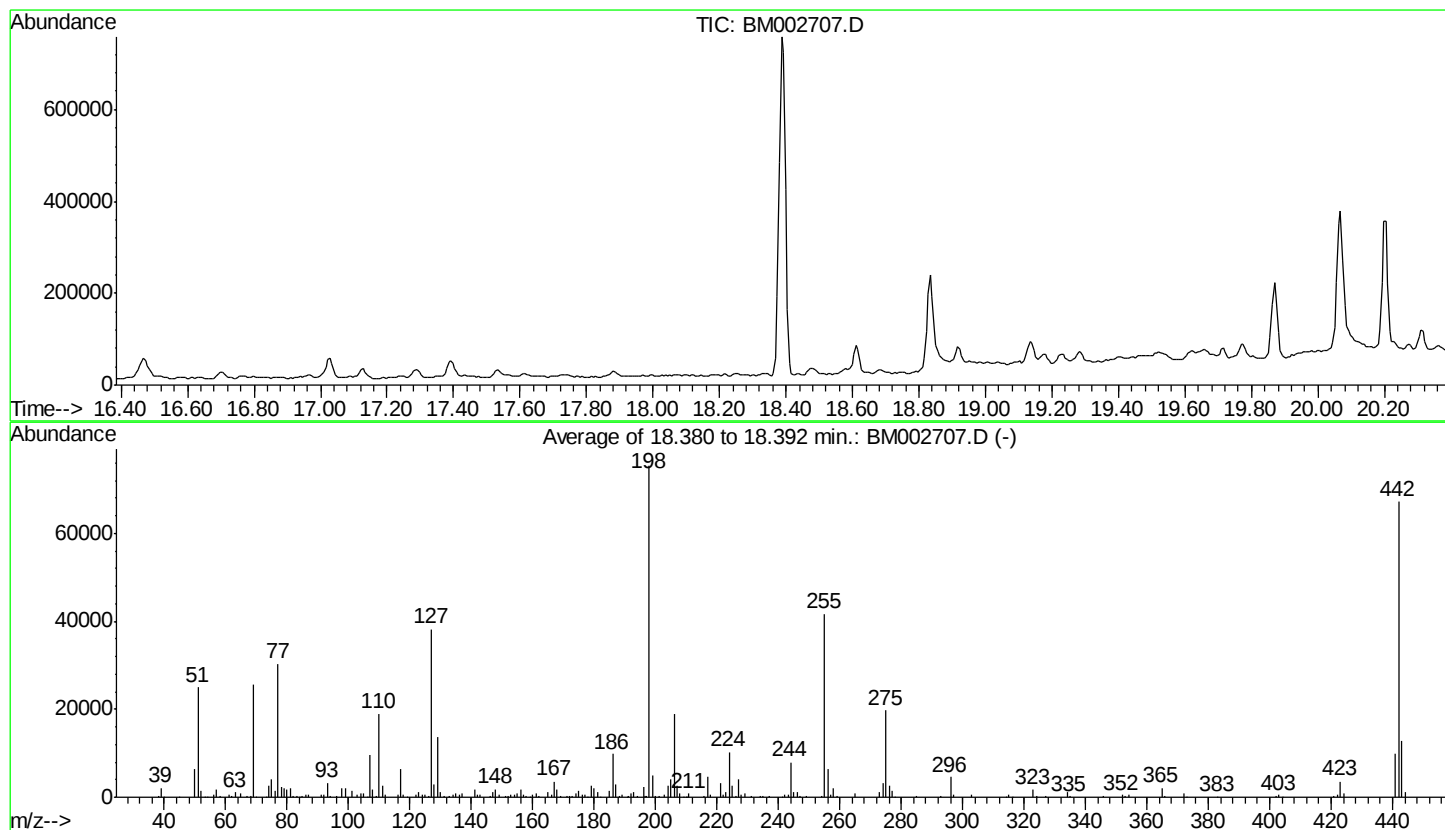

AutoFind: Scans 2600, 2601, 2602; Background Corrected with Scan 2594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	24997	PASS
68	69	0.00	2	1.4	366	PASS
69	198	0.00	100	34.1	25684	PASS
70	69	0.00	2	0.5	118	PASS
127	198	10	80	50.7	38189	PASS
197	198	0.00	1	0.4	299	PASS
198	198	100	100	100.0	75352	PASS
199	198	5	9	6.7	5056	PASS
275	198	10	60	26.1	19668	PASS
365	198	1	100	2.9	2157	PASS
441	443	0.01	100	76.9	9921	PASS
442	198	50	100	89.1	67125	PASS
443	442	15	24	19.2	12899	PASS

m/z	Abundance
38.00	373.0
39.00	2462.0
40.00	628.0
41.00	1546.0
42.00	618.0
43.00	2591.0
44.00	2516.0
45.00	870.0
50.00	5623.0
51.10	21944.0
52.00	1320.0
53.00	443.0
54.00	319.0
55.00	1441.0
56.00	1147.0
57.00	2690.0
58.00	310.0
60.00	1162.0
61.00	550.0
62.00	382.0
63.00	940.0
65.00	647.0
67.00	412.0
68.00	685.0
69.00	22280.0
70.00	411.0
71.10	578.0
73.00	1317.0
74.00	2354.0
75.00	3746.0
76.00	1093.0
77.00	24728.0
78.00	1913.0
79.00	1871.0
80.00	1461.0
81.00	2157.0
81.90	708.0
83.10	860.0
84.00	443.0
85.00	773.0
85.90	649.0
87.00	478.0
91.00	779.0
91.90	544.0
93.00	2622.0
95.00	403.0
96.00	377.0
97.00	524.0
98.00	2226.0
99.00	1759.0
101.00	1229.0
103.00	445.0
103.90	815.0
105.00	781.0
107.00	8012.0
108.00	1408.0
109.00	391.0
110.00	15272.0
111.00	2233.0
111.90	324.0
115.00	352.0
116.00	523.0
117.00	5500.0
118.00	470.0
121.90	529.0
122.90	859.0
123.90	470.0
125.00	494.0
126.10	347.0
127.00	30440.0
128.00	2389.0
129.00	11336.0
130.00	1017.0
131.10	421.0
133.90	380.0
135.00	897.0
136.00	456.0
137.00	743.0
141.00	1358.0
142.00	585.0
143.00	510.0
146.00	406.0
147.00	788.0
148.00	1464.0
149.00	390.0
151.00	315.0
153.00	520.0
154.00	323.0
155.00	866.0
156.00	1298.0
157.00	554.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

160.00	512.0
161.00	658.0
165.00	871.0
166.00	541.0
167.00	2715.0
167.90	1417.0
172.90	316.0
174.00	577.0
175.00	1153.0
176.00	424.0
176.90	631.0
179.00	1819.0
180.00	1539.0
181.00	808.0
185.00	1163.0
186.00	7296.0
187.00	2010.0
188.00	313.0
189.00	514.0
190.90	314.0
191.90	665.0
193.00	724.0
196.00	1699.0
197.00	325.0
198.00	56600.0
199.00	3773.0
203.00	419.0
204.00	1955.0
205.00	2953.0
206.00	13706.0
207.00	2352.0
207.90	697.0
210.90	530.0
217.00	3286.0
217.90	398.0
221.00	2365.0
223.00	768.0
224.00	7185.0
225.00	1849.0
227.00	2628.0
227.90	429.0
228.90	604.0
231.00	346.0
242.00	388.0
243.00	386.0
244.10	5799.0
245.00	848.0
246.00	943.0
254.10	309.0
255.00	28752.0
256.00	4424.0
256.90	388.0
257.90	1352.0
259.00	310.0
264.90	609.0
272.90	780.0
274.00	2402.0
275.00	13198.0
276.00	1989.0
277.00	1012.0
296.00	3079.0
297.00	422.0
303.10	366.0
314.90	412.0
323.00	984.0
334.00	761.0
351.90	361.0
354.00	329.0
365.00	1269.0
372.00	563.0
403.00	321.0
423.00	2067.0
424.00	500.0
441.00	5799.0
442.00	37496.0
443.00	7665.0
444.00	695.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

m/z	Abundance
38.00	524.0
39.00	2812.0
40.00	610.0
41.10	1461.0
42.00	662.0
43.00	2462.0
44.00	2442.0
45.00	820.0
50.00	7175.0
51.00	28696.0
52.10	1732.0
53.00	436.0
55.10	1538.0
56.00	1326.0
57.00	3131.0
58.00	381.0
60.00	1141.0
61.00	539.0
62.00	500.0
63.00	1363.0
65.00	796.0
67.00	409.0
68.00	814.0
69.00	31392.0
70.00	534.0
71.00	626.0
73.00	1304.0
74.00	3032.0
75.00	4902.0
76.00	1729.0
77.00	35856.0
78.10	2814.0
79.00	2486.0
80.00	1820.0
81.00	2607.0
82.00	907.0
83.00	1005.0
83.90	453.0
85.00	1028.0
86.00	812.0
87.00	481.0
91.00	955.0
92.00	781.0
93.00	3719.0
93.90	353.0
95.00	391.0
95.90	439.0
97.00	543.0
98.00	3034.0
99.00	2549.0
101.00	1671.0
103.00	648.0
104.00	1064.0
104.90	1068.0
106.00	339.0
107.00	11347.0
108.00	1862.0
109.00	338.0
110.00	21928.0
111.00	3322.0
112.00	553.0
115.00	333.0
115.90	699.0
117.00	7500.0
118.00	652.0
118.90	301.0
122.00	860.0
123.00	1285.0
123.90	616.0
124.90	565.0
125.90	432.0
127.00	45032.0
128.00	3238.0
129.00	16336.0
130.00	1403.0
130.90	441.0
133.00	314.0
134.00	544.0
135.00	1604.0
136.00	780.0
137.00	1078.0
141.00	2196.0
141.90	713.0
143.00	568.0
146.00	515.0
147.00	1408.0
148.00	2099.0
149.00	617.0
151.00	398.0
152.00	374.0
153.00	682.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

153.90	591.0
155.00	1009.0
156.00	1921.0
157.00	456.0
158.00	403.0
159.00	357.0
160.00	608.0
161.10	969.0
162.00	401.0
165.00	1284.0
166.00	729.0
167.00	4070.0
168.00	2001.0
168.90	418.0
171.00	318.0
171.90	381.0
173.00	483.0
174.00	899.0
175.00	1700.0
176.10	501.0
177.00	782.0
178.00	325.0
179.00	3090.0
180.00	2194.0
181.00	1090.0
182.00	355.0
185.00	1525.0
186.00	11189.0
187.00	3486.0
188.10	312.0
189.00	816.0
191.10	365.0
191.90	1076.0
193.00	1266.0
193.90	346.0
196.00	2727.0
197.00	572.0
198.00	87080.0
198.90	5852.0
199.90	500.0
201.40	465.0
203.00	600.0
204.00	3014.0
205.00	4855.0
206.00	21944.0
207.00	3413.0
208.00	985.0
210.00	356.0
211.00	921.0
216.00	434.0
217.00	5259.0
217.90	766.0
221.10	3874.0
221.80	786.0
223.00	1262.0
224.00	12081.0
225.00	3078.0
226.00	383.0
227.00	4559.0
228.00	580.0
229.00	1023.0
231.10	484.0
233.90	310.0
234.90	400.0
236.90	387.0
242.10	685.0
243.00	521.0
244.10	8948.0
245.00	1201.0
246.00	1550.0
246.90	368.0
248.90	406.0
254.10	340.0
255.00	47616.0
256.00	7208.0
257.00	656.0
258.00	2424.0
259.00	454.0
265.00	1016.0
273.00	1368.0
274.00	4054.0
275.00	22960.0
276.00	3086.0
276.90	1736.0
285.10	315.0
292.90	354.0
296.00	5138.0
296.90	821.0
303.00	699.0
314.00	308.0
314.90	623.0
323.00	2082.0
324.00	449.0
326.90	346.0
334.10	1181.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

334.90	356.0
346.00	310.0
352.00	561.0
353.00	391.0
354.00	646.0
365.00	2541.0
365.90	348.0
372.00	1171.0
402.00	486.0
402.90	601.0
404.00	322.0
420.90	573.0
422.00	633.0
423.00	3992.0
424.00	909.0
441.00	11421.0
442.00	75536.0
443.00	14521.0
444.00	1240.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

m/z	Abundance
38.00	347.0
39.00	2472.0
39.90	583.0
41.00	1499.0
42.00	642.0
43.10	2505.0
44.00	2480.0
45.00	744.0
50.00	6151.0
51.00	24352.0
52.00	1435.0
53.10	419.0
55.10	1608.0
56.00	1114.0
57.00	2862.0
60.00	1183.0
61.00	566.0
62.00	371.0
63.00	1062.0
65.00	804.0
67.10	364.0
68.00	641.0
69.00	26288.0
70.00	519.0
71.10	614.0
73.00	1352.0
74.10	2602.0
75.00	3962.0
76.10	1320.0
77.10	30408.0
78.00	2066.0
79.00	1929.0
80.00	1646.0
81.00	2591.0
82.00	744.0
83.00	1005.0
84.10	381.0
85.00	831.0
86.00	722.0
86.90	545.0
90.90	844.0
92.00	655.0
93.00	3417.0
94.00	419.0
96.00	397.0
97.00	466.0
98.00	2605.0
99.00	1937.0
101.00	1434.0
102.90	639.0
103.90	810.0
104.90	886.0
107.00	9336.0
108.00	1722.0
109.00	505.0
110.00	19840.0
111.00	3123.0
112.00	509.0
116.00	652.0
117.00	6420.0
118.00	546.0
122.00	740.0
122.90	1316.0
124.00	538.0
125.00	564.0
126.10	324.0
127.00	39096.0
128.00	3011.0
129.00	14658.0
130.00	1283.0
131.00	339.0
133.00	347.0
134.00	522.0
135.00	1276.0
135.90	474.0
137.00	871.0
141.00	1779.0
142.00	583.0
142.90	455.0
146.90	1000.0
148.00	1939.0
148.90	632.0
151.00	396.0
152.10	314.0
152.90	652.0
154.00	470.0
154.90	1061.0
156.00	1809.0
157.10	538.0
158.00	323.0
159.90	647.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

161.00	966.0
162.00	381.0
165.00	1184.0
165.90	587.0
167.00	4015.0
168.00	1815.0
169.00	383.0
170.90	305.0
171.90	329.0
173.00	441.0
174.00	1013.0
175.00	1566.0
176.00	516.0
176.90	765.0
178.90	2730.0
180.00	2205.0
181.00	1258.0
185.00	1512.0
186.00	10795.0
187.00	3099.0
188.00	331.0
189.00	706.0
191.10	458.0
192.00	959.0
192.90	1268.0
194.00	320.0
196.00	2478.0
196.70	488.0
198.00	82376.0
199.00	5543.0
200.00	511.0
201.30	423.0
203.00	512.0
204.00	2859.0
205.00	4591.0
206.00	21000.0
207.00	3381.0
208.10	995.0
209.00	328.0
210.20	461.0
210.90	862.0
215.90	362.0
217.00	5292.0
217.90	737.0
221.00	3604.0
221.80	887.0
223.00	1167.0
224.00	11690.0
225.00	3083.0
226.10	320.0
227.00	4822.0
227.90	611.0
228.90	1002.0
231.00	373.0
234.00	368.0
235.00	313.0
237.00	426.0
241.10	369.0
242.00	647.0
243.10	649.0
244.00	9136.0
245.00	1256.0
246.00	1400.0
247.00	384.0
249.00	343.0
254.10	331.0
255.00	48816.0
256.00	7219.0
257.00	500.0
257.90	2325.0
258.90	371.0
265.00	962.0
273.00	1525.0
274.00	3506.0
275.00	22848.0
276.00	2965.0
277.00	1729.0
278.00	331.0
284.90	313.0
292.90	395.0
296.00	5445.0
297.00	822.0
303.00	759.0
315.00	565.0
316.00	342.0
323.00	1946.0
324.00	315.0
326.90	392.0
334.00	1296.0
335.00	362.0
345.90	421.0
352.00	704.0
352.90	467.0
354.00	691.0
364.90	2662.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

365.90	497.0
372.00	1217.0
373.00	303.0
382.90	413.0
402.00	479.0
403.00	716.0
420.90	617.0
422.00	778.0
423.00	4716.0
424.00	1040.0
441.00	12545.0
442.00	88344.0
443.00	16512.0
444.00	1553.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15

m/z	Abundance
39.00	470.0
40.00	555.0
41.10	1521.0
42.00	687.0
43.10	2705.0
44.00	2528.0
45.00	769.0
53.00	327.0
55.00	1684.0
56.00	518.0
57.10	1192.0
60.00	1252.0
68.00	347.0
69.00	969.0
70.00	370.0
71.00	631.0
73.00	1185.0
81.00	427.0
82.00	395.0
83.10	742.0
84.00	402.0
85.00	564.0
91.00	380.0
95.00	355.0
97.00	643.0
98.00	458.0
111.00	322.0
115.00	325.0
129.10	455.0
135.00	304.0
207.00	557.0

Instrument :
BNA_M
ClientSampleId :
DFTPP15